

SUPERVISOR TEST




NEW HARTFORD TOWN
POLICE DEPT
DATAMASTER dmt: 127606

Date: 03/06/2020

OPERATOR NAME:
MICHAEL T KOWALSKI
Permit #: 31077
Operator Agency/Dept: NEW HARTFORD TOWN PD
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:51
INTERNAL STANDARD	VERIFIED	10:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	10:52
BLANK TEST	0.00	10:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	10:53
BLANK TEST	0.00	10:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	10:54
BLANK TEST	0.00	10:55

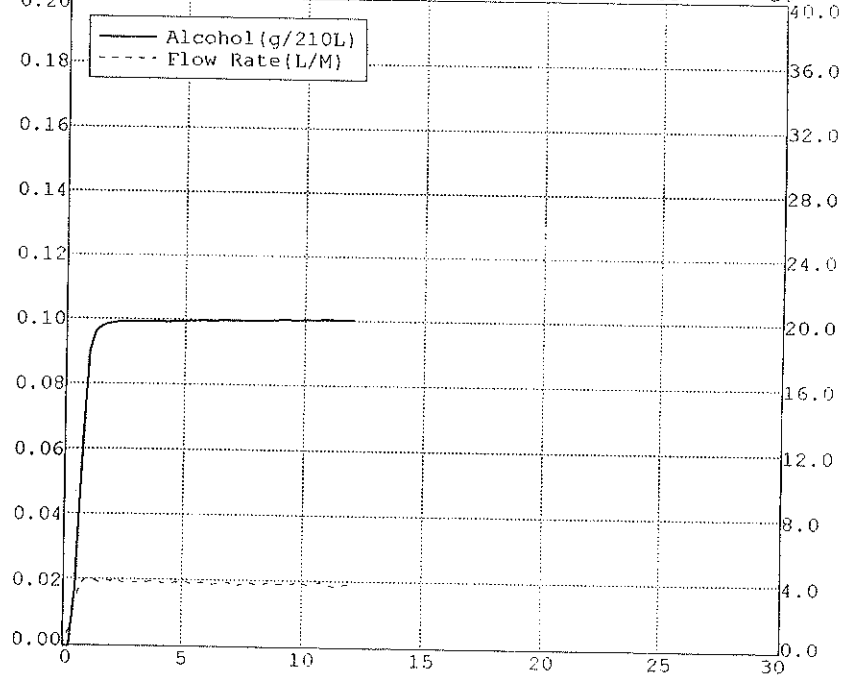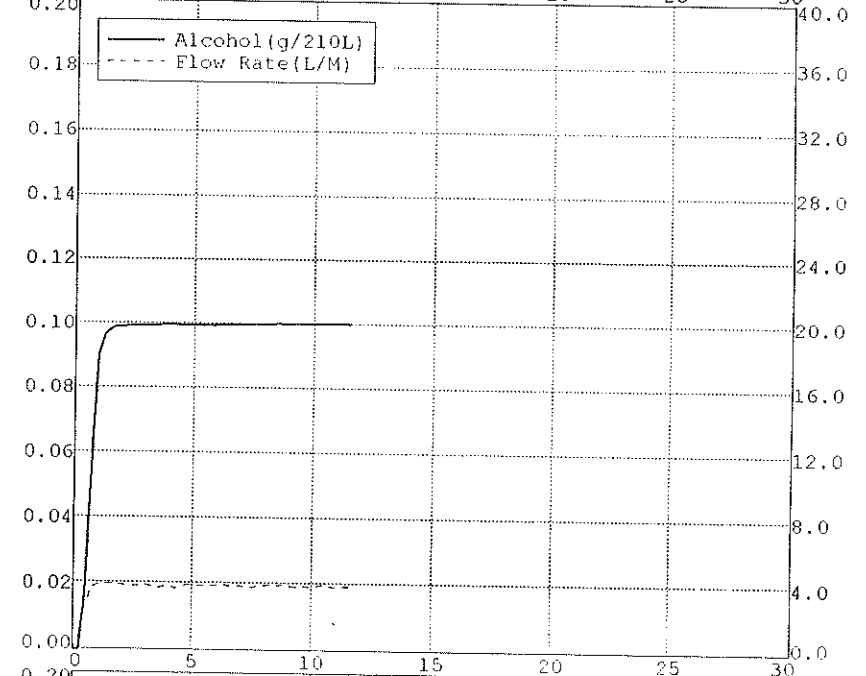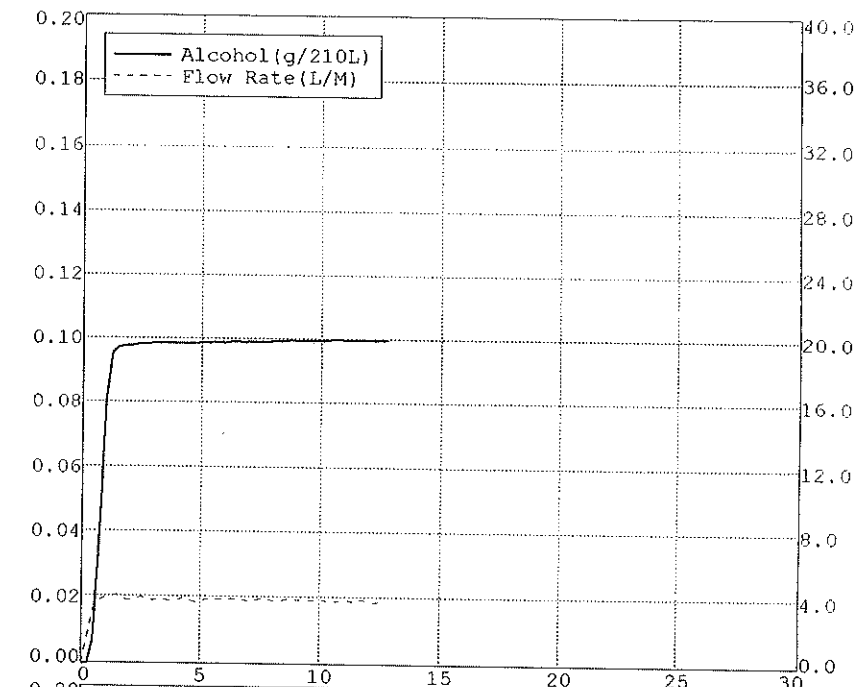

SUPERVISOR TEST




NEW HARTFORD TOWN
POLICE DEPT
DATAMASTER dmt: 127606

Date: 03/01/2020

OPERATOR NAME:
MICHAEL T KOWALSKI
Permit #: 31077
Operator Agency/Dept: NEW HARTFORD TOWN PD
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:08
INTERNAL STANDARD	VERIFIED	23:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	23:08
BLANK TEST	0.00	23:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	23:09
BLANK TEST	0.00	23:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	23:10
BLANK TEST	0.00	23:11

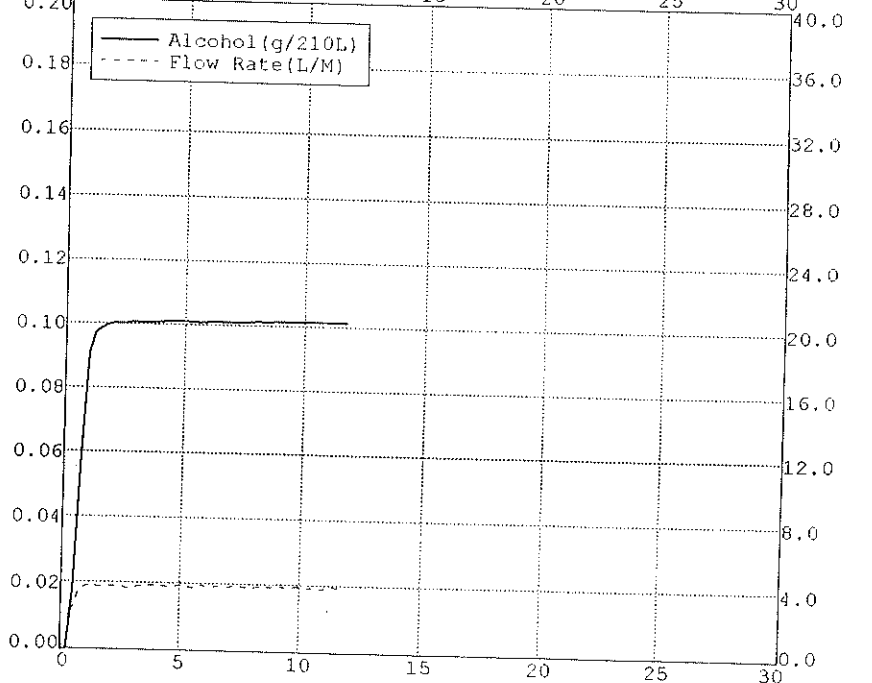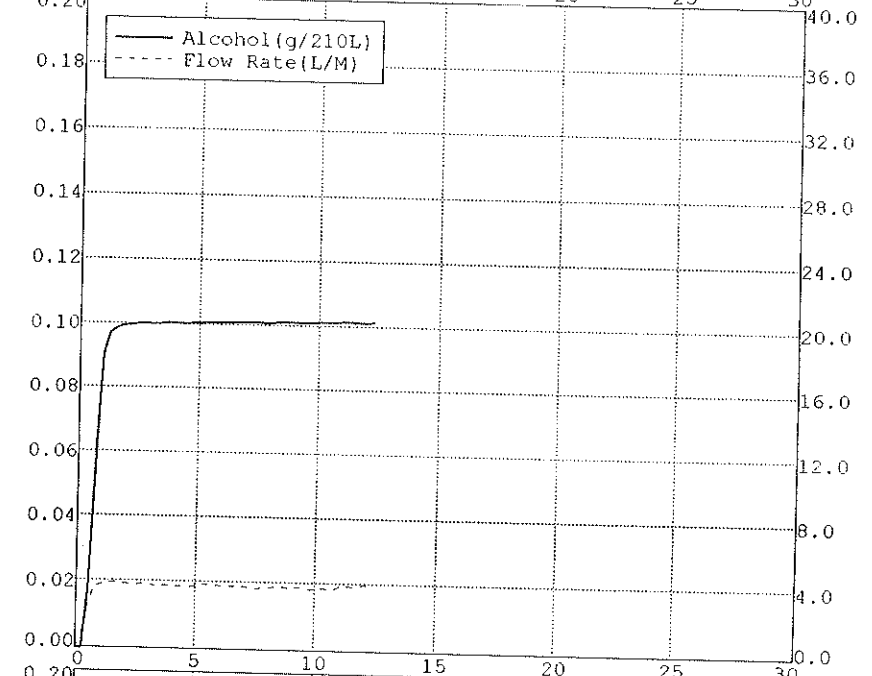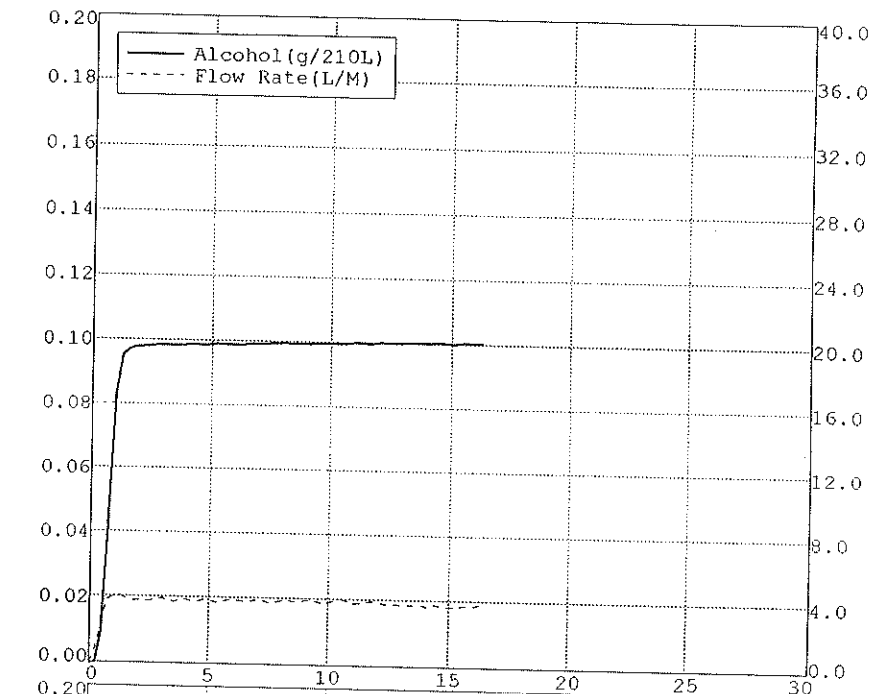

SUPERVISOR TEST

NEW HARTFORD TOWN
POLICE DEPT
DATAMASTER dmt: 127606

Date: 02/26/2020

OPERATOR NAME:
MICHAEL T KOWALSKI
Permit #: 31077
Operator Agency/Dept: NEW HARTFORD TOWN PD
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:36
INTERNAL STANDARD	VERIFIED	09:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:37
BLANK TEST	0.00	09:37
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:38
BLANK TEST	0.00	09:39
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:39
BLANK TEST	0.00	09:40

