

SUPERVISOR TEST




NEW HARTFORD TOWN
POLICE DEPT
DATAMASTER dmt: 127606

Date: 06/10/2020

OPERATOR NAME:
MICHAEL T KOWALSKI
Permit #: 31077
Operator Agency/Dept: NEW HARTFORD TOWN PD
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:31
INTERNAL STANDARD	VERIFIED	07:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:32
BLANK TEST	0.00	07:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:33
BLANK TEST	0.00	07:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:34
BLANK TEST	0.00	07:35

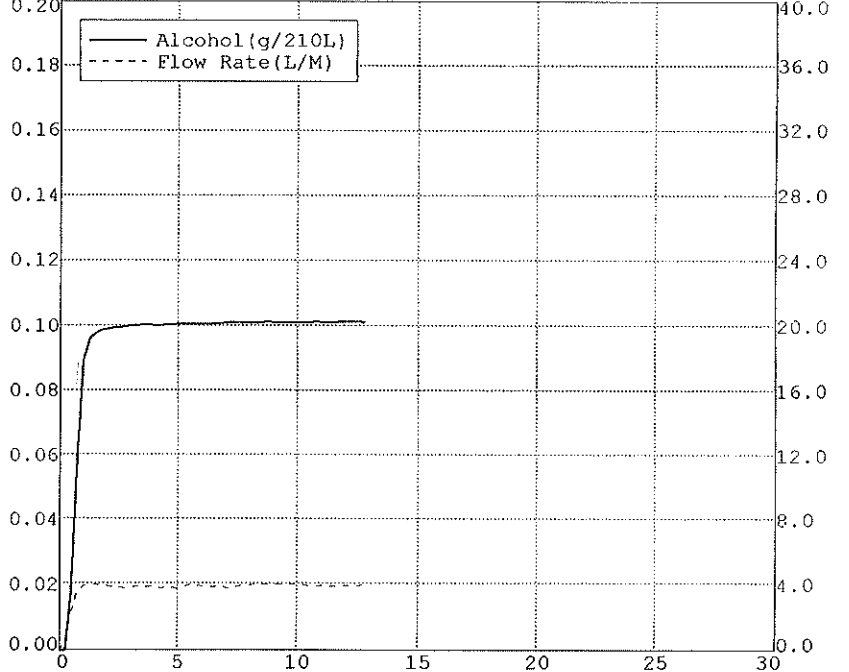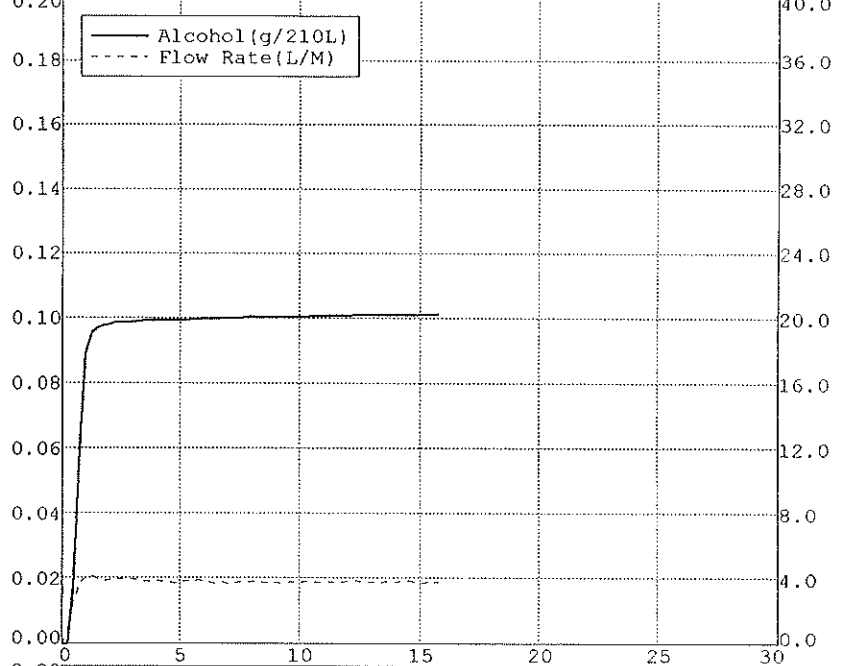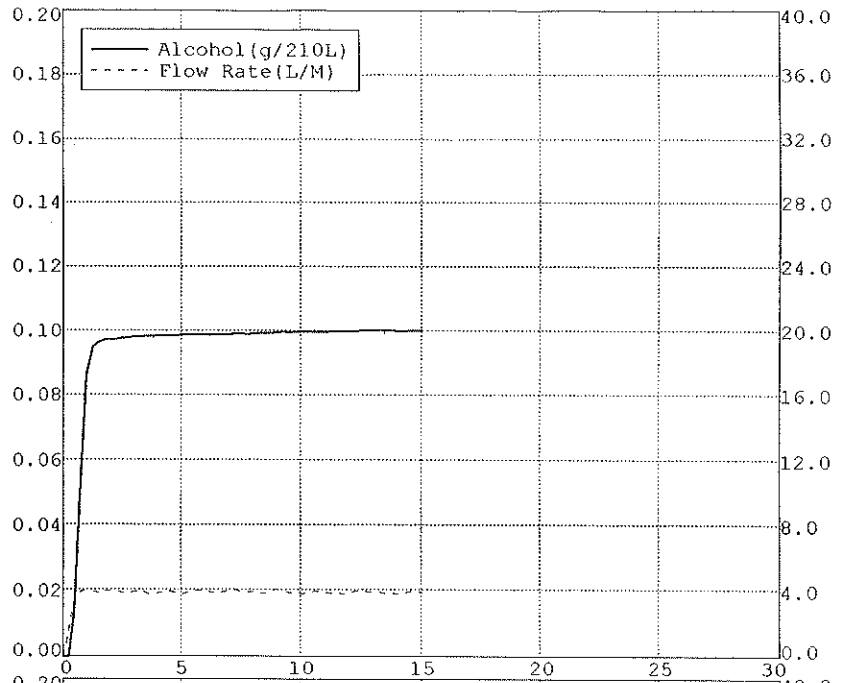

SUPERVISOR TEST




NEW HARTFORD TOWN
POLICE DEPT
DATAMASTER dmt: 127606

Date: 06/10/2020

OPERATOR NAME:
MICHAEL T KOWALSKI
Permit #: 31077
Operator Agency/Dept: NEW HARTFORD TOWN PD
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:49
INTERNAL STANDARD	VERIFIED	20:49
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	20:50
BLANK TEST	0.00	20:50
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	20:51
BLANK TEST	0.00	20:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	20:52
BLANK TEST	0.00	20:53

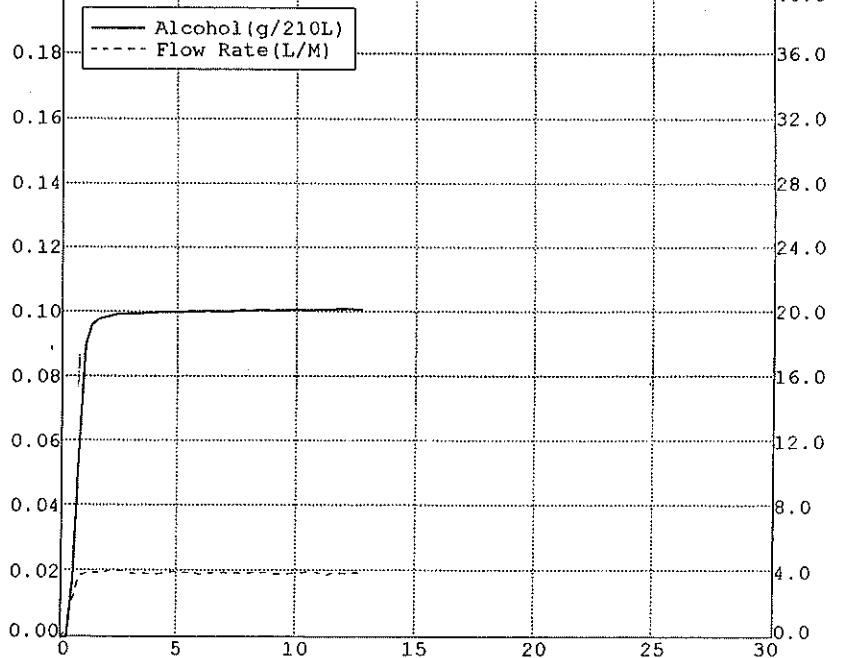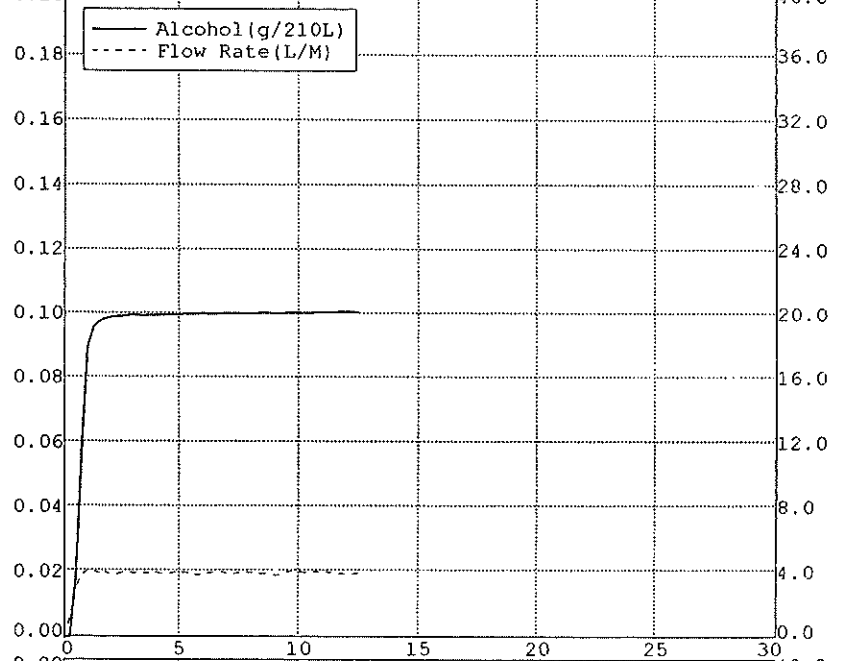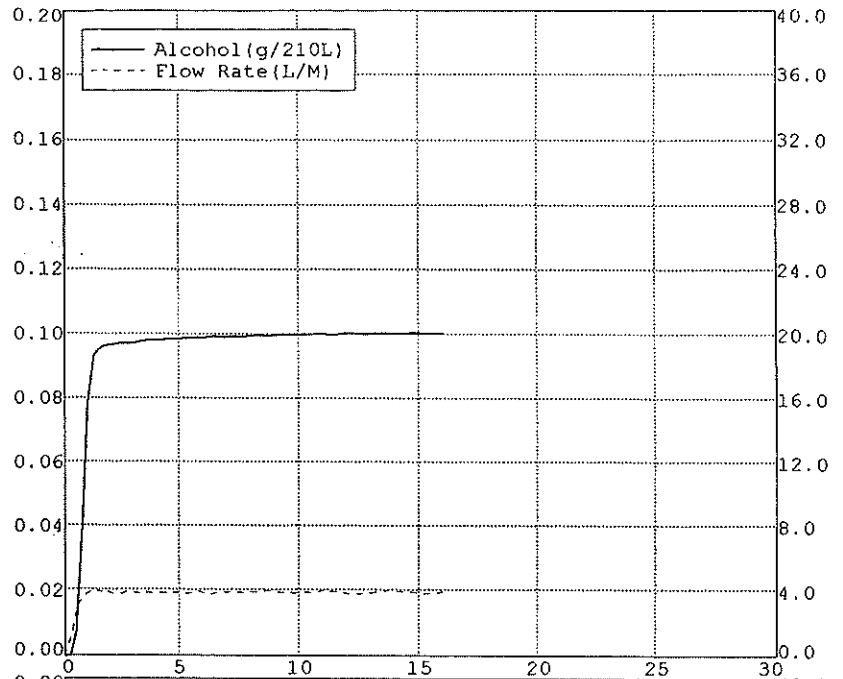

SUPERVISOR TEST




NEW HARTFORD TOWN
POLICE DEPT
DATAMASTER dmt: 127606

Date: 06/10/2020

OPERATOR NAME:
MICHAEL T KOWALSKI
Permit #: 31077
Operator Agency/Dept: NEW HARTFORD TOWN PD
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:05
INTERNAL STANDARD	VERIFIED	21:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:06
BLANK TEST	0.00	21:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:07
BLANK TEST	0.00	21:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:08
BLANK TEST	0.00	21:09

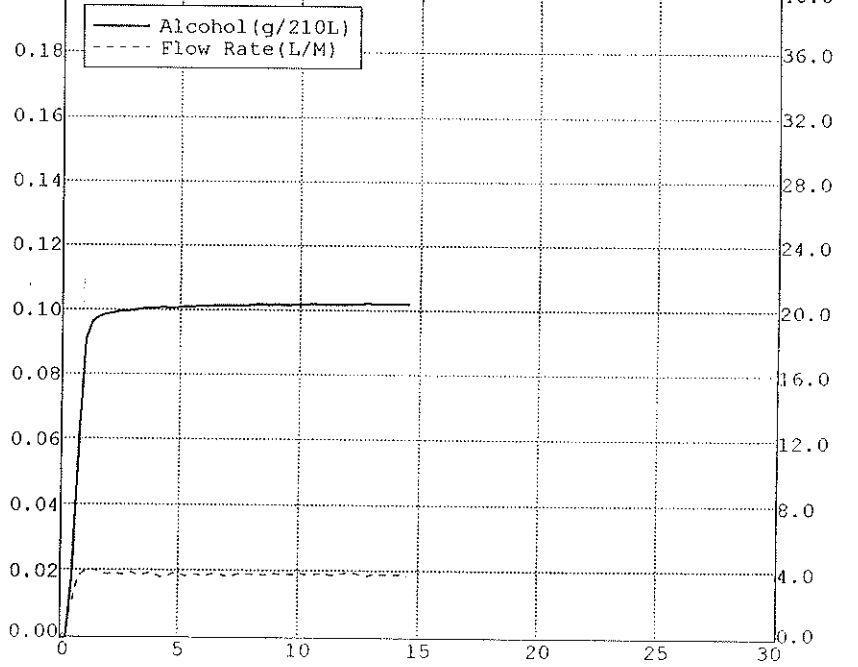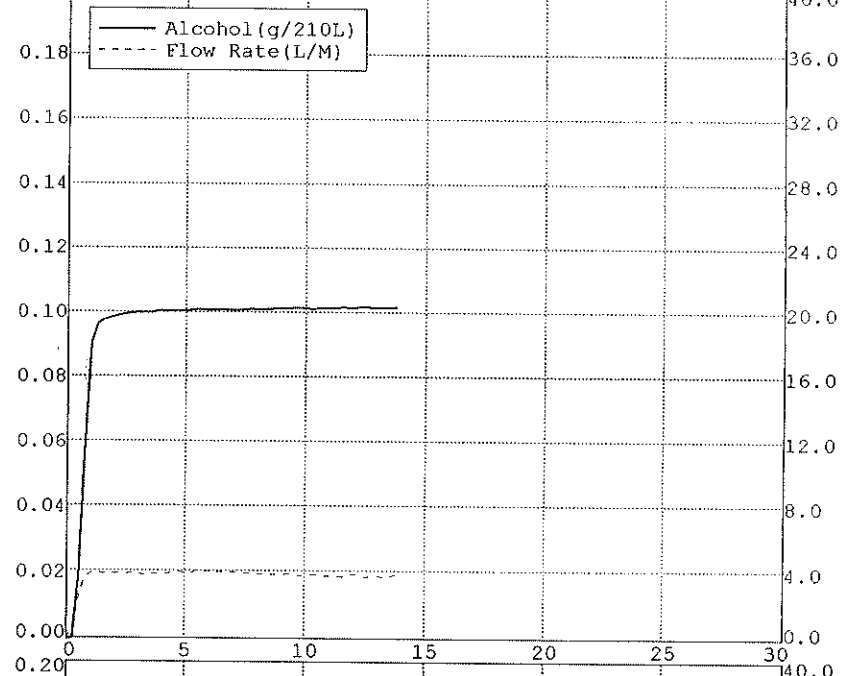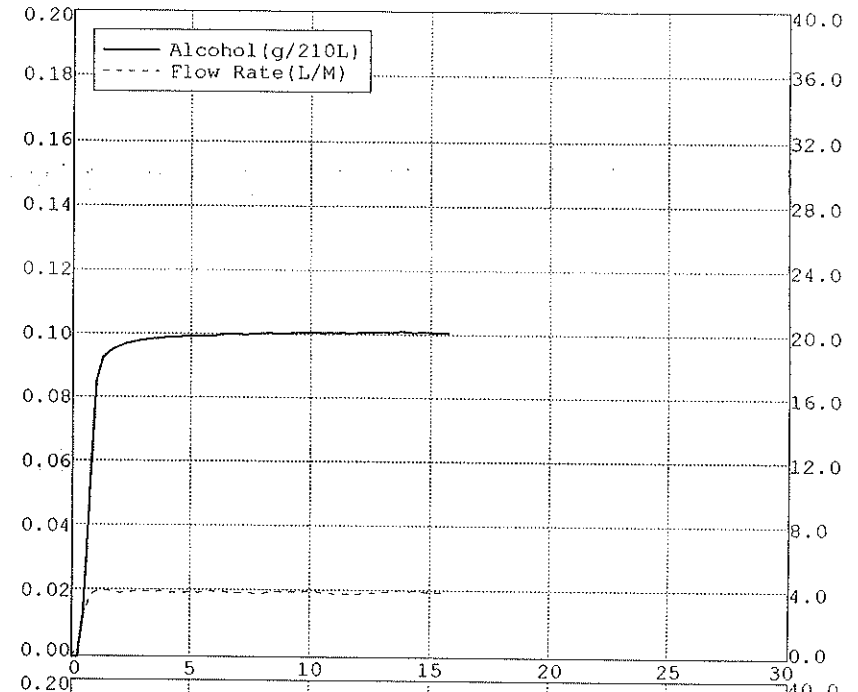

Supervisor Report

Control Test Record

Serial Number: 127606

Test Date: 06/10/2020 07:30:41

Location: 144

NEW HARTFORD POLICE DEPT.

Supervisor Information

First Name: Michael T

Last Name: Kowalski

Permit: 31077

Agency: NEW HARTFORD TOWN PD

Simulator Information


Lot: 20170 Nominal: 0.100

Test Results

Alcohol 1:	0.10	34.00
Alcohol 2:	0.10	34.00
Alcohol 3:	0.10	34.00

Solution Change:

Plot 1 of 3 <=>

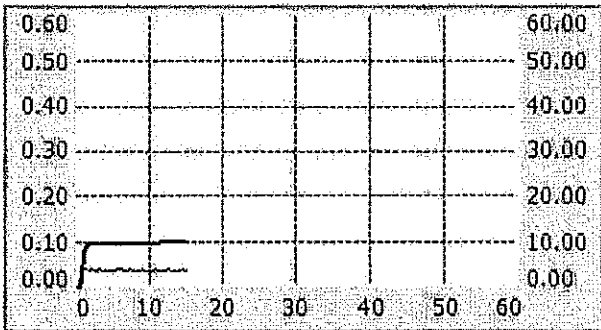

Status

Status Code: _____

Date Time: _____

Message: _____

Control Test Record

Serial Number: 127606
Test Date: 06/10/2020 20:48:42
Location: 144
NEW HARTFORD POLICE DEPT.

Simulator Information

Lot: 20170 Nominal: 0.100

Test Results


Alcohol 1: 0.10 34.00
Alcohol 2: 0.10 34.01
Alcohol 3: 0.10 34.01

Solution Change:

Supervisor Information

First Name: Michael T
Last Name: Kowalski
Pemit: 31077
Agency: NEW HARTFORD TOWN PD

Plot 1 of 3 =>

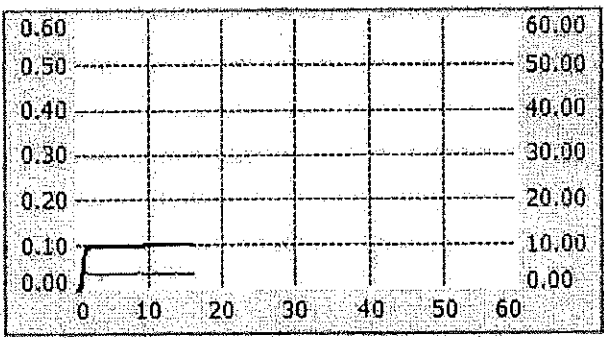

Status

Status Code:
Date Time:
Message:

Control Test Record

Serial Number: 127606
Test Date: 06/10/2020 21:04:40
Location: 144

NEW HARTFORD POLICE DEPT.

Supervisor Information

First Name: Michael T
Last Name: Kowalski
Permit: 31077
Agency: NEW HARTFORD TOWN PD

Simulator Information


Lot: 20170 Nominal: 0.100

Test Results

Alcohol 1:	0.10	34.01
Alcohol 2:	0.10	34.01
Alcohol 3:	0.10	34.01

Solution Change:

Plot 1 of 3

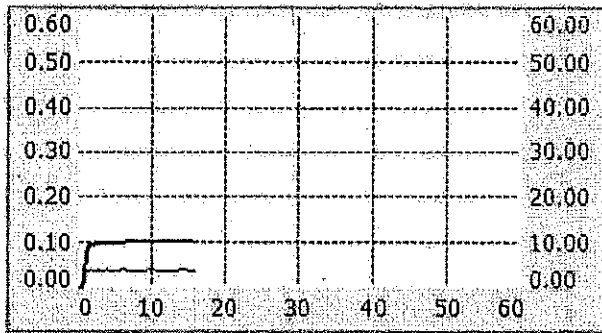

Status:

Status Code:
Date Time:
Message:

SUPERVISOR TEST




NEW HARTFORD TOWN
POLICE DEPT
DATAMASTER dmt: 127606

Date: 06/18/2020

OPERATOR NAME:
MICHAEL T KOWALSKI
Permit #: 31077
Operator Agency/Dept: NEW HARTFORD TOWN PD
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:12
INTERNAL STANDARD	VERIFIED	15:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:12
BLANK TEST	0.00	15:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:13
BLANK TEST	0.00	15:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:15
BLANK TEST	0.00	15:16

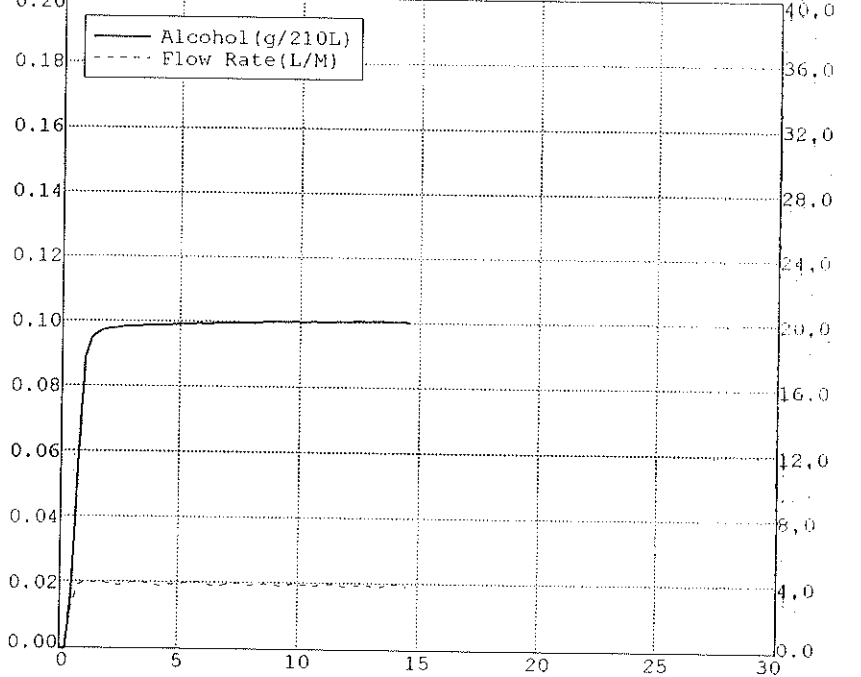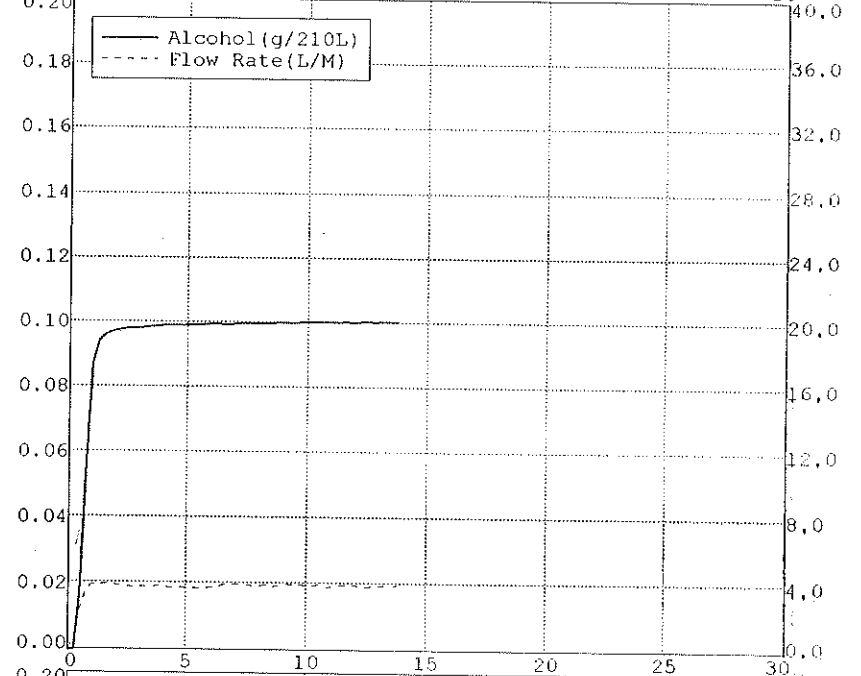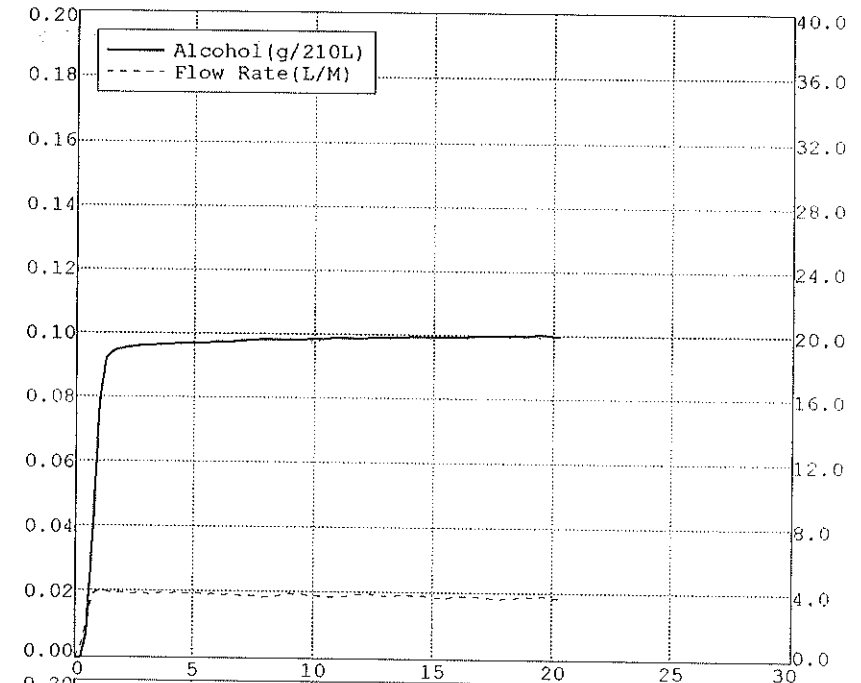

SUPERVISOR TEST




NEW HARTFORD TOWN
POLICE DEPT
DATAMASTER dmt: 127606

Date: 06/18/2020

OPERATOR NAME:
MICHAEL T KOWALSKI
Permit #: 31077
Operator Agency/Dept: NEW HARTFORD TOWN PD
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:37
INTERNAL STANDARD	VERIFIED	15:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:38
BLANK TEST	0.00	15:39
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:39
BLANK TEST	0.00	15:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:40
BLANK TEST	0.00	15:41

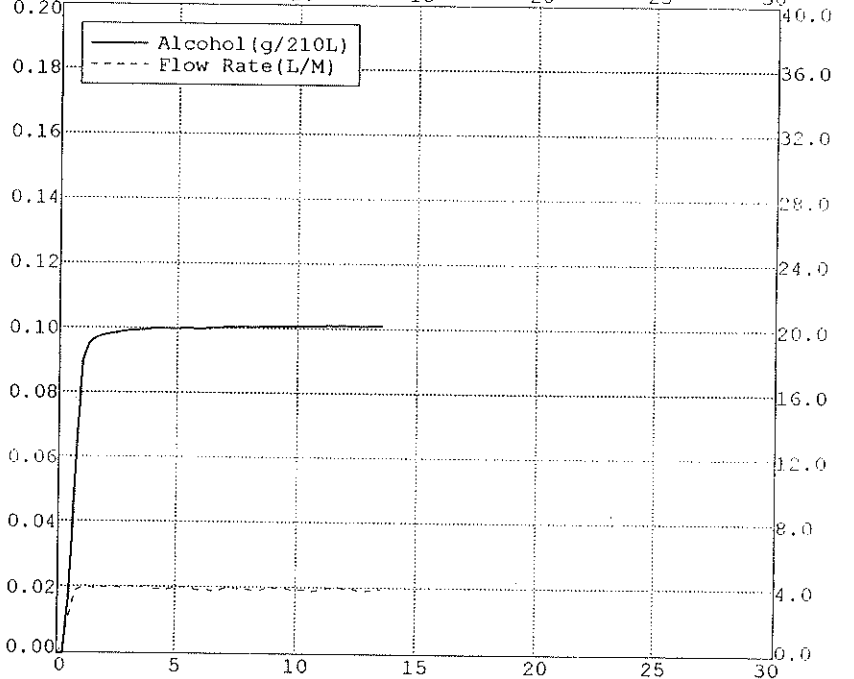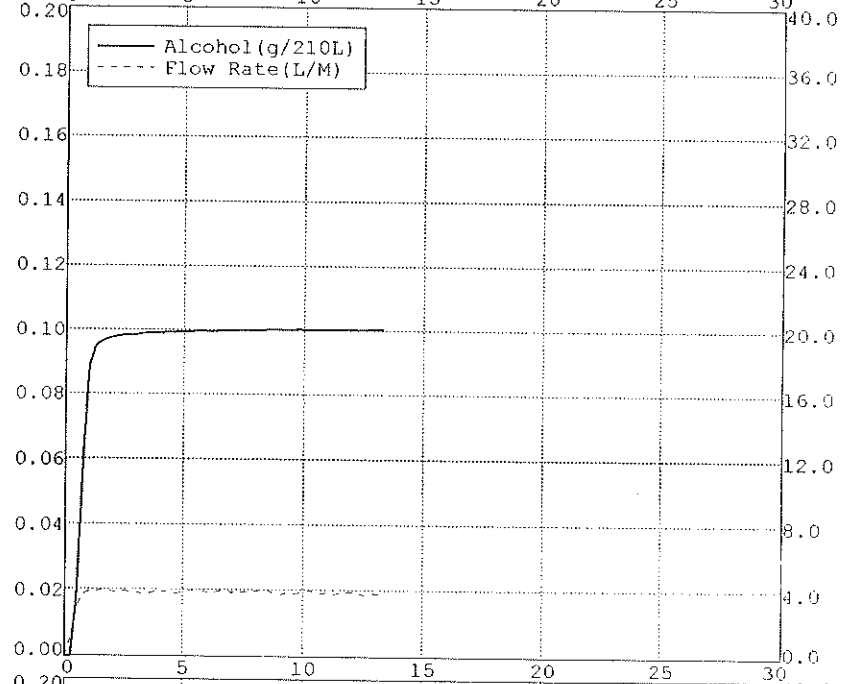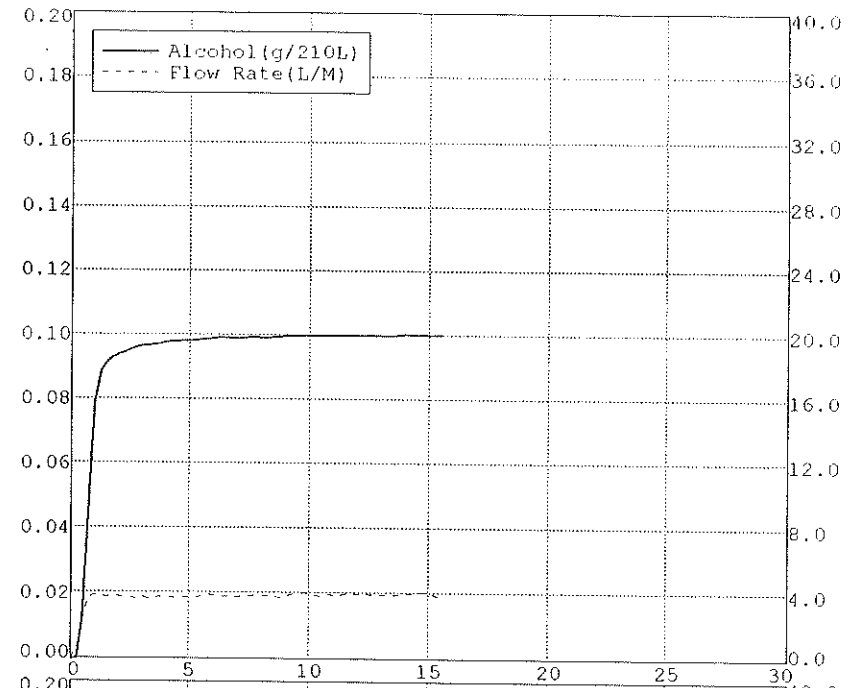

SUPERVISOR TEST




NEW HARTFORD TOWN
 POLICE DEPT
 DATAMASTER dmt: 127606

Date: 06/22/2020

OPERATOR NAME:
 MICHAEL T KOWALSKI
 Permit #: 31077
 Operator Agency/Dept: NEW HARTFORD TOWN PD
 Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:01
INTERNAL STANDARD	VERIFIED	09:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:01
BLANK TEST	0.00	09:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:03
BLANK TEST	0.00	09:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:04
BLANK TEST	0.00	09:05

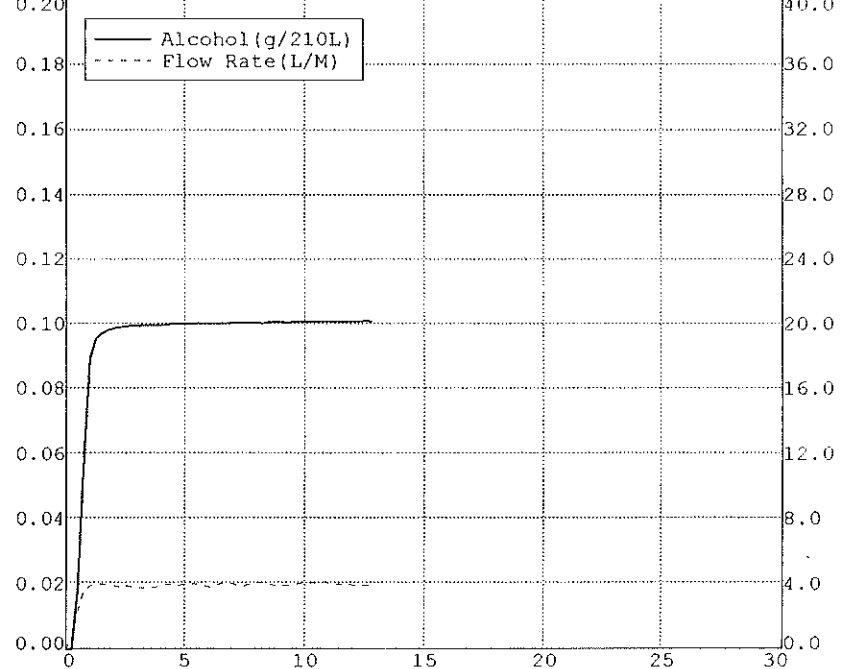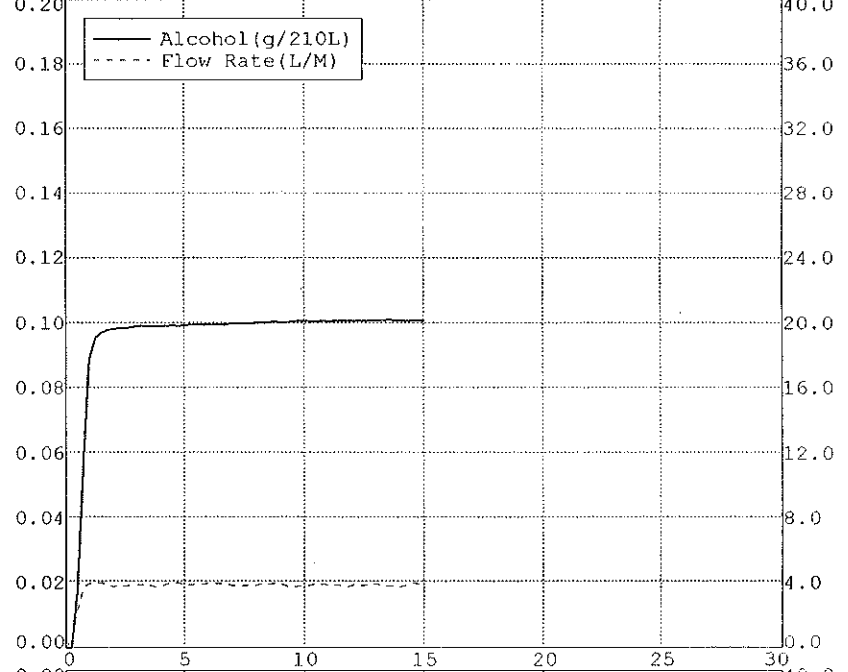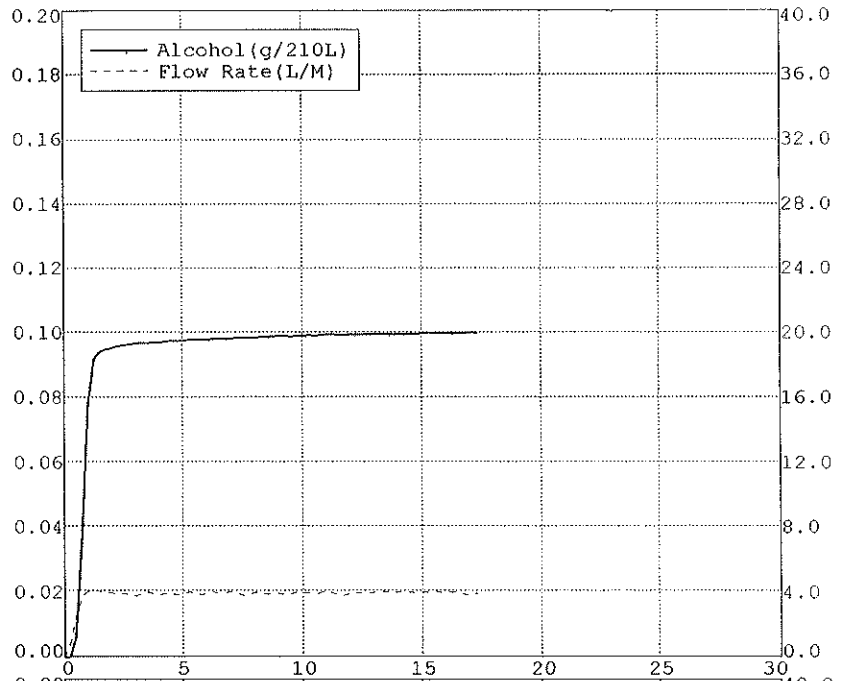

Michael T. Kowalski

From: Coffin, George (DCJS) <George.Coffin@dcjs.ny.gov>
Sent: Thursday, June 18, 2020 3:48 PM
To: Michael T. Kowalski
Subject: Weekly tests
Attachments: Weekly_tests.PDF

Hello,

Attached are the relevant weekly tests.
Please let me know if you have any further questions or concerns.

Thanks,
George Coffin

Michael T. Kowalski

From: Michael T. Kowalski
Sent: Thursday, June 18, 2020 3:48 PM
To: All Users PD
Subject: Data master

They Datamaster is out of service until further notice due to a printer issue. Please contact UPD for arrests requiring a breath test.

Mk

Sent from my iPhone