

SUPERVISOR TEST




NEW HARTFORD TOWN
POLICE DEPT
DATAMASTER dmt: 127606

Date: 05/15/2020

OPERATOR NAME:
MICHAEL T KOWALSKI
Permit #: 31077
Operator Agency/Dept: NEW HARTFORD TOWN PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:39
INTERNAL STANDARD	VERIFIED	09:39
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:39
BLANK TEST	0.00	09:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:40
BLANK TEST " " "	0.00	09:41
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:41
BLANK TEST	0.00	09:42



SUPERVISOR TEST




NEW HARTFORD TOWN
POLICE DEPT
DATAMASTER dmt: 127606

Date: 05/22/2020

OPERATOR NAME:
MICHAEL T KOWALSKI
Permit #: 31077
Operator Agency/Dept: NEW HARTFORD TOWN PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:10
INTERNAL STANDARD	VERIFIED	10:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	10:11
BLANK TEST	0.00	10:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	10:12
BLANK TEST	0.00	10:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	10:13
BLANK TEST	0.00	10:14



SUPERVISOR TEST




NEW HARTFORD TOWN
POLICE DEPT
DATAMASTER dmt: 127606

Date: 05/29/2020

OPERATOR NAME:
MICHAEL T KOWALSKI
Permit #: 31077
Operator Agency/Dept: NEW HARTFORD TOWN PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:26
INTERNAL STANDARD	VERIFIED	07:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:26
BLANK TEST	0.00	07:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:27
BLANK TEST	0.00	07:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:29
BLANK TEST	0.00	07:29

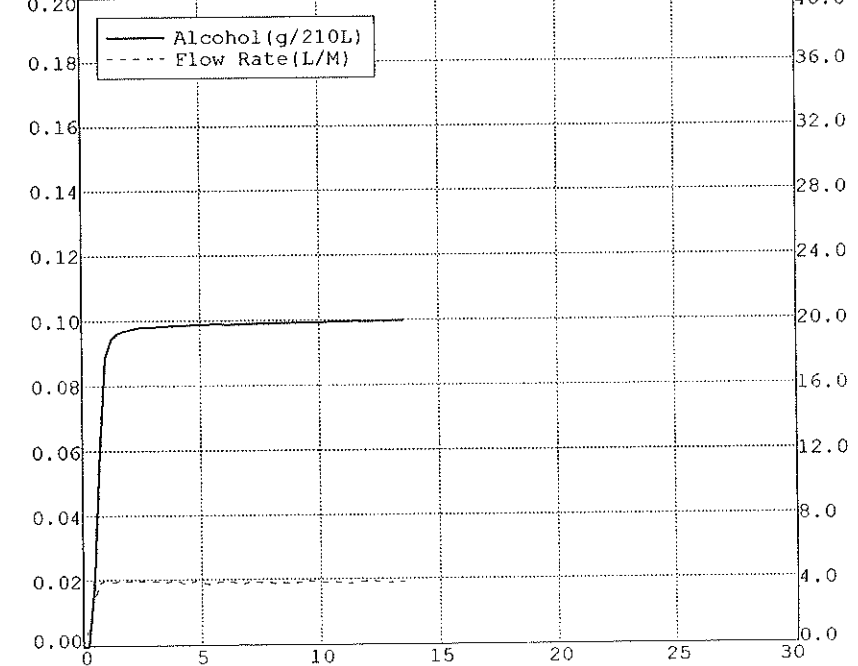

SOLUTION CHANGE




NEW HARTFORD TOWN
 POLICE DEPT
 DATAMASTER dmt: 127606

Date: 06/01/2020

OPERATOR NAME:
 MICHAEL T KOWALSKI
 Permit #: 31077
 Operator Agency/Dept: NEW HARTFORD TOWN PD
 Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:07
INTERNAL STANDARD	VERIFIED	13:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:08
BLANK TEST	0.00	13:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	13:09
BLANK TEST	0.00	13:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:10
BLANK TEST	0.00	13:11



BREATH INSTRUMENT
CALIBRATION TEST RECORD

Dept. NEW HARTFORD POLICE DEPARTMENT

Inst. No. 127606

DATE	SOLUTION LOT NO.	TEST RESULTS			TEMP.	OPERATOR	SIMULATOR EQUILIBRA
		1	2	3			
3/1/20	19350					new solution	MP4199
3/1/20	19350	.10	.10	.10	34.0	Kawinski	" "
3/6/20	19350	.10	.10	.10	34.0	" "	" "
3/12/20	19350	.10	.10	.10	34.0	" "	" "
3/20/20	19350	.10	.10	.10	34.0	" "	" "
3/27/20	19350	.10	.10	.10	34.0	" "	" "
3/31/20	20070					new solution	" "
3/31/20	20070	.10	.10	.10	34.0	Kawinski	" "
4/7/20	20070	.10	.10	.10	34.0	" "	" "
4/15/20	20070	.10	.10	.10	34.0	" "	" "
4/22/20	20070	.10	.10	.10	34.0	" "	" "
4/29/20	20070	.09	.10	.10	34.0	" "	" "
5/3/20	20070					new solution	" "
5/3/20	20070	.10	.10	.10	34.0	Kawinski	" "
5/7/20	20070	.10	.10	.10	34.0	" "	" "
5/15/20	20070	.10	.10	.10	34.0	" "	" "
5/22/20	20070	.10	.10	.10	34.0	" "	" "
5/29/20	20070	.09	.09	.10	34.0	" "	" "
6/1/20	20170					new solution	" "
6/1/20	20170	.10	.10	.10	34.0	Kawinski	" "