

SOLUTION CHANGE



ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 07/03/2019

OPERATOR NAME:
MICHAEL P BAKER
Permit #: 44230
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:09
INTERNAL STANDARD	VERIFIED	19:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	19:09
BLANK TEST	0.00	19:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	19:11
BLANK TEST	0.00	19:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	19:12
BLANK TEST	0.00	19:13

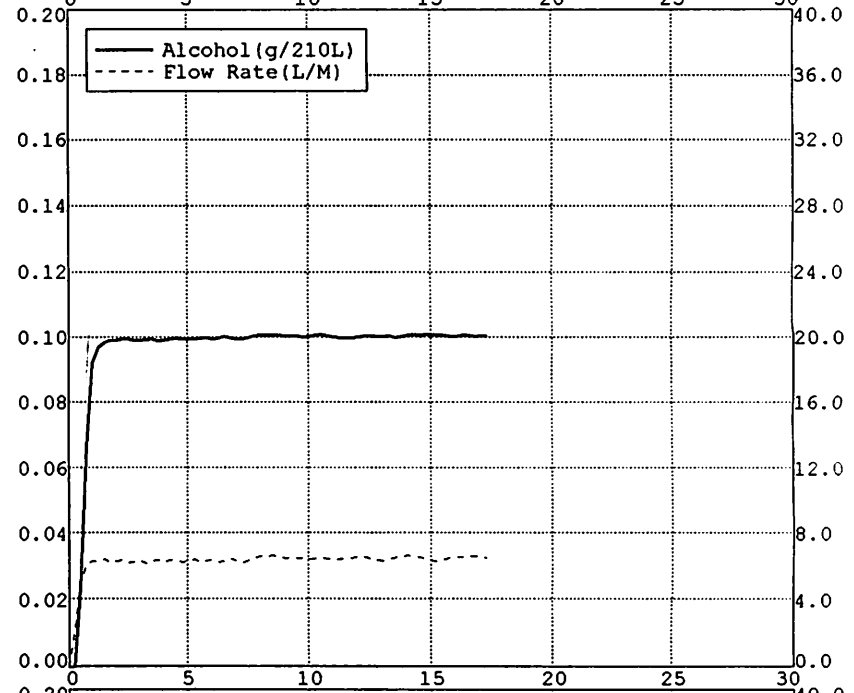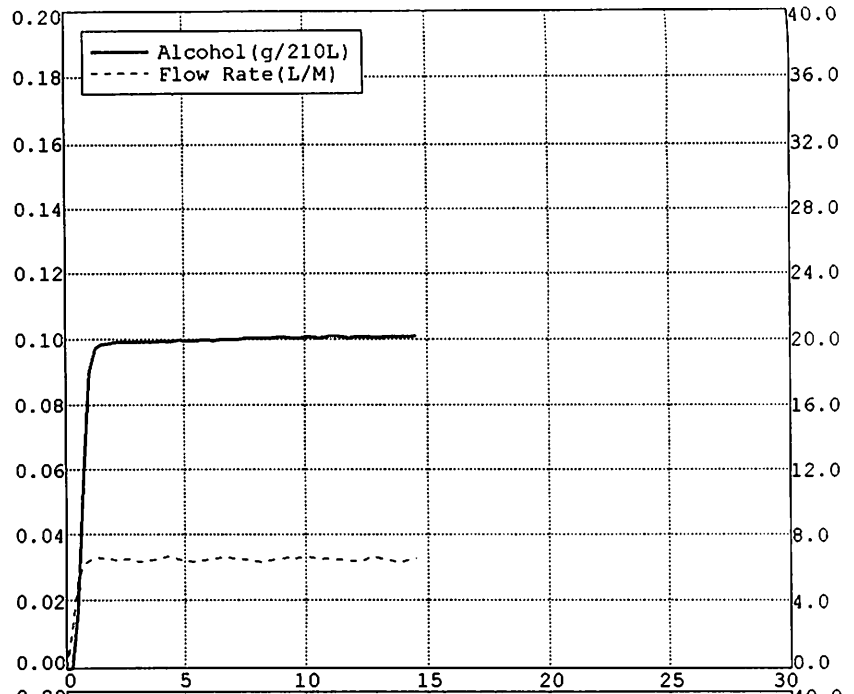

SOLUTION CHANGE




ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 07/03/2019

OPERATOR NAME:
MICHAEL P BAKER
Permit #: 44230
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:09
INTERNAL STANDARD	VERIFIED	19:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	19:09
BLANK TEST	0.00	19:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	19:11
BLANK TEST	0.00	19:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	19:12
BLANK TEST	0.00	19:13

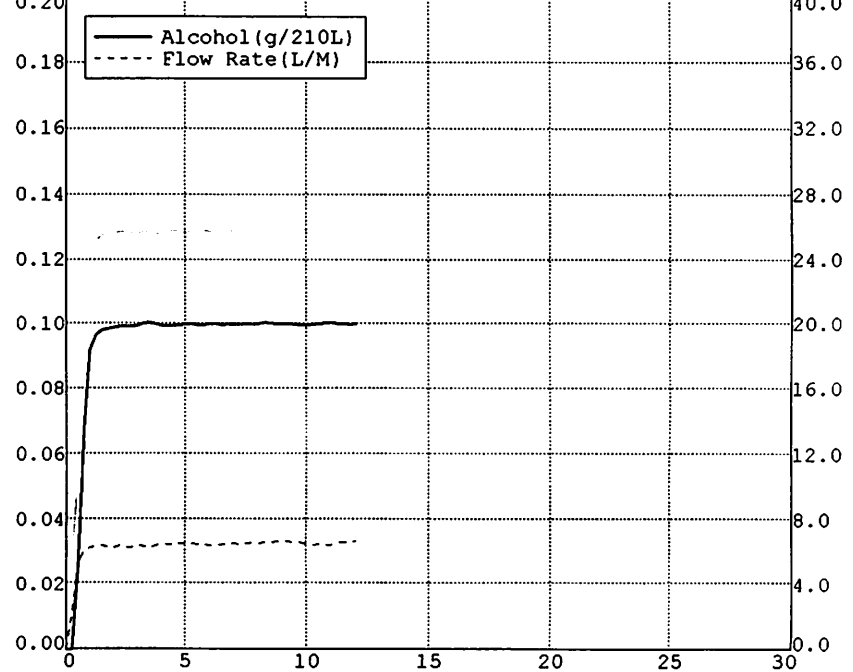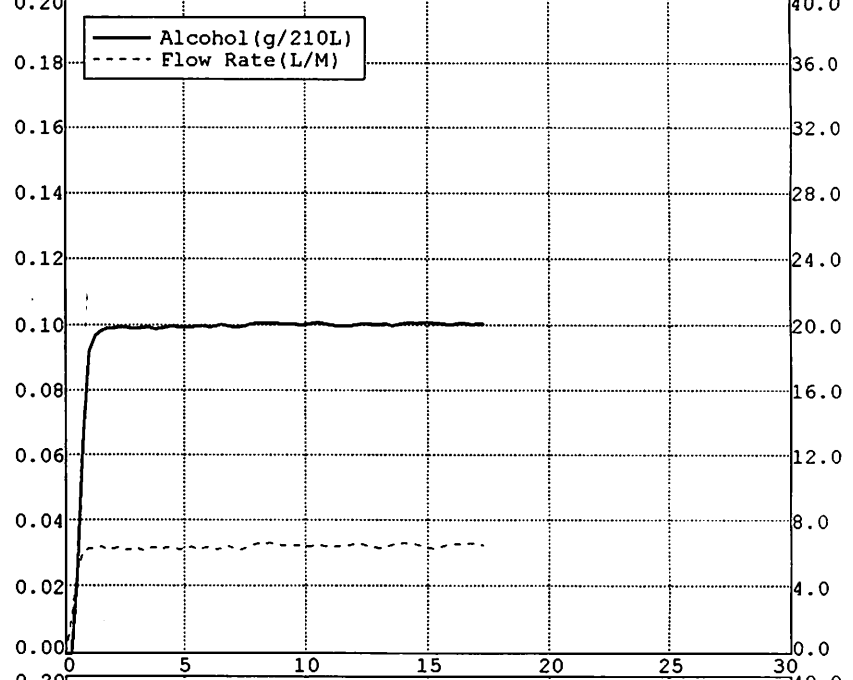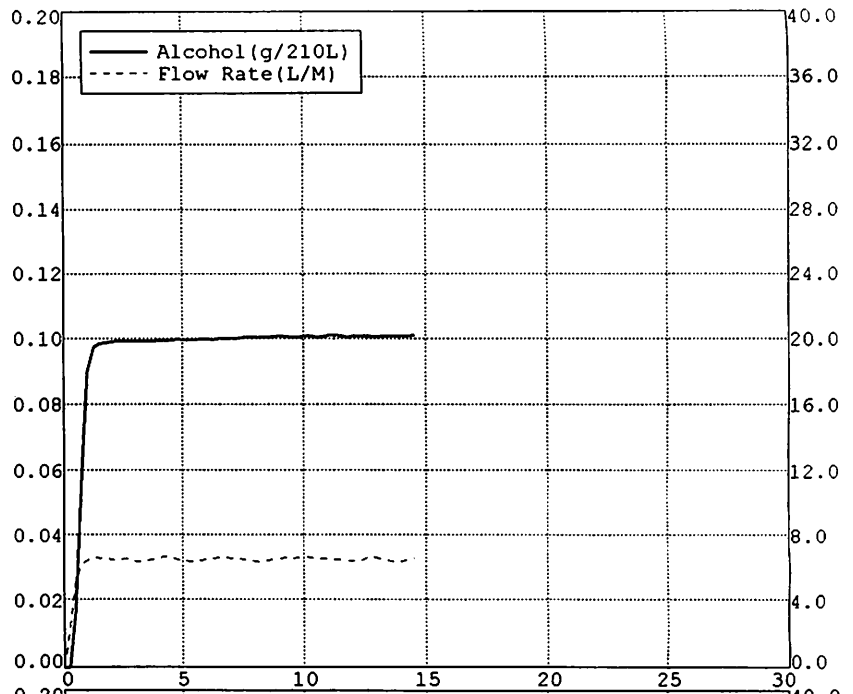

SUPERVISOR TEST

LEB




ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 07/10/2019

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:28
INTERNAL STANDARD	VERIFIED	18:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:28
BLANK TEST	0.00	18:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:29
BLANK TEST	0.00	18:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:31
BLANK TEST	0.00	18:31

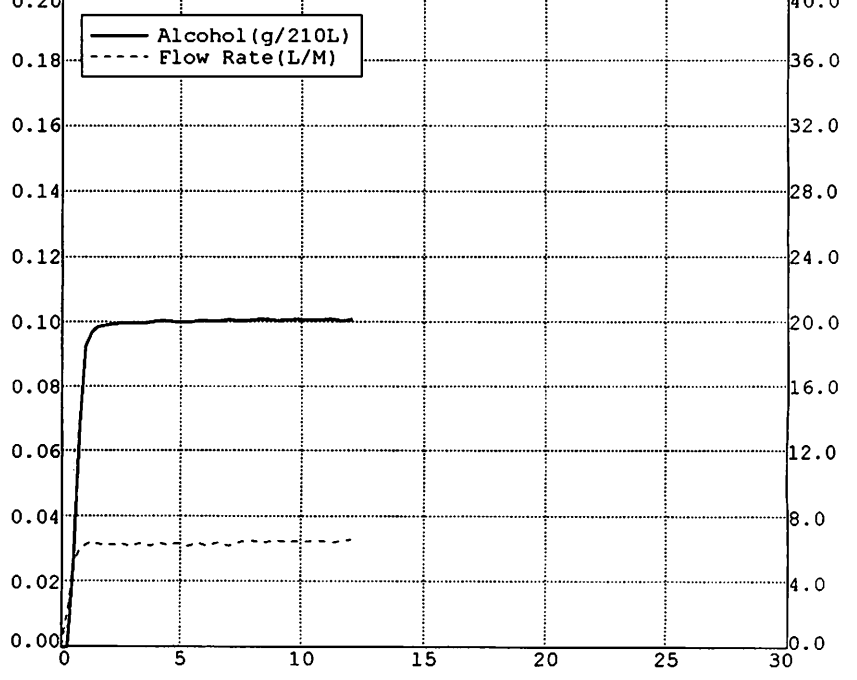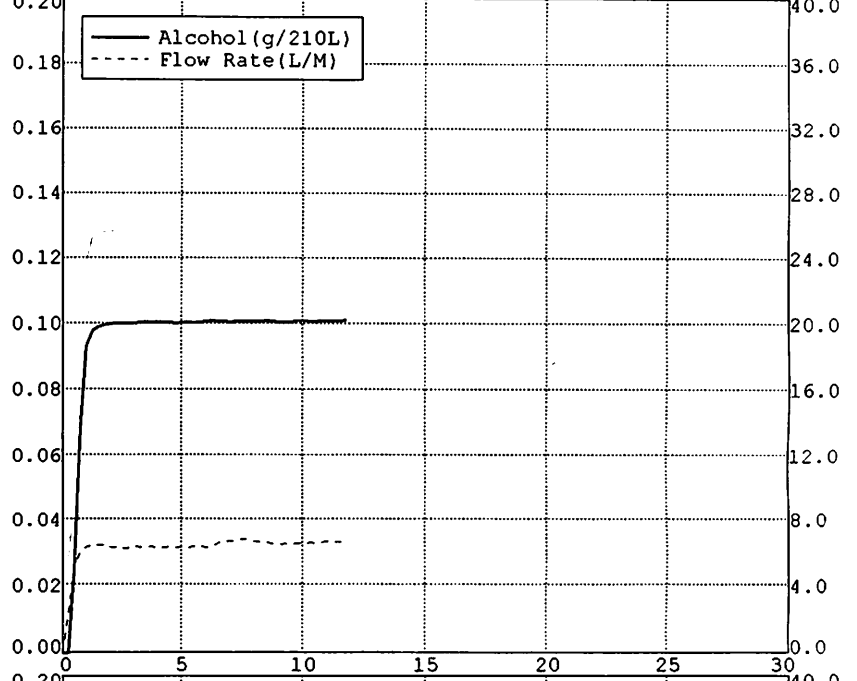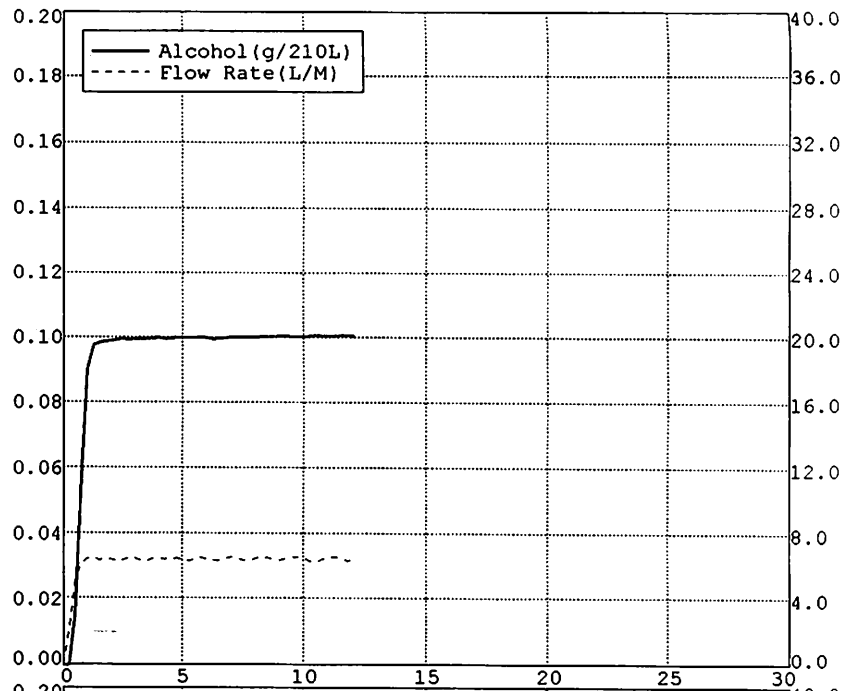

SUPERVISOR TEST



ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 07/19/2019

OPERATOR NAME:
BRANDON J RUTLEDGE
Permit #: 43762
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:29
INTERNAL STANDARD	VERIFIED	05:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:30
BLANK TEST	0.00	05:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:31
BLANK TEST	0.00	05:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:32
BLANK TEST	0.00	05:33

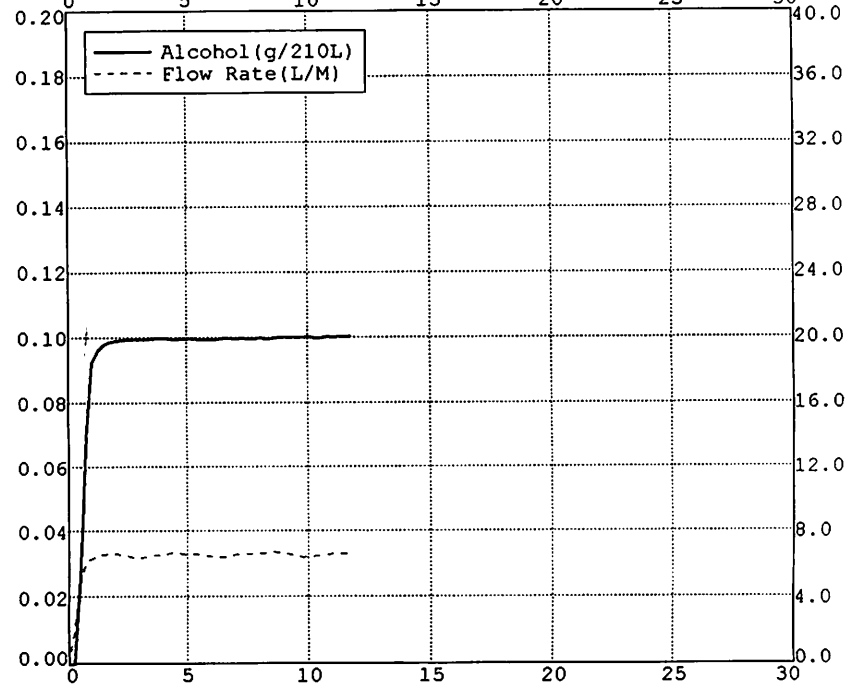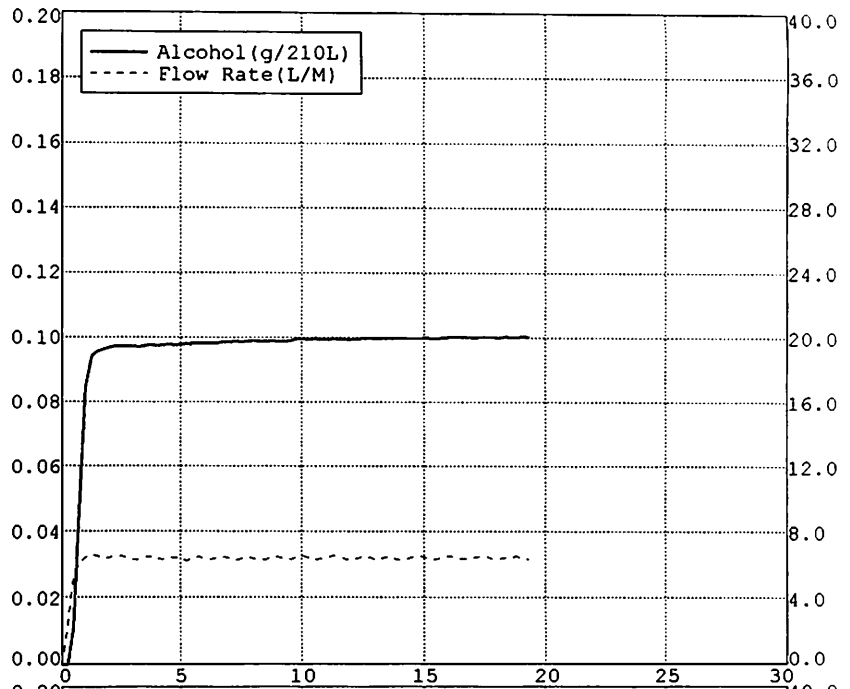

SUPERVISOR TEST

LEB




ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 07/24/2019

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:56
INTERNAL STANDARD	VERIFIED	17:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:56
BLANK TEST	0.00	17:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:57
BLANK TEST	0.00	17:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:59
BLANK TEST	0.00	17:59

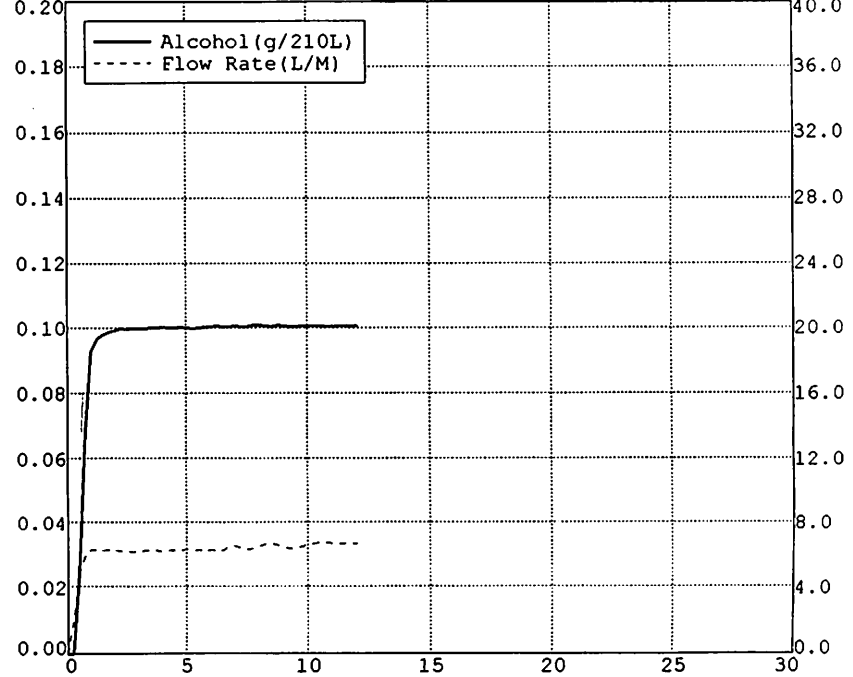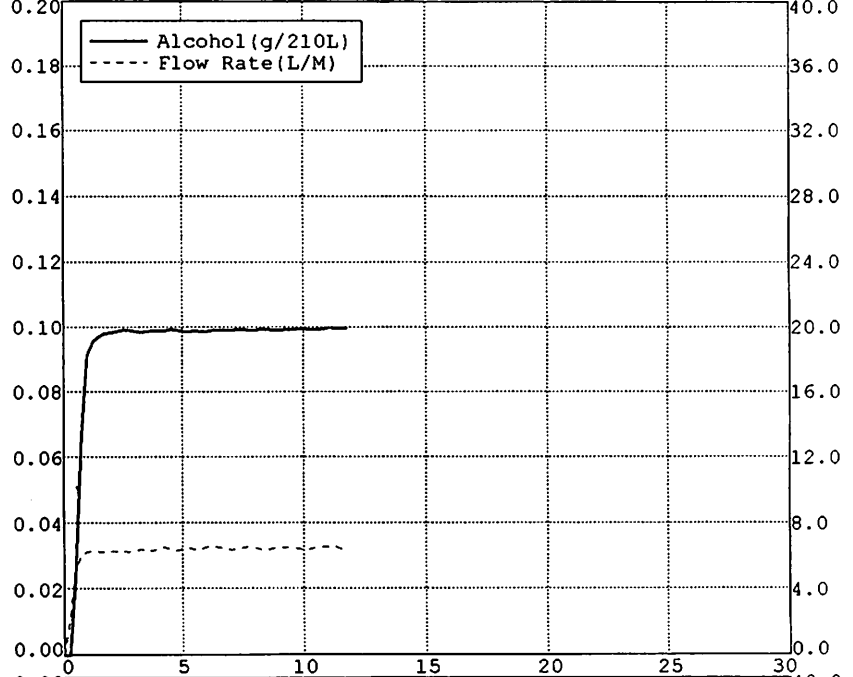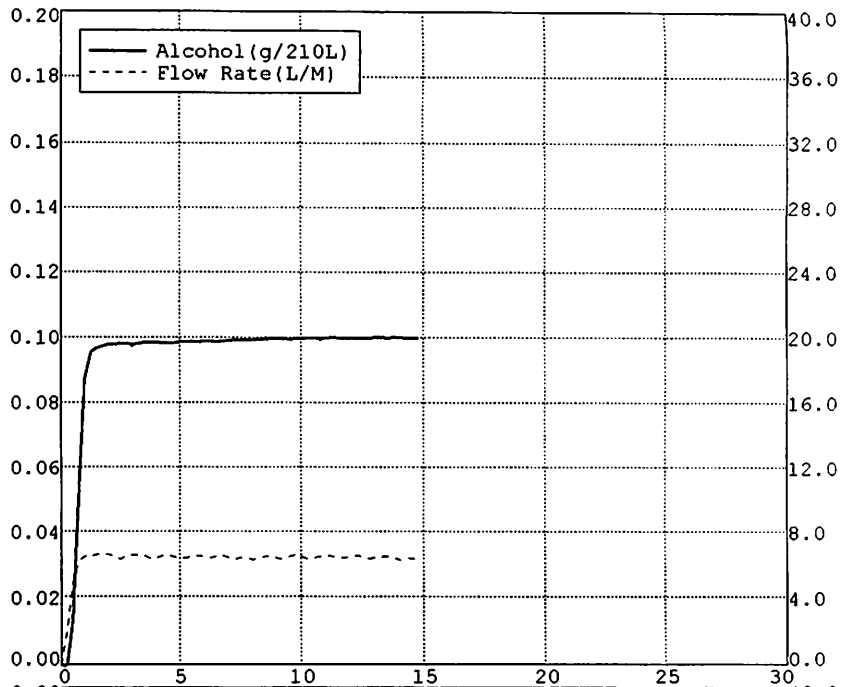

LES

SOLUTION CHANGE




ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 08/01/2019

OPERATOR NAME:
JOHN R BOWERS
Permit #: 46887
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:38
INTERNAL STANDARD	VERIFIED	18:38
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:38
BLANK TEST	0.00	18:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:40
BLANK TEST	0.00	18:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:41
BLANK TEST	0.00	18:42

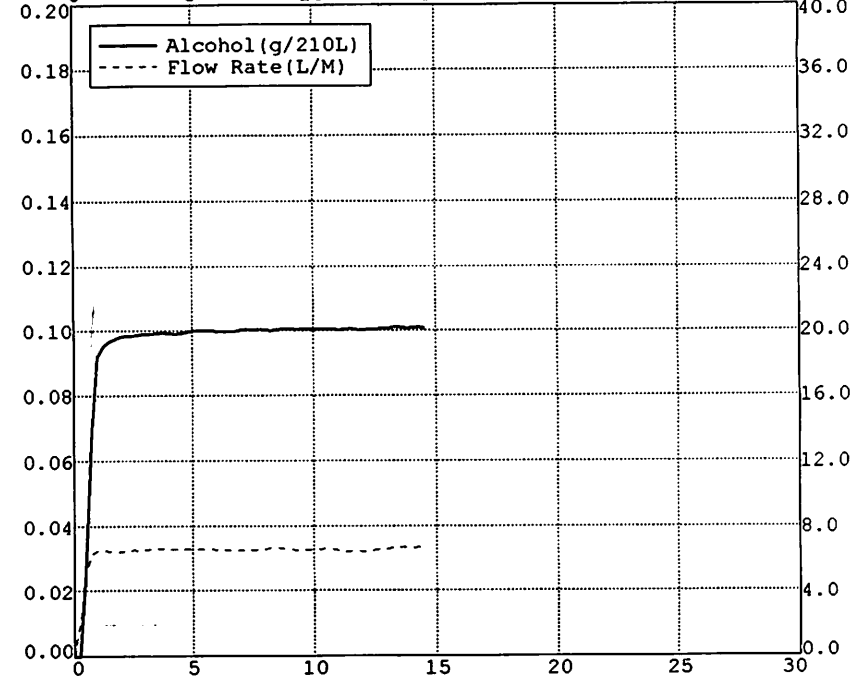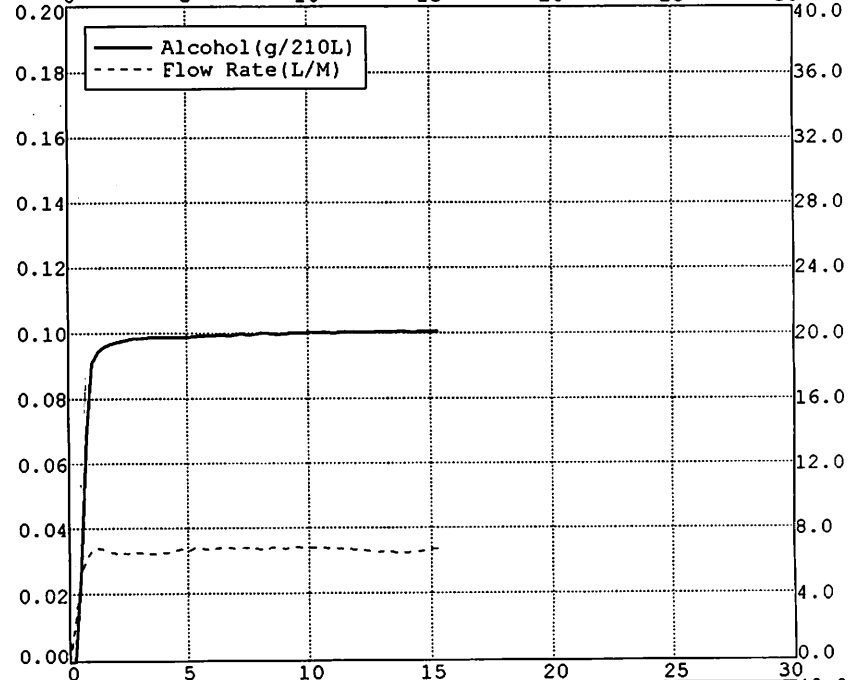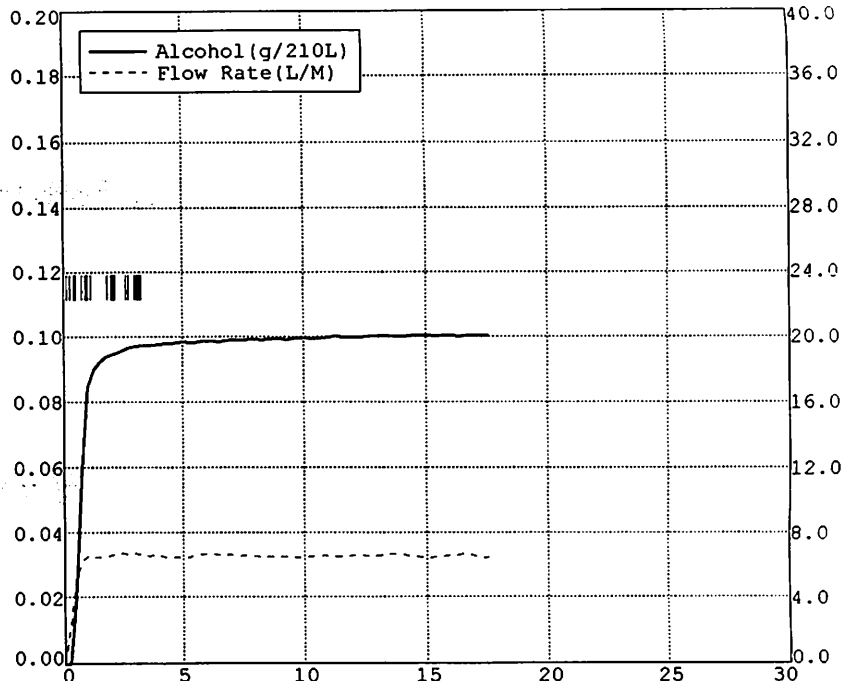

SUPERVISOR TEST

LEB

ONEIDA COUNTY
 SHERIFF'S OFFICE
 DATAMASTER dmt: 113606

Date: 08/07/2019




OPERATOR NAME:
 BRETT A GRABELDINGER
 Permit #: 46896
 Operator Agency/Dept: ONEIDA CO. SO
 Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:04
INTERNAL STANDARD	VERIFIED	18:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:04
BLANK TEST	0.00	18:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:05
BLANK TEST	0.00	18:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:06
BLANK TEST	0.00	18:07

ONEIDA CO. SO

0.09 18:05

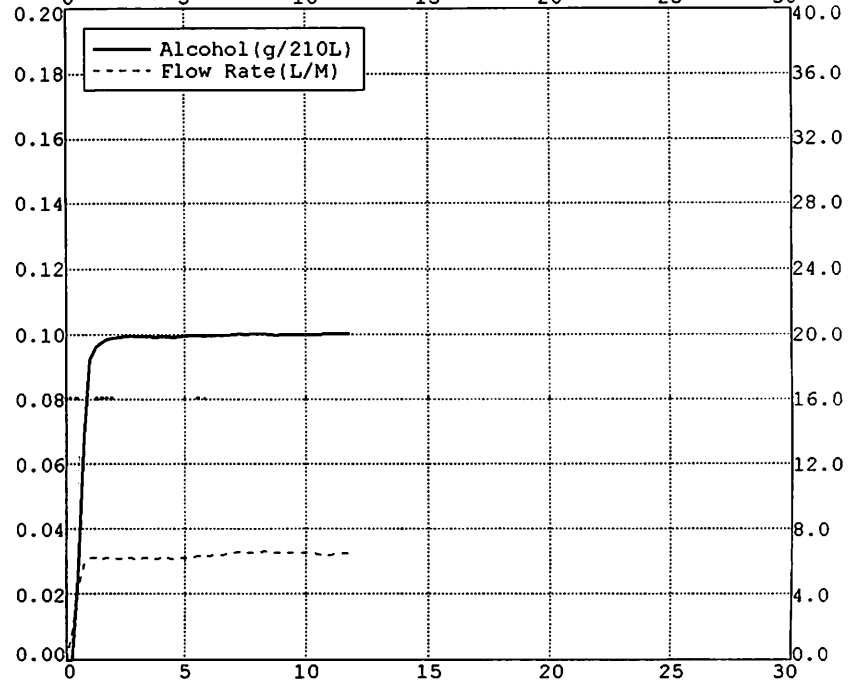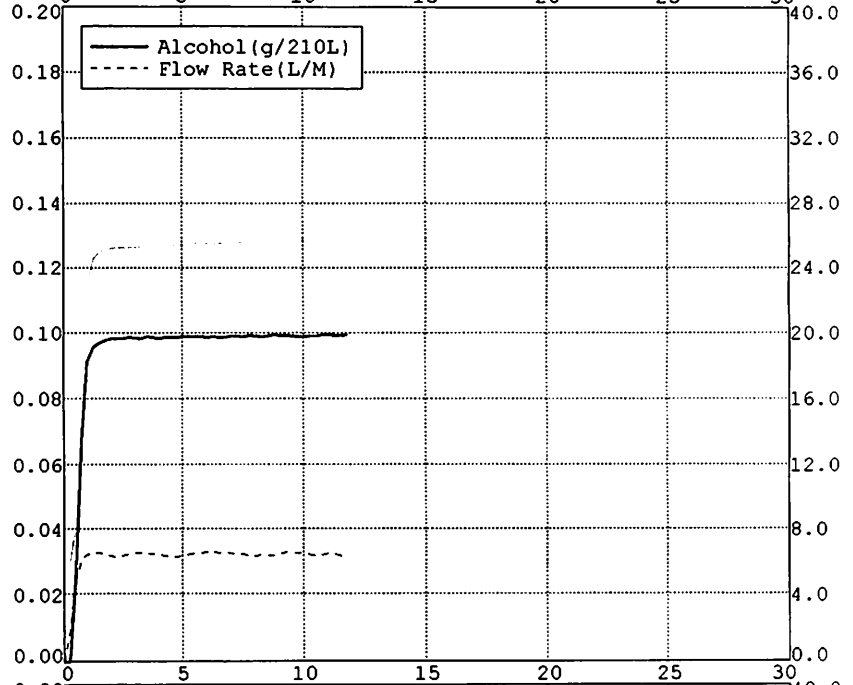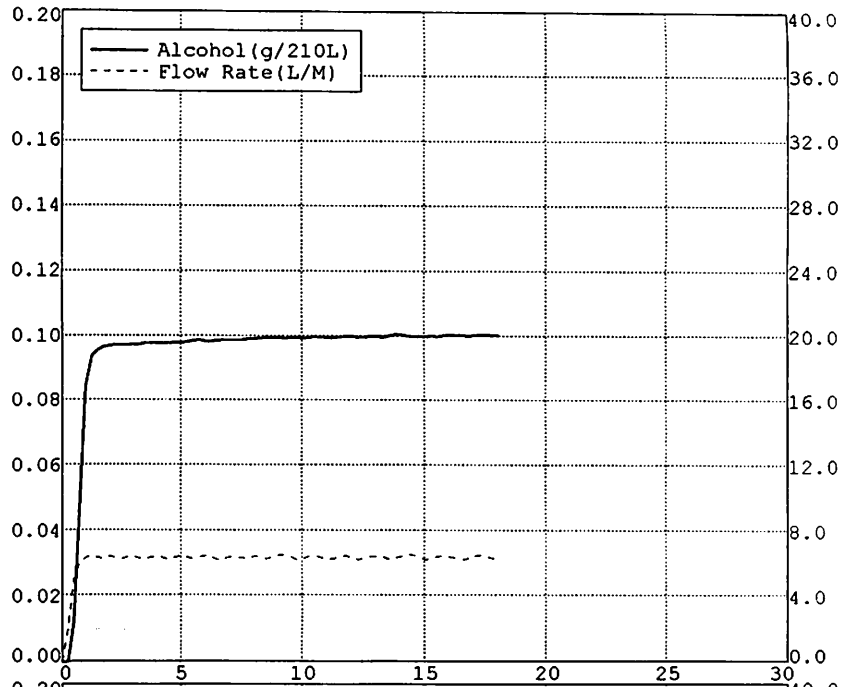

LEB

SUPERVISOR TEST




ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 08/14/2019

OPERATOR NAME:
JOHN R BOWERS
Permit #: 46887
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:43
INTERNAL STANDARD	VERIFIED	23:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	23:43
BLANK TEST	0.00	23:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:45
BLANK TEST	0.00	23:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:46
BLANK TEST	0.00	23:47

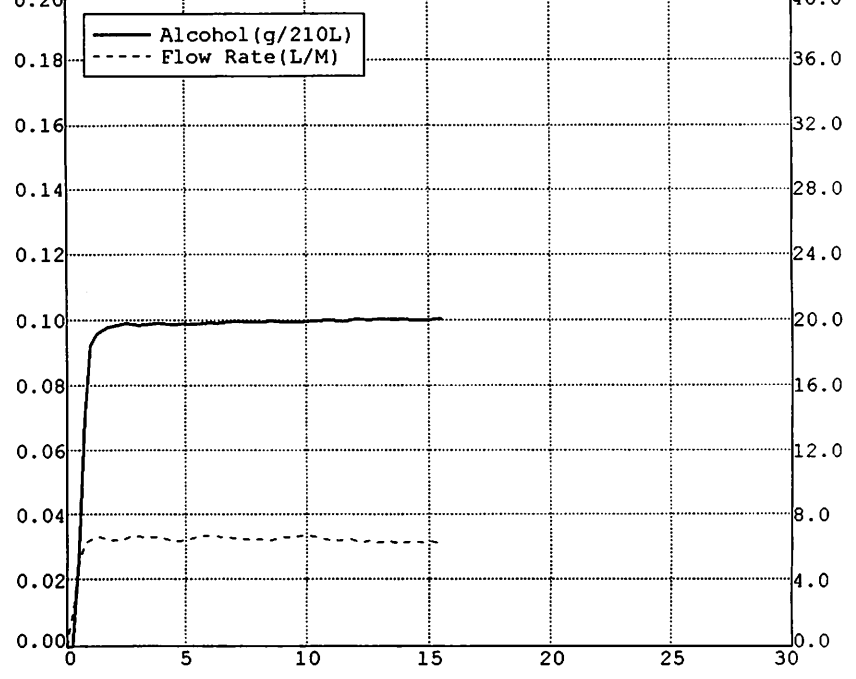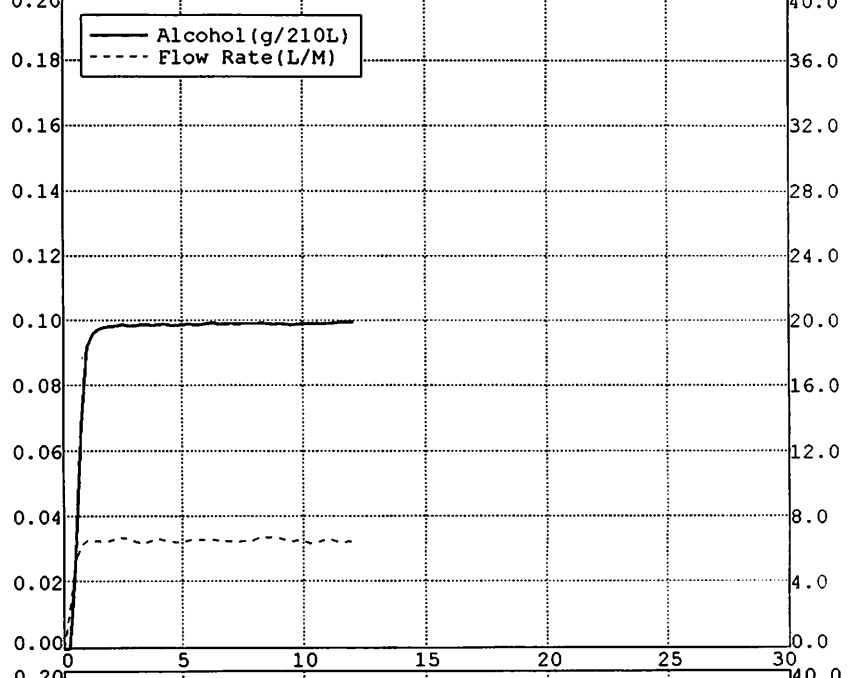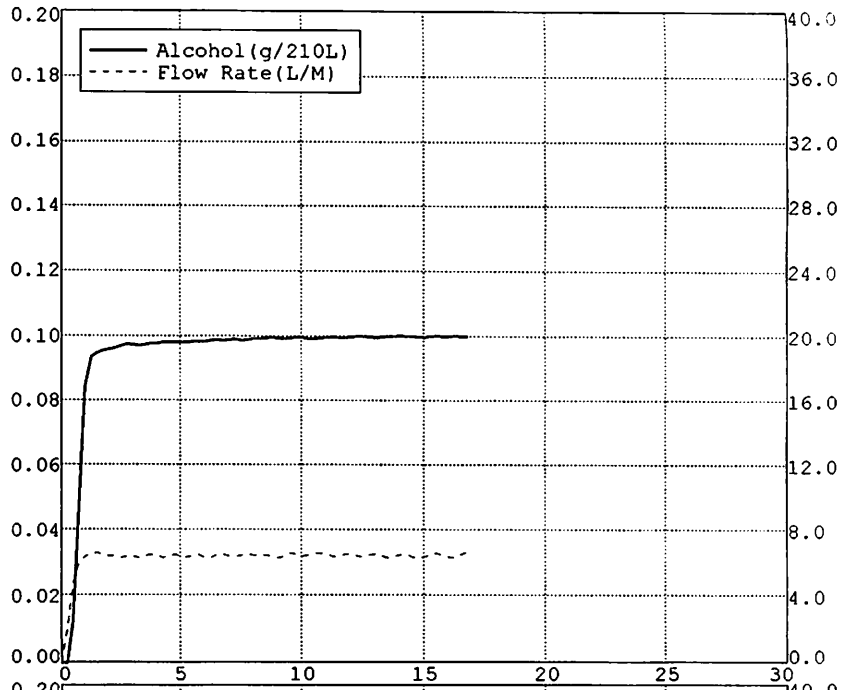

SUPERVISOR TEST

LEB




ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 08/21/2019

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:44
INTERNAL STANDARD	VERIFIED	18:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:45
BLANK TEST	0.00	18:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:46
BLANK TEST	0.00	18:47
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:47
BLANK TEST	0.00	18:48

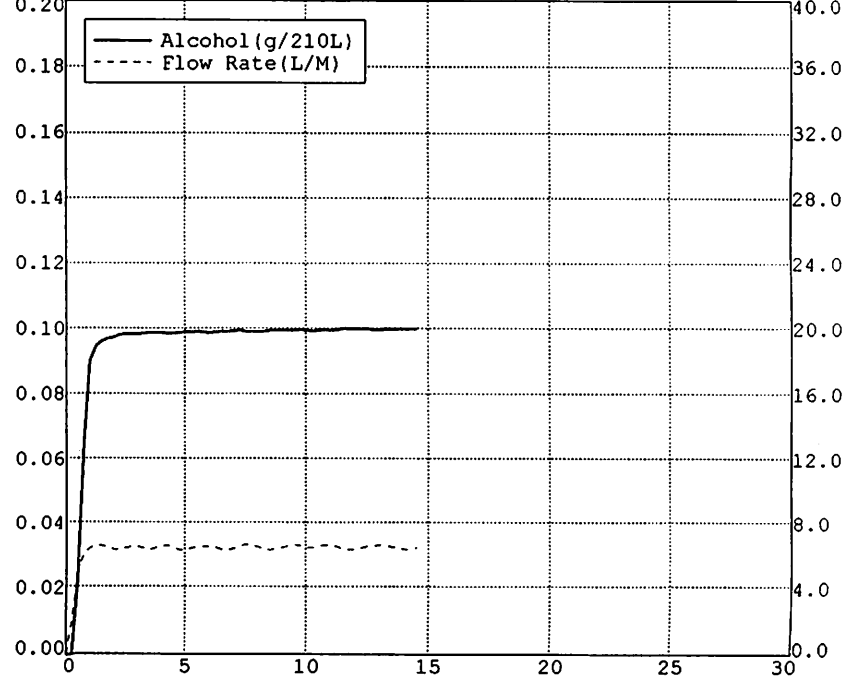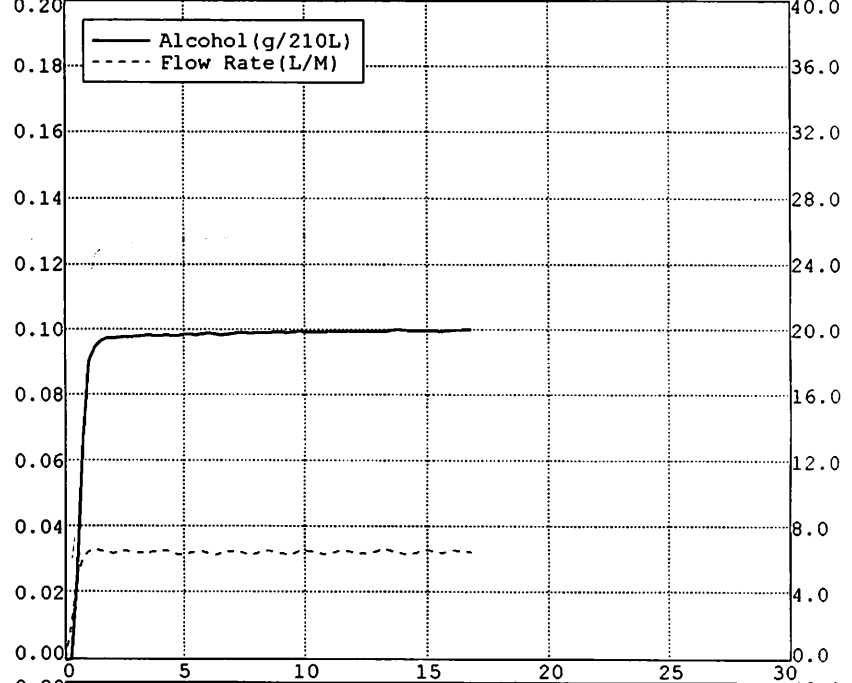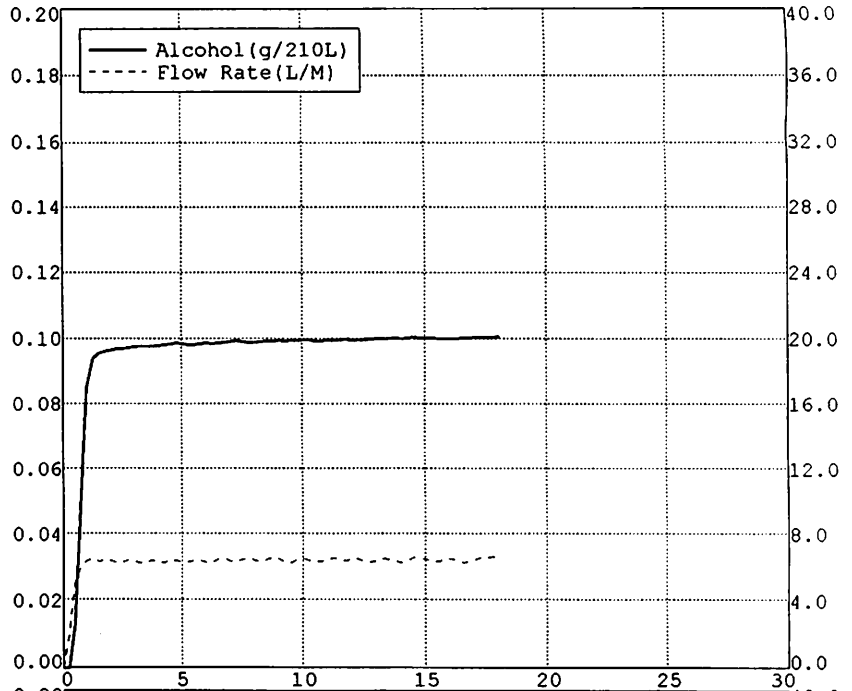

SUPERVISOR TEST



ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 08/28/2019

OPERATOR NAME:
BRANDON J RUTLEDGE
Permit #: 43762
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:55
INTERNAL STANDARD	VERIFIED	19:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	19:55
BLANK TEST	0.00	19:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	19:57
BLANK TEST	0.00	19:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	19:58
BLANK TEST	0.00	19:59

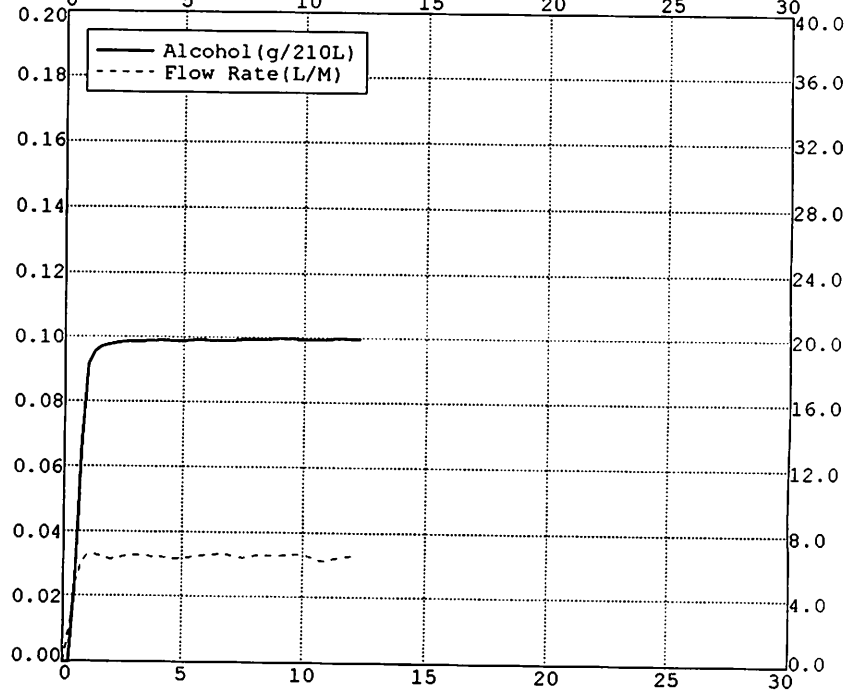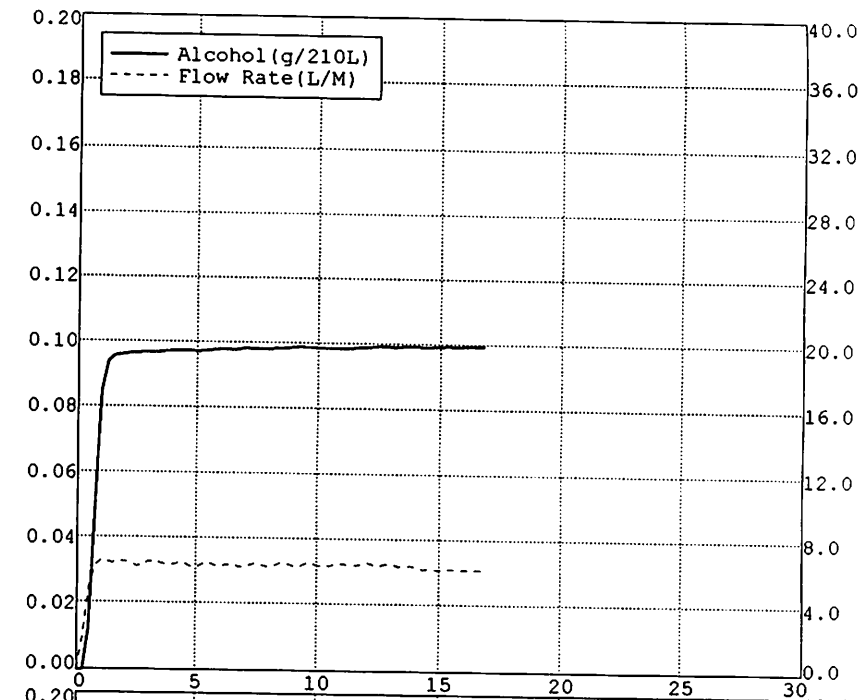

SUPERVISOR TEST

LEB




ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 09/01/2019

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 16896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:30
INTERNAL STANDARD	VERIFIED	18:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:31
BLANK TEST	0.00	18:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:32
BLANK TEST	0.00	18:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:33
BLANK TEST	0.00	18:34

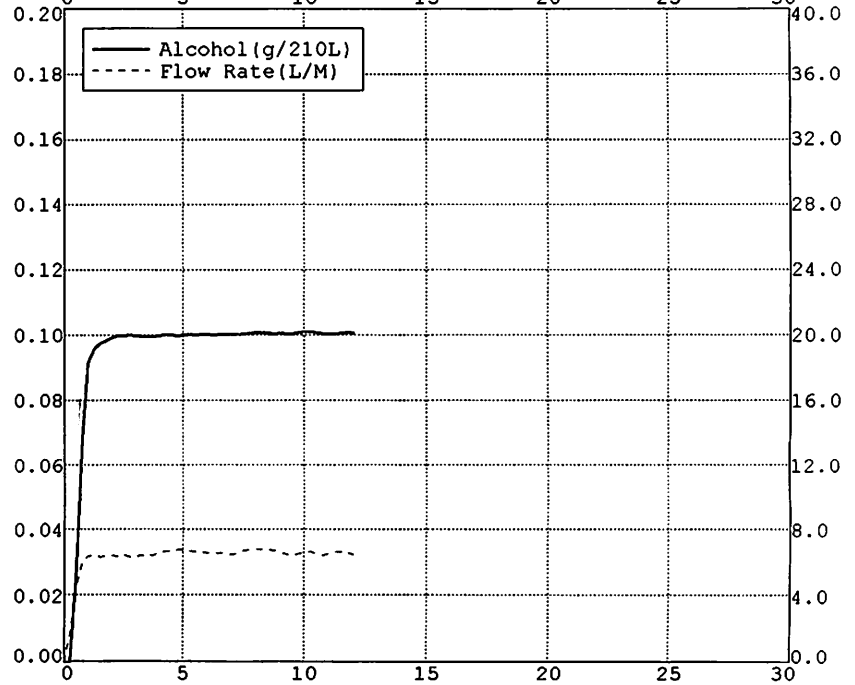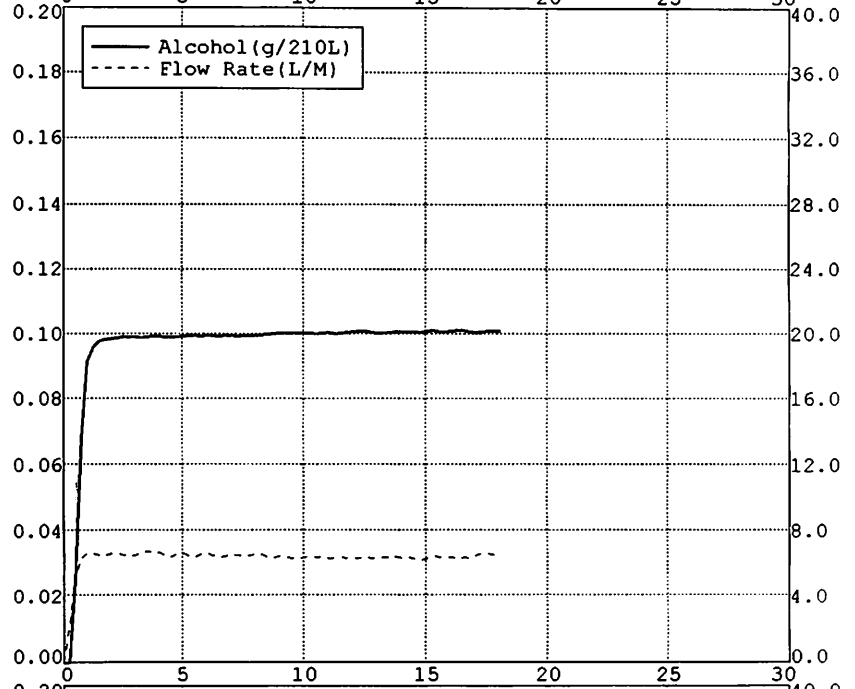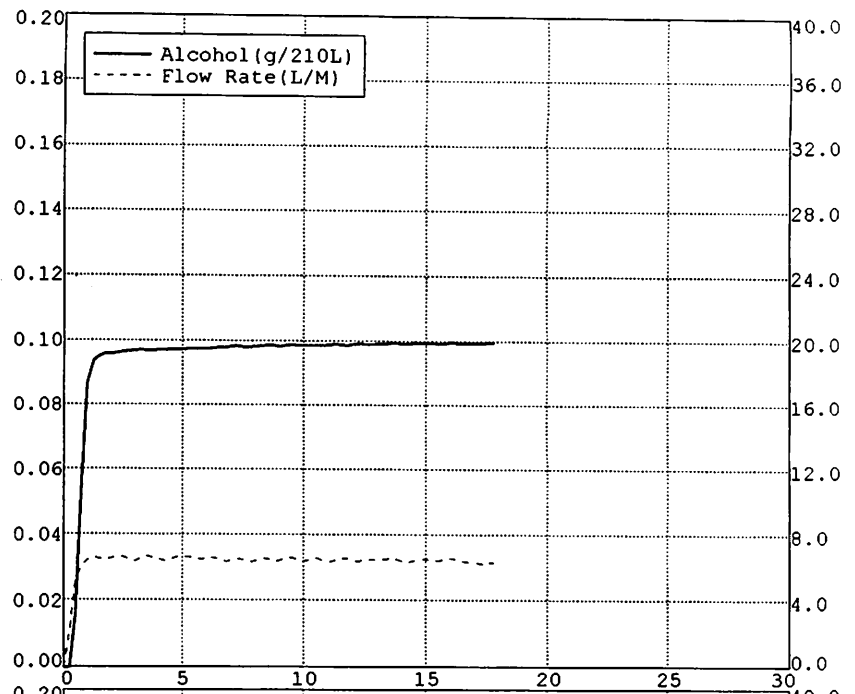

SUPERVISOR TEST

LEB




ONEIDA COUNTY
 SHERIFF'S OFFICE
 DATAMASTER dmt: 113606

Date: 09/04/2019

OPERATOR NAME:
 BRETT A GRABELDINGER
 Permit #: 46896
 Operator Agency/Dept: ONEIDA CO. SO
 Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:18
INTERNAL STANDARD	VERIFIED	18:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:18
BLANK TEST	0.00	18:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:19
BLANK TEST	0.00	18:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:20
BLANK TEST	0.00	18:21

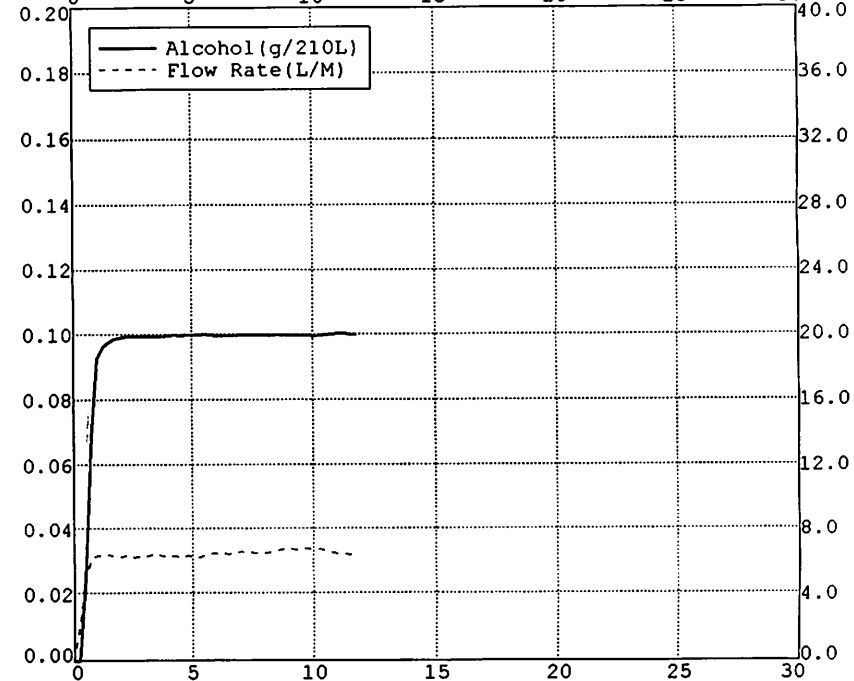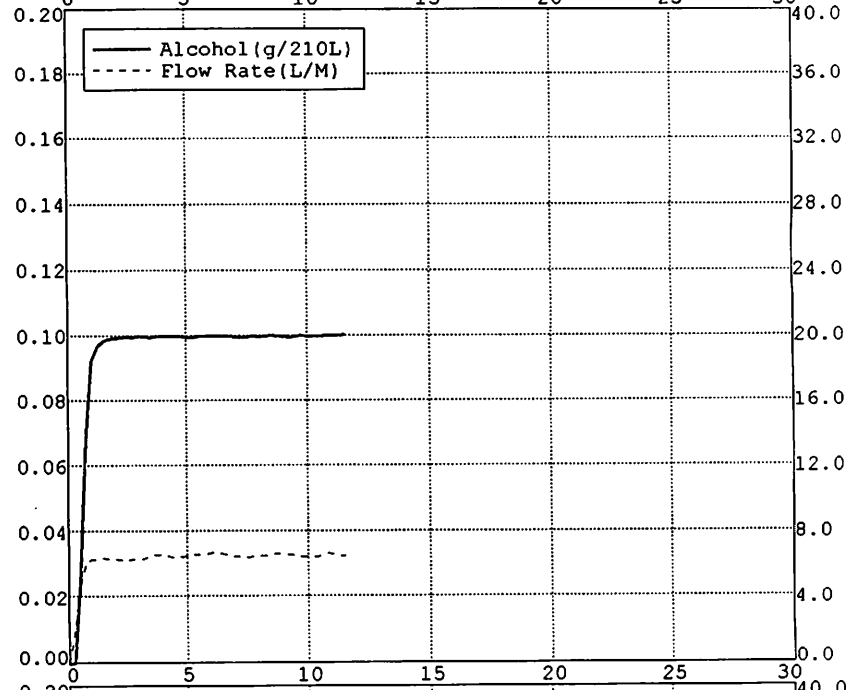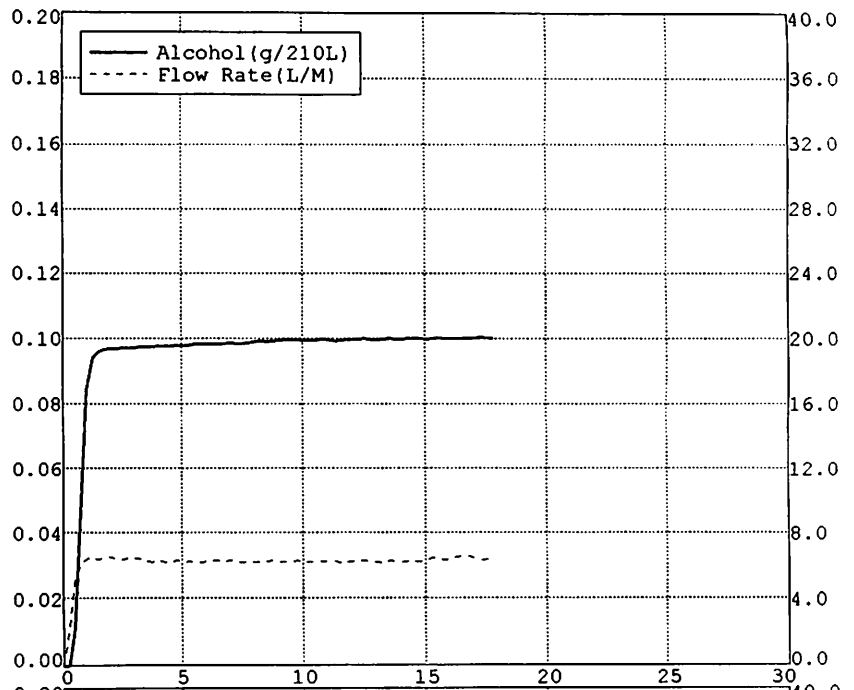

SUPERVISOR TEST




 ONEIDA COUNTY
 SHERIFF'S OFFICE
 DATAMASTER dmt: 113606

Date: 09/11/2019

OPERATOR NAME:
 BRANDON J RUTLEDGE
 Permit #: 43762
 Operator Agency/Dept: ONEIDA CO. SO
 Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:16
INTERNAL STANDARD	VERIFIED	21:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:16
BLANK TEST	0.00	21:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:17
BLANK TEST	0.00	21:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:19
BLANK TEST	0.00	21:20

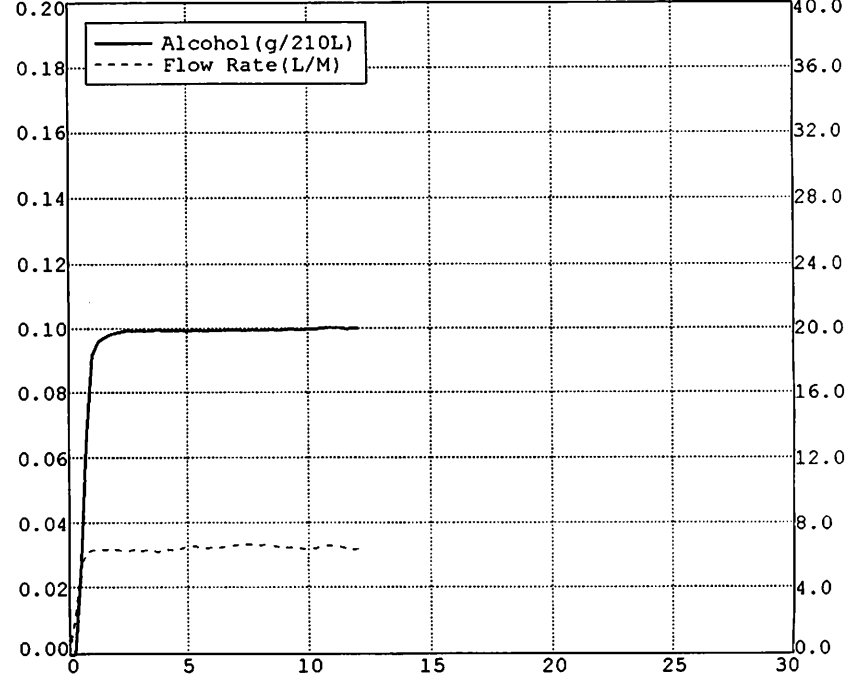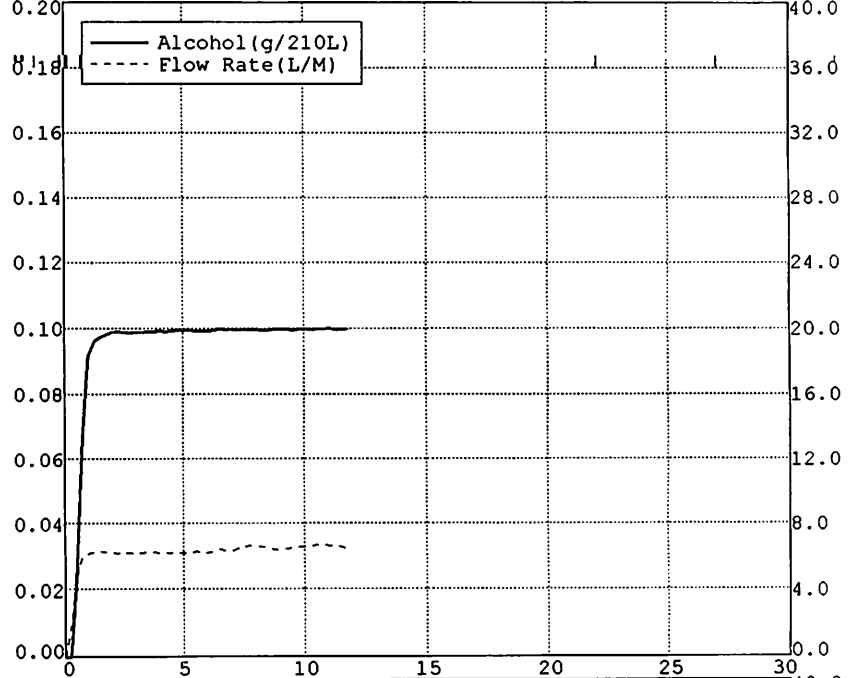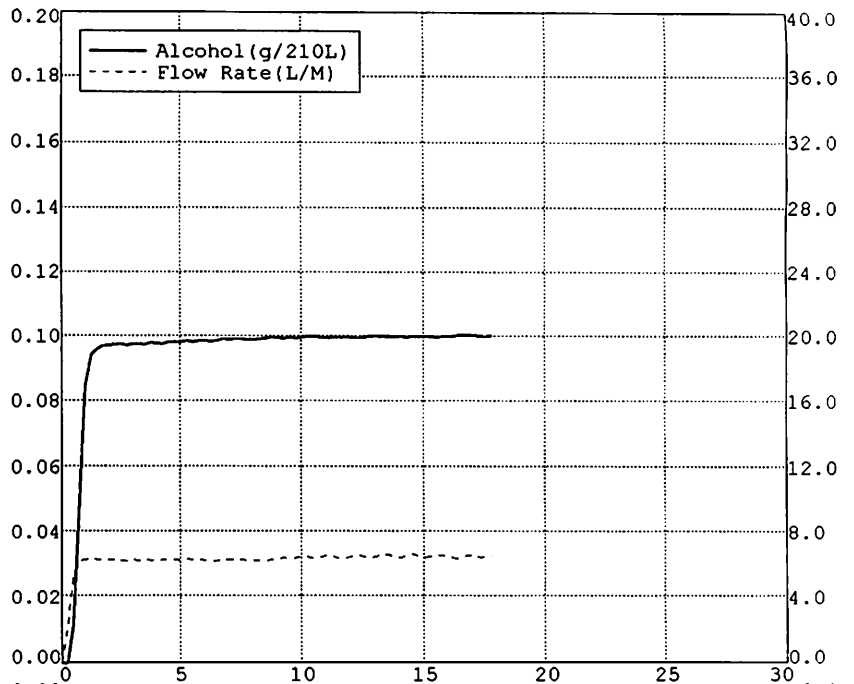

SUPERVISOR TEST

LEB




ONEIDA COUNTY
 SHERIFF'S OFFICE
 DATAMASTER dmt: 113606

Date: 09/18/2019

OPERATOR NAME:
 BRETT A GRABELDINGER
 Permit #: 46896
 Operator Agency/Dept: ONEIDA CO. SO
 Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:14
INTERNAL STANDARD	VERIFIED	18:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:15
BLANK TEST	0.00	18:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:16
BLANK TEST	0.00	18:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:17
BLANK TEST	0.00	18:18

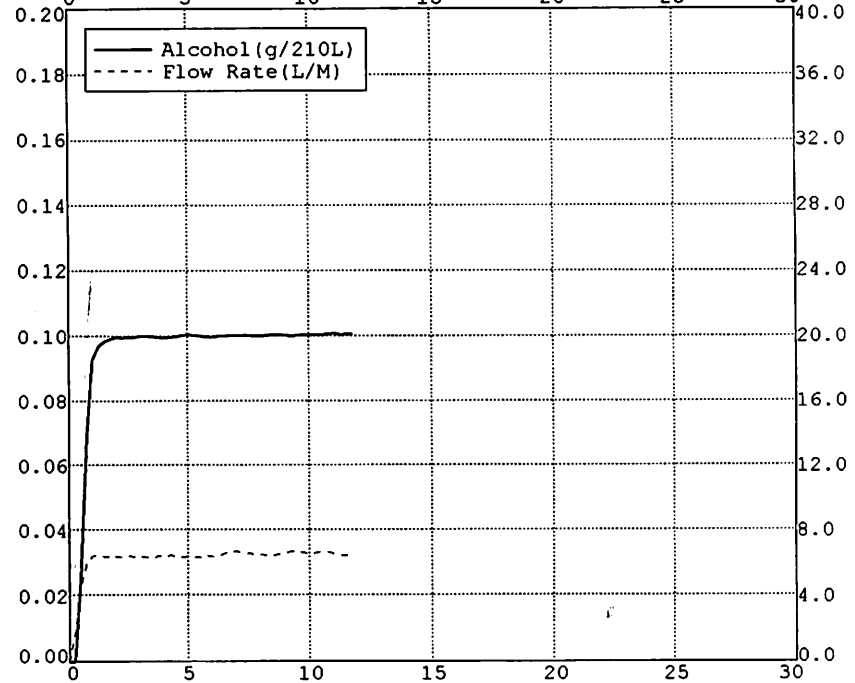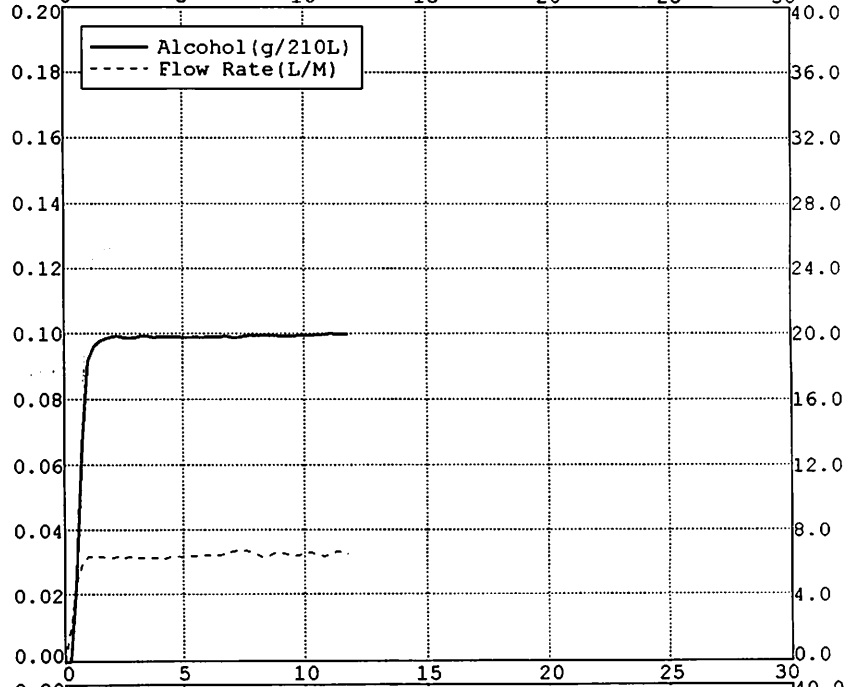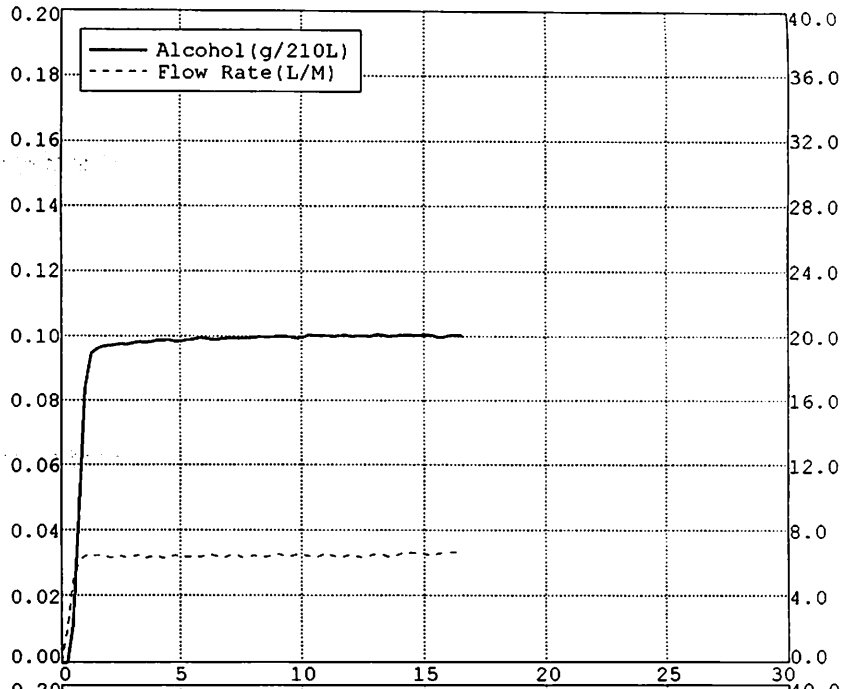

SUPERVISOR TEST


ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 09/26/2019


OPERATOR NAME:
MICHAEL P BAKER
Permit #: 44230
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:25
INTERNAL STANDARD	VERIFIED	02:25
REFERENCE STANDARD TEMP	34.01C	

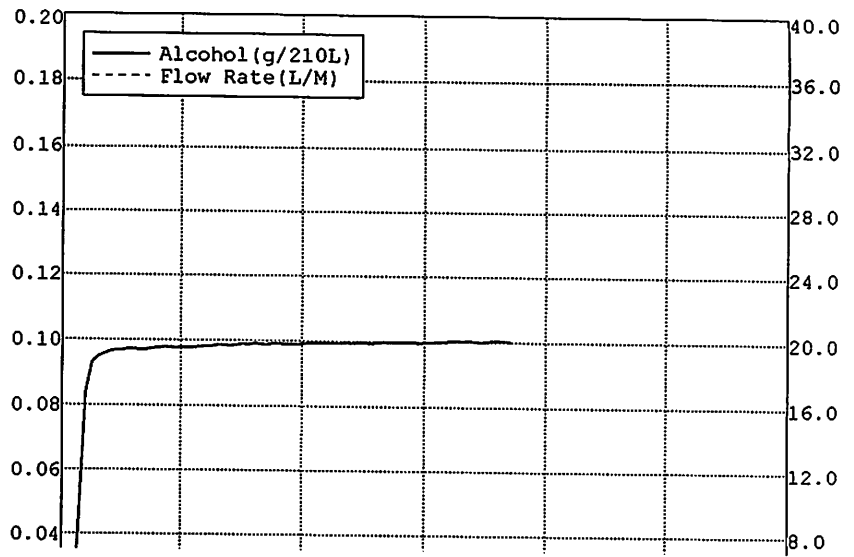

REFERENCE STANDARD	0.10	02:26
BLANK TEST	0.00	02:27
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:27
BLANK TEST	0.00	02:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:28
BLANK TEST	0.00	02:29

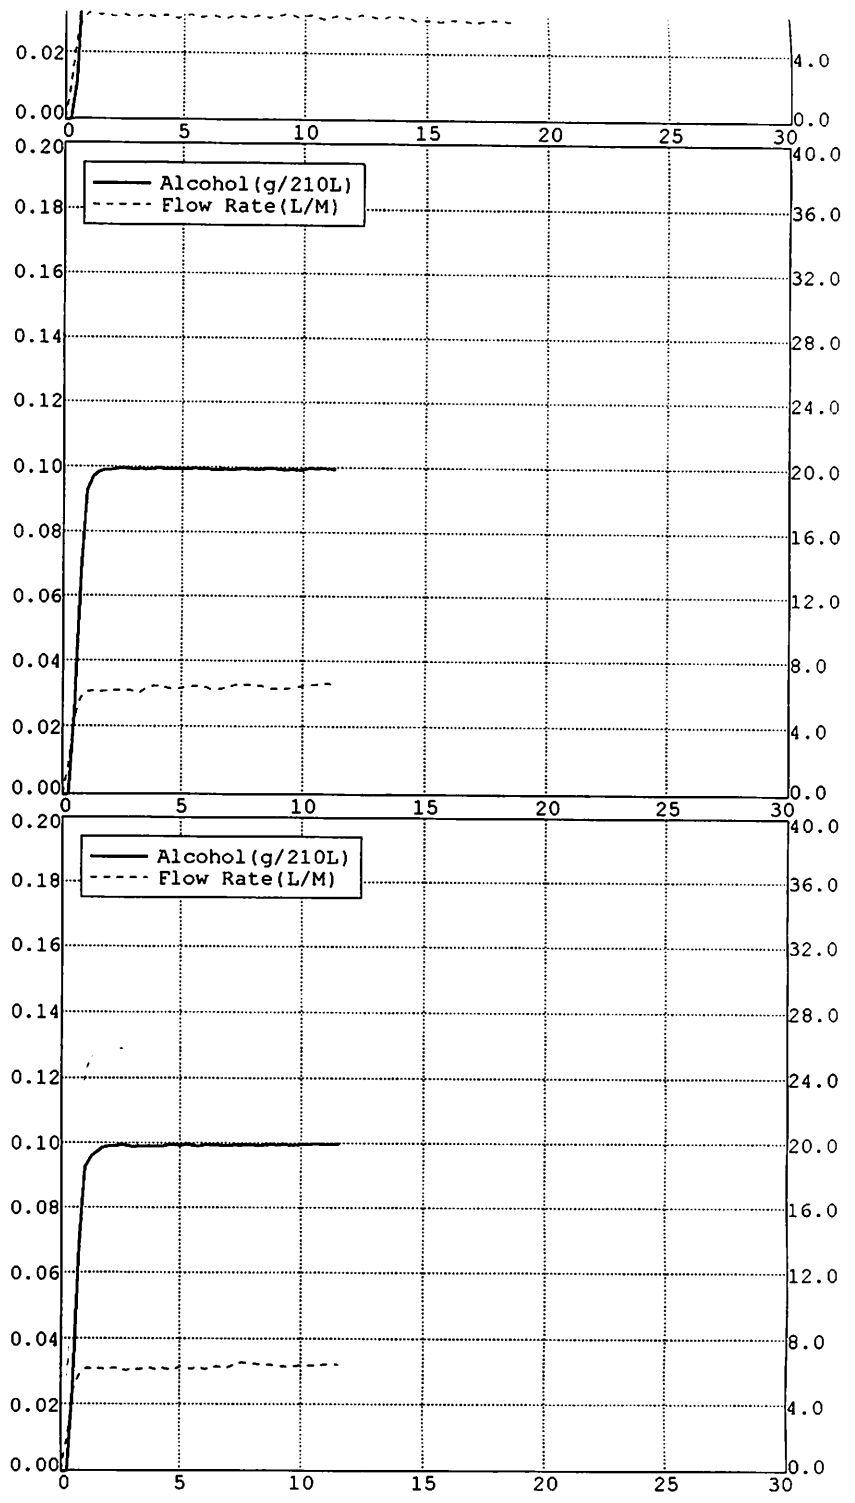

SOLUTION CHANGE

LEB




ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 10/08/2019

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:21
INTERNAL STANDARD	VERIFIED	18:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:22
BLANK TEST	0.00	18:23
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:23
BLANK TEST	0.00	18:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:24
BLANK TEST	0.00	18:25

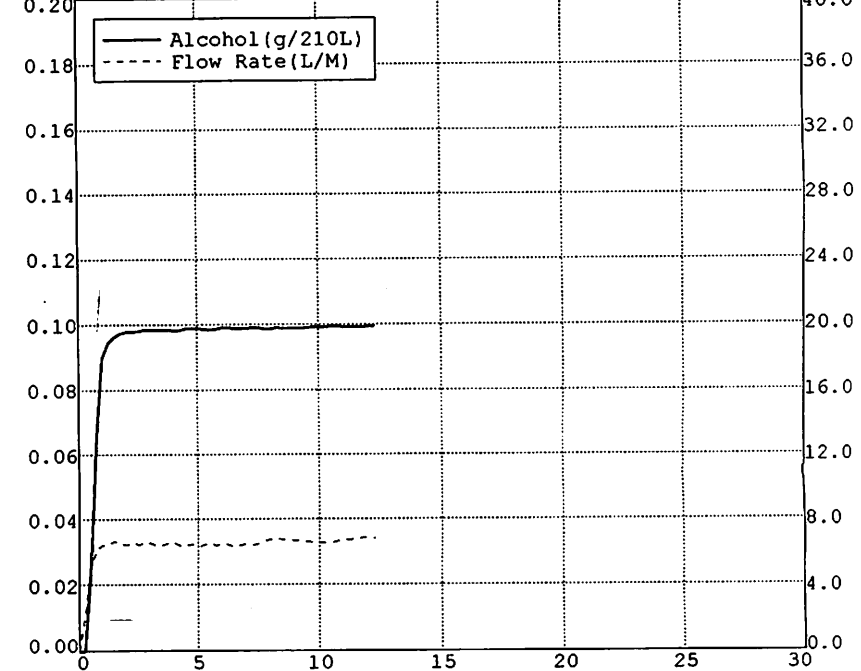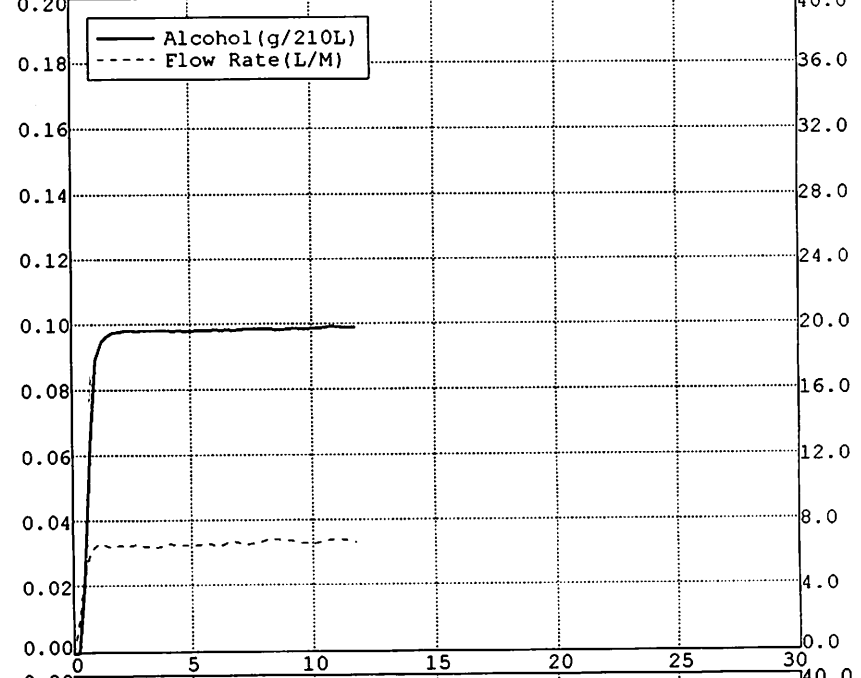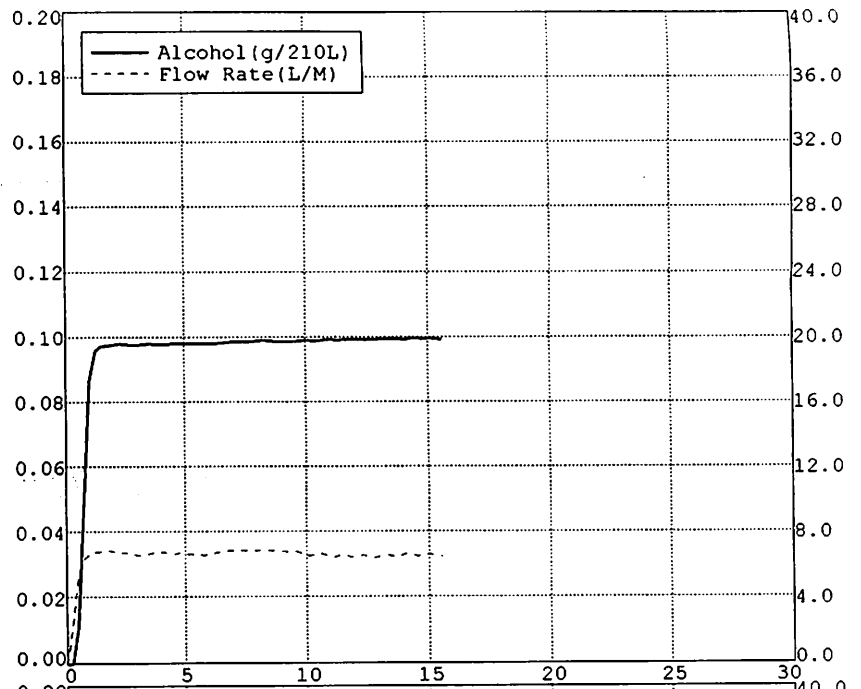

SUPERVISOR TEST

LEB

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 10/16/2019




OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:27
INTERNAL STANDARD	VERIFIED	18:27
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:27
BLANK TEST	0.00	18:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:29
BLANK TEST	0.00	18:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:30
BLANK TEST	0.00	18:31

Operator Agency/Dept: ONEIDA CO. SO

		18:27
		18:27
		18:27
		18:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:29

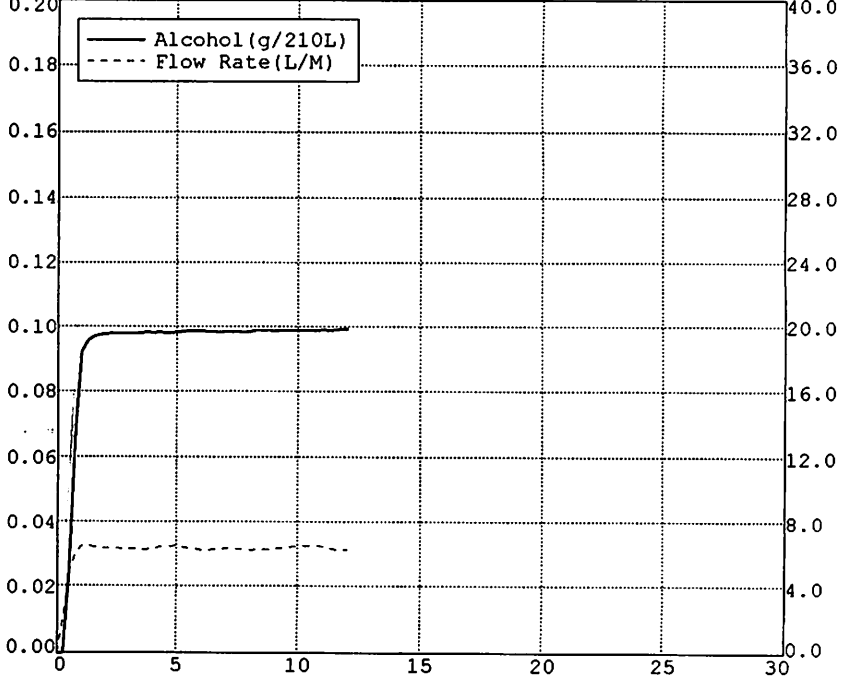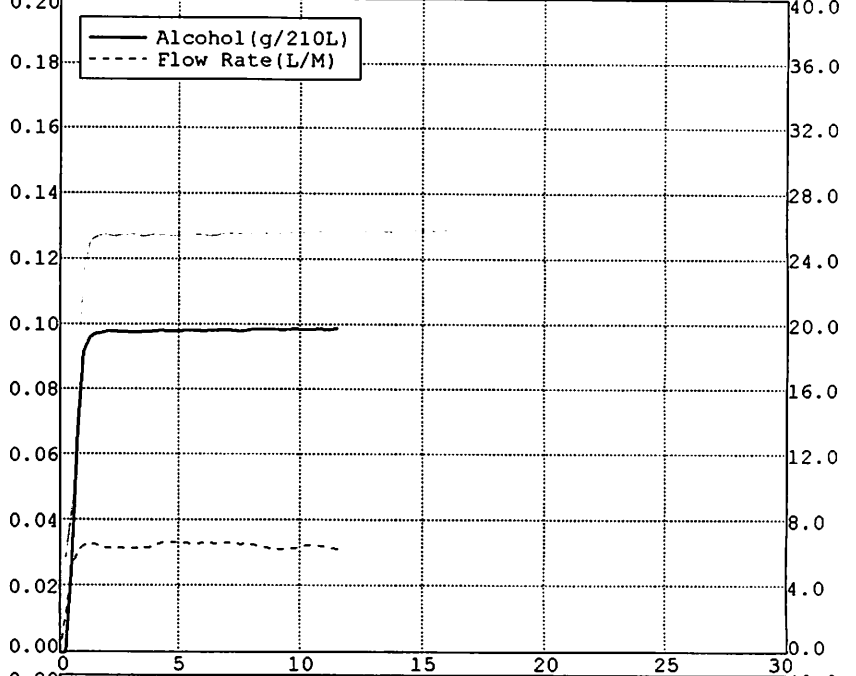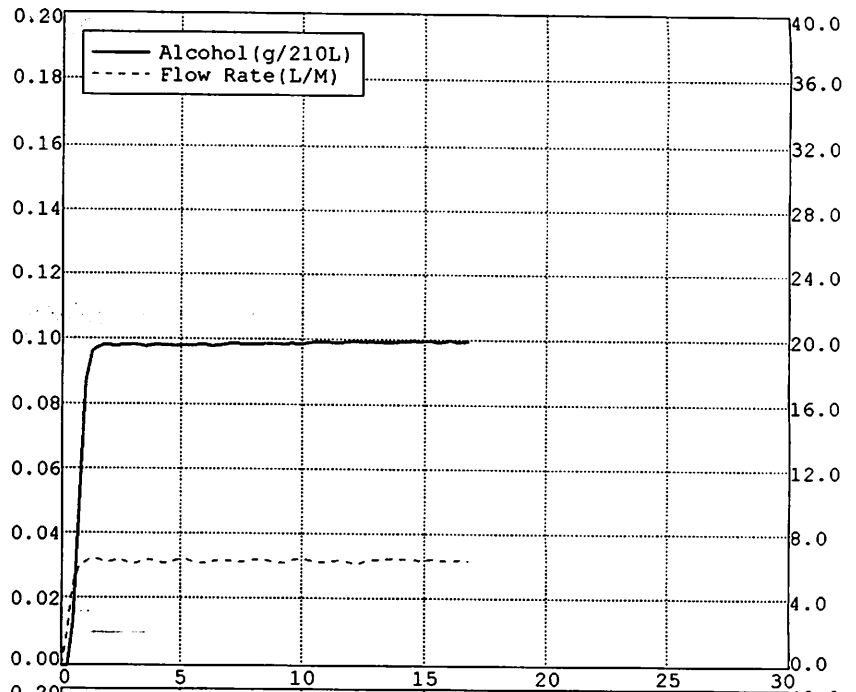

SUPERVISOR TEST

LATIC

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

LEB
(Bottle change)
Same bt #

Date: 11/01/2018

OPERATOR NAME:
EMRAH LATIC
Permit #: 46908
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:40
INTERNAL STANDARD	VERIFIED	18:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:41
BLANK TEST	0.00	18:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:42
BLANK TEST	0.00	18:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:43
BLANK TEST	0.00	18:44

ONEIDA CO. SO
Standard #: 19180

