

SOLUTION CHANGE

LEB




ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 10/08/2019

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:21
INTERNAL STANDARD	VERIFIED	18:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:22
BLANK TEST	0.00	18:23
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:23
BLANK TEST	0.00	18:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:24
BLANK TEST	0.00	18:25

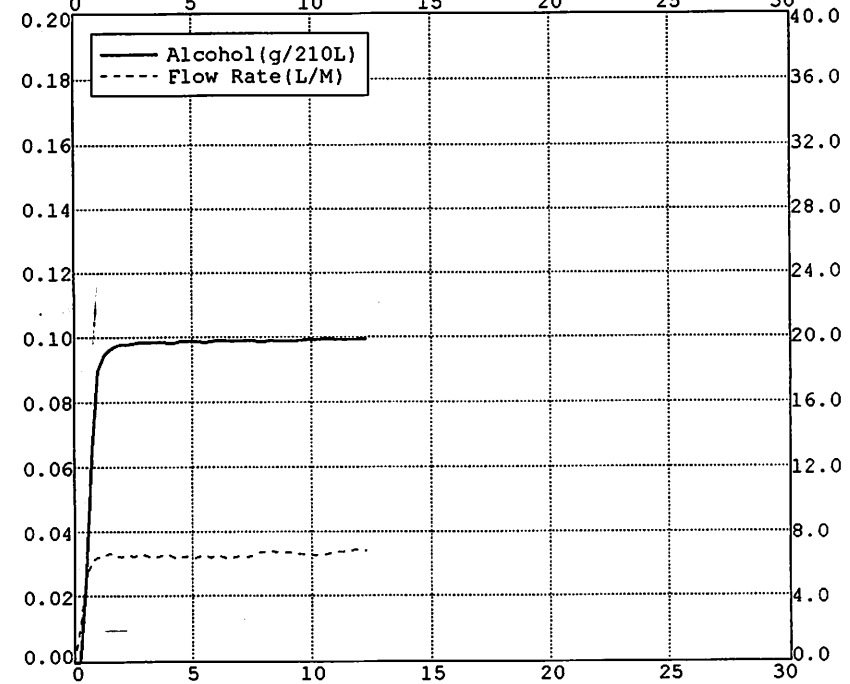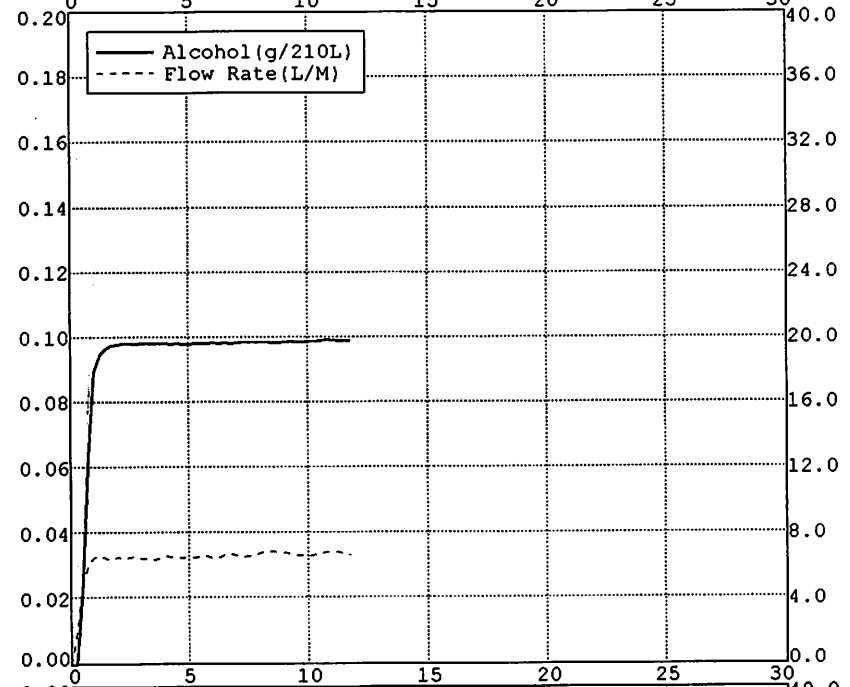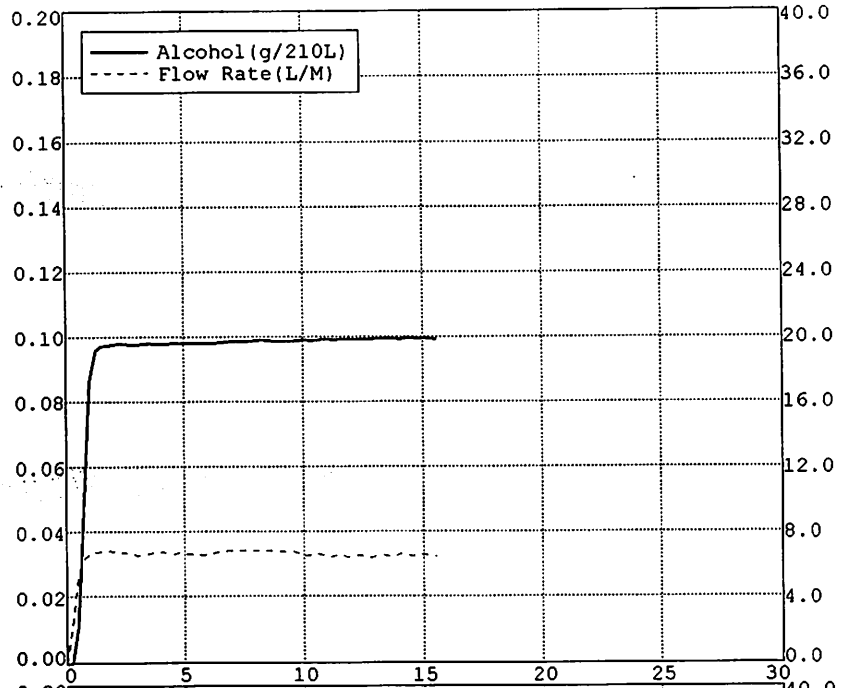

SUPERVISOR TEST

LEB

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606




Date: 10/16/2019

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:27
INTERNAL STANDARD	VERIFIED	18:27
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:27
BLANK TEST	0.00	18:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:29
BLANK TEST	0.00	18:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:30
BLANK TEST	0.00	18:31

Operator Agency/Dept: ONEIDA CO. SO

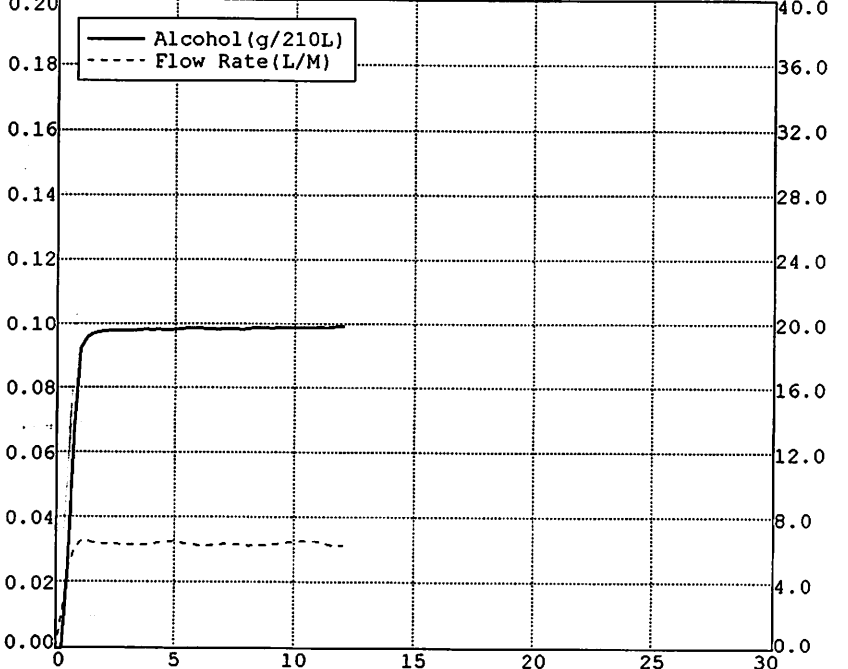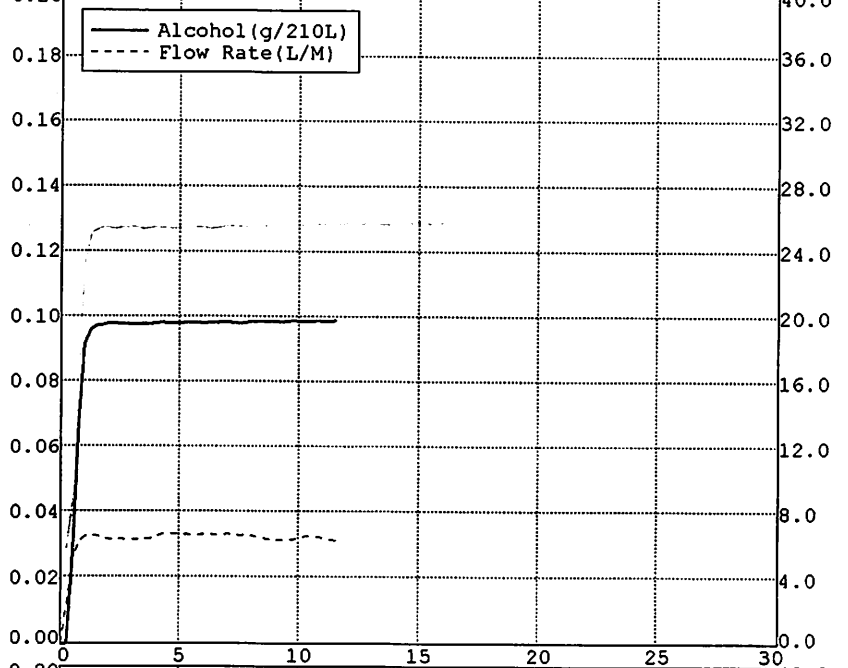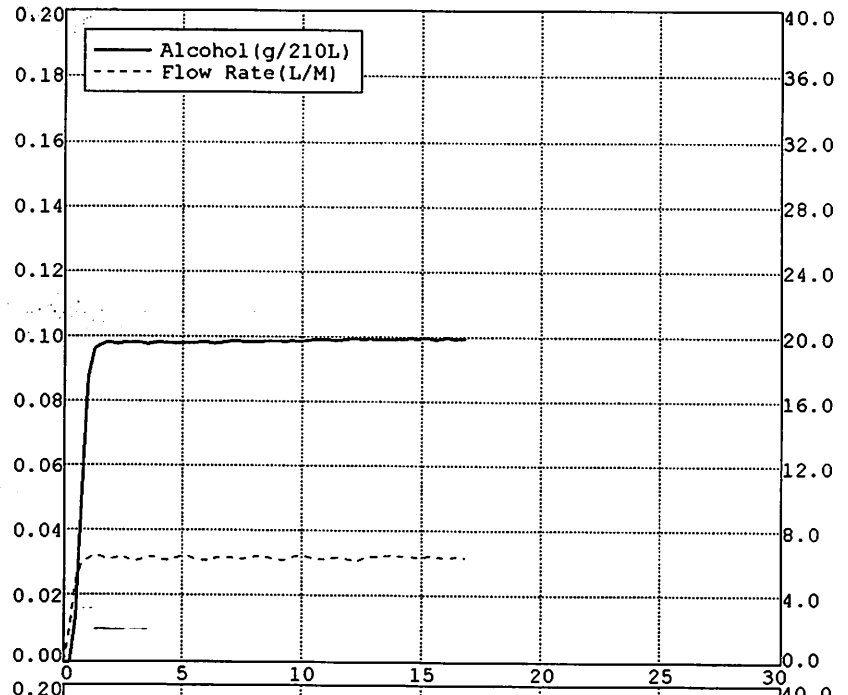

SUPERVISOR TEST

LATIC

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

LEB
(Bottle change
Save lot #)

Date: 11/01/2019




OPERATOR NAME:
EMRAH LATIC
Permit #: 46908
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:40
INTERNAL STANDARD	VERIFIED	18:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:41
BLANK TEST	0.00	18:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:42
BLANK TEST	0.00	18:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:43
BLANK TEST	0.00	18:44

ONEIDA CO. SO
Standard #: 19180

		18:40
		18:41
		18:42
REFERENCE STANDARD	0.09	18:42
BLANK TEST	0.00	18:43
REFERENCE STANDARD TEMP	34.01c	

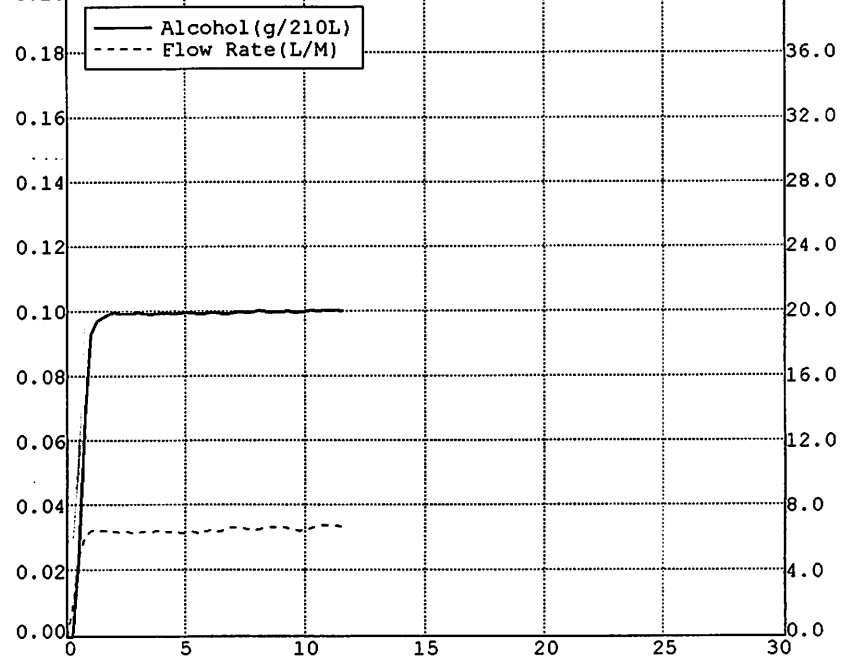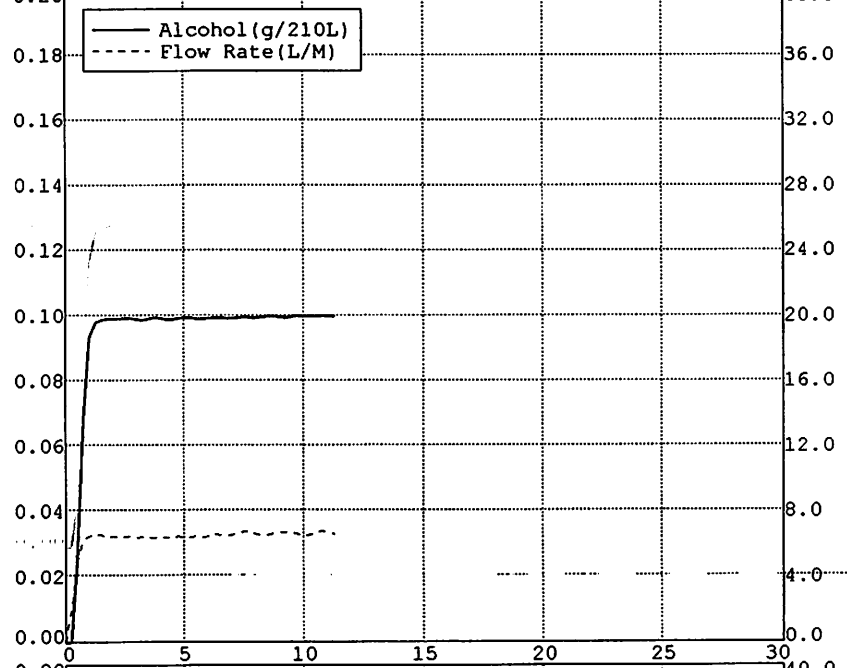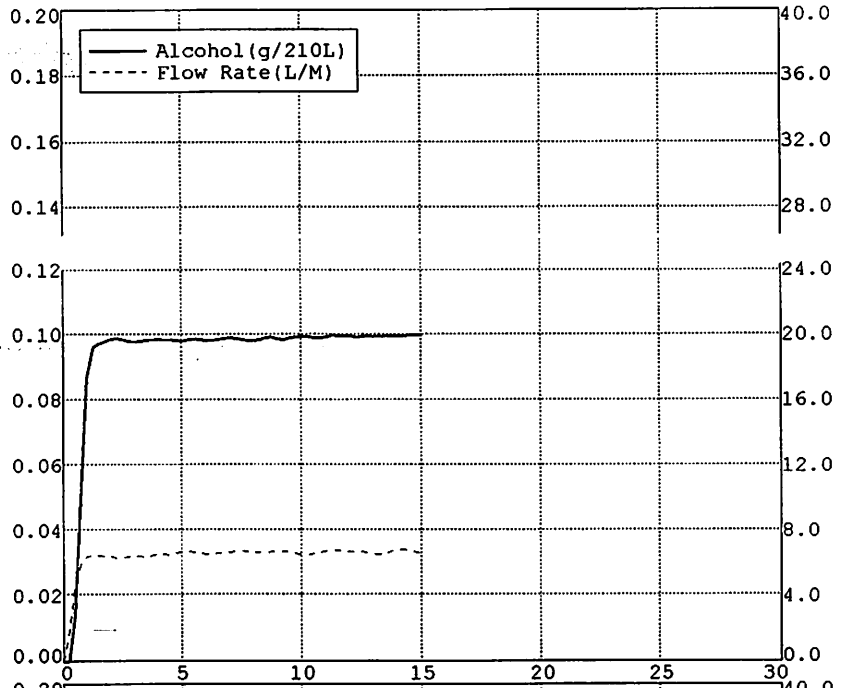

SUPERVISOR TEST




ONEIDA COUNTY
 SHERIFF'S OFFICE
 DATAMASTER dmt: 113606

Date: 11/07/2019

OPERATOR NAME:
 MICHAEL P BAKER
 Permit #: 44230
 Operator Agency/Dept: ONEIDA CO. SO
 Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:25
INTERNAL STANDARD	VERIFIED	00:25
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:26
BLANK TEST	0.00	00:27
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:27
BLANK TEST	0.00	00:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:28
BLANK TEST	0.00	00:29

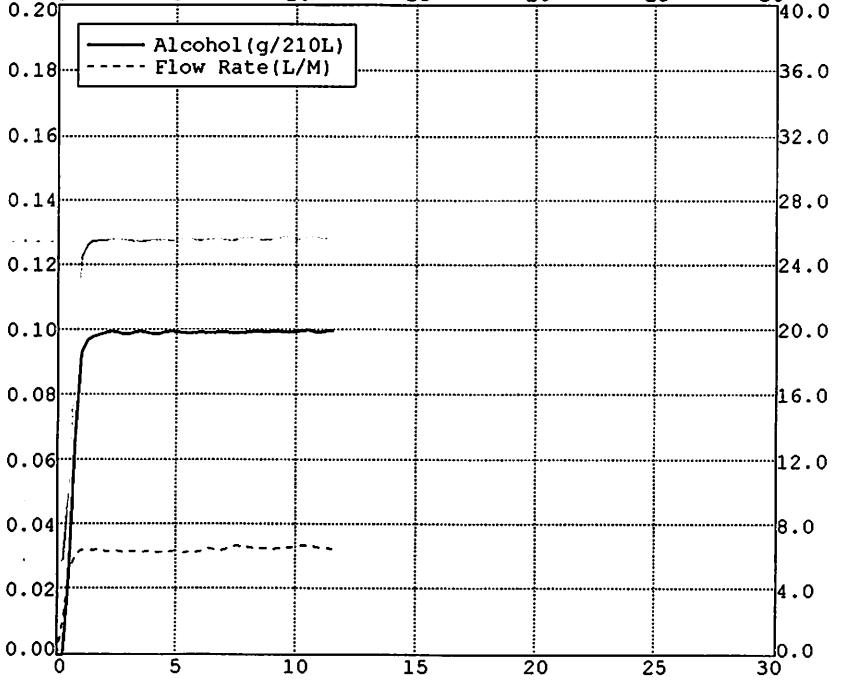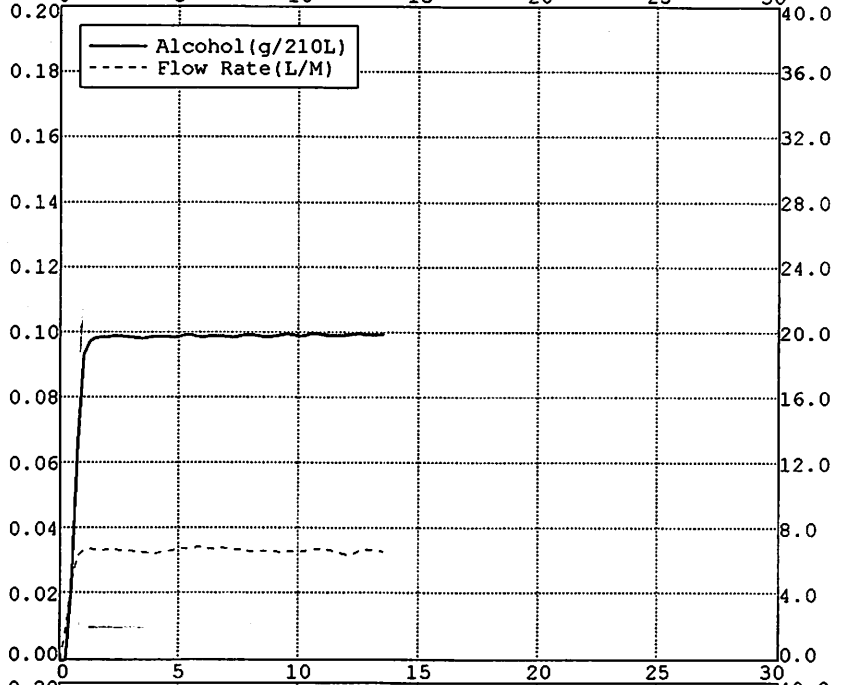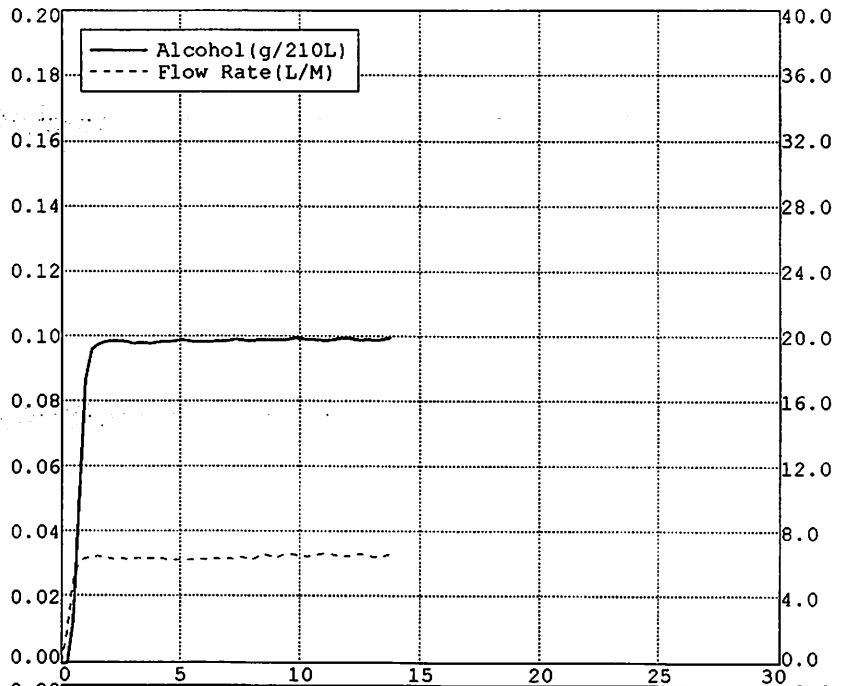

SUPERVISOR TEST

LEB

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 11/13/2019

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19180




Nominal = 0.10 g/210L

BLANK TEST	0.00	18:15
INTERNAL STANDARD	VERIFIED	18:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:16
BLANK TEST	0.00	18:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:17
BLANK TEST	0.00	18:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:18
BLANK TEST	0.00	18:19

OPERATOR NAME:
BRETT A GRABELDINGER

		18:15
	VERIFIED	18:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:16
BLANK TEST	0.00	18:17
		18:18
		18:19

aç|†⊕† -♦†ç-→ùG L^n⊙8!♥α

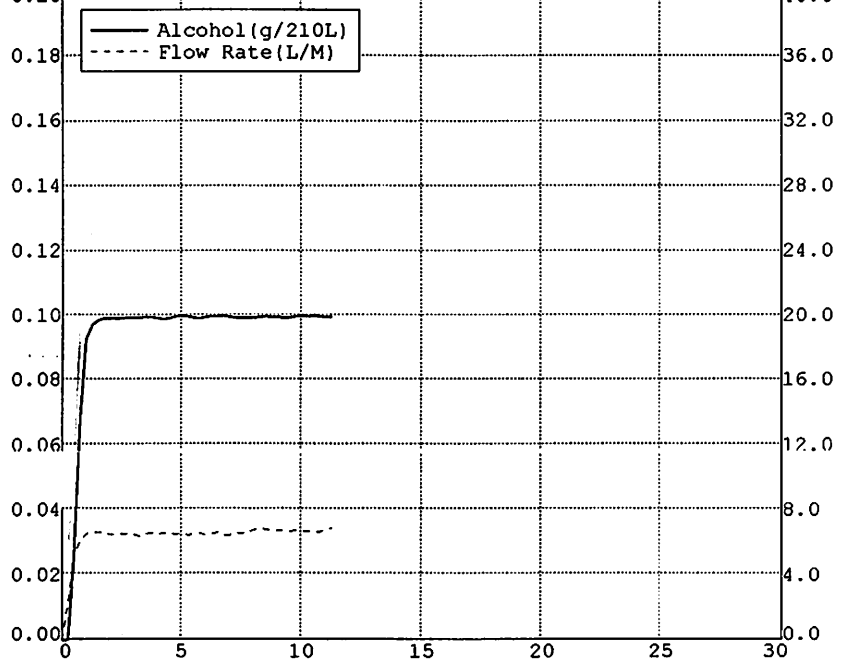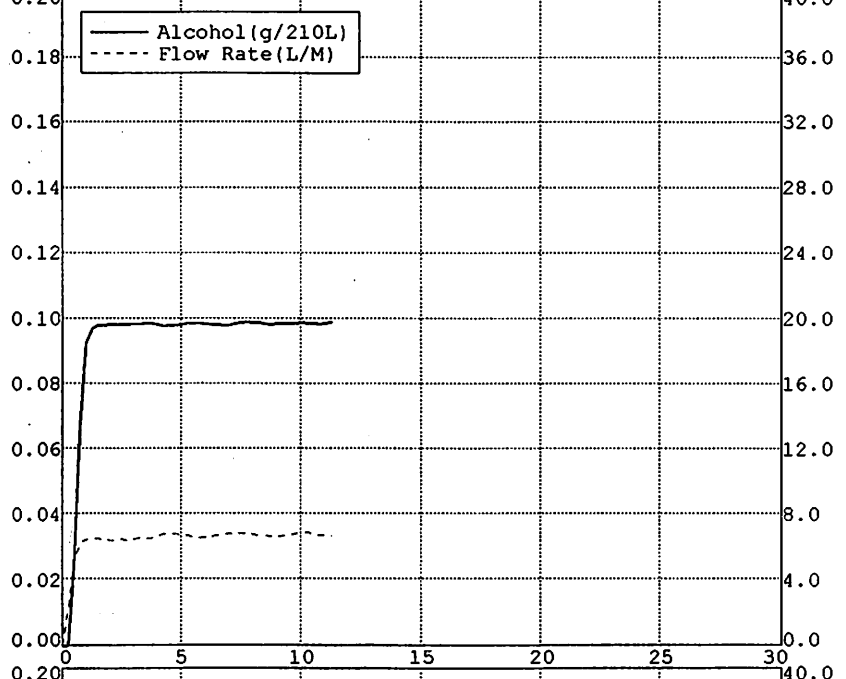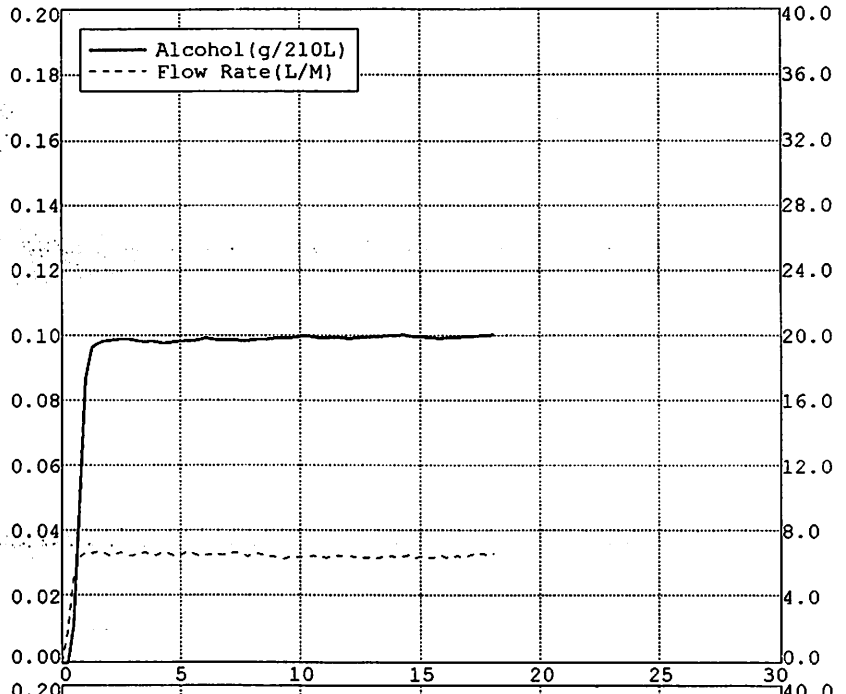

SUPERVISOR TEST

LATIC
LEB




ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 11/21/2019

OPERATOR NAME:
EMRAH LATIC
Permit #: 46908
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:23
INTERNAL STANDARD	VERIFIED	01:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:24
BLANK TEST	0.00	01:25
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:25
BLANK TEST	0.00	01:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:26
BLANK TEST	0.00	01:27

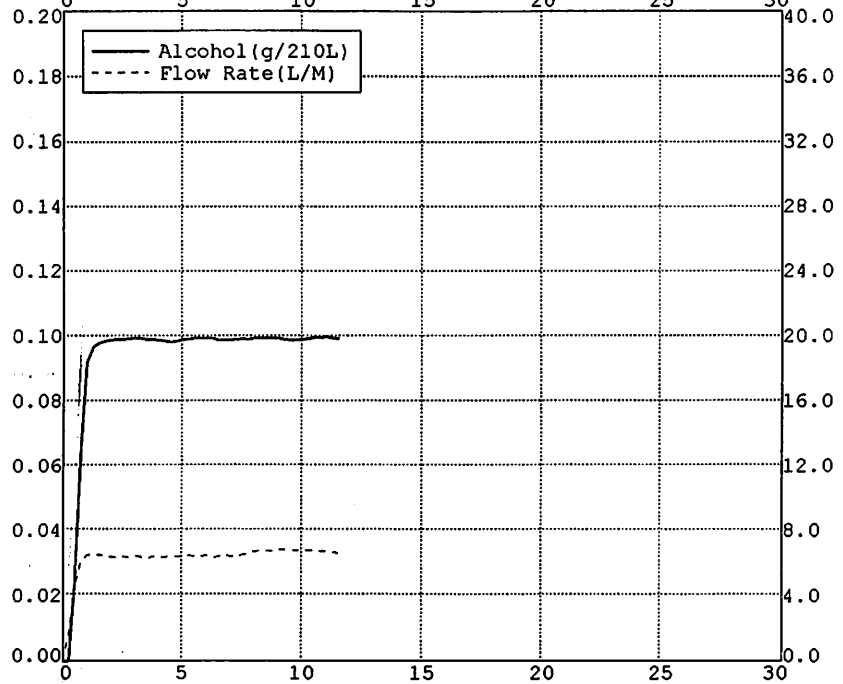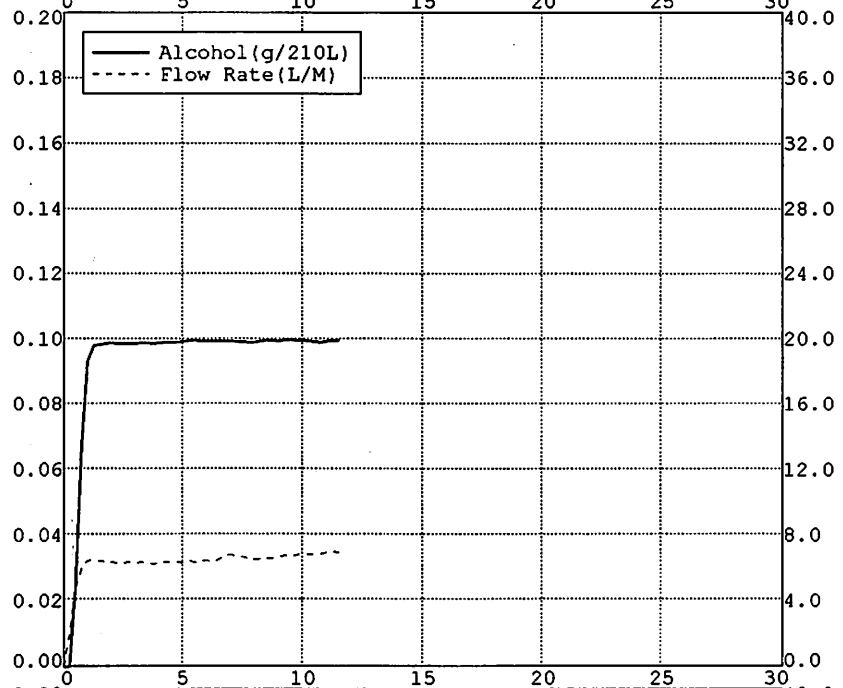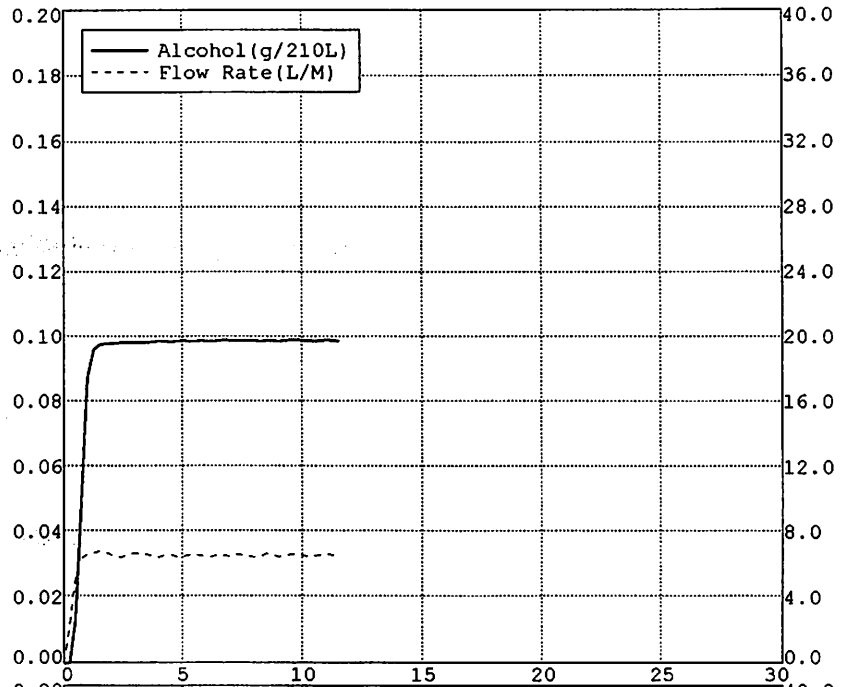

SUPERVISOR TEST

LEB




ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 11/27/2019

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:18
INTERNAL STANDARD	VERIFIED	18:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:18
BLANK TEST	0.00	18:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:20
BLANK TEST	0.00	18:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:21
BLANK TEST	0.00	18:22

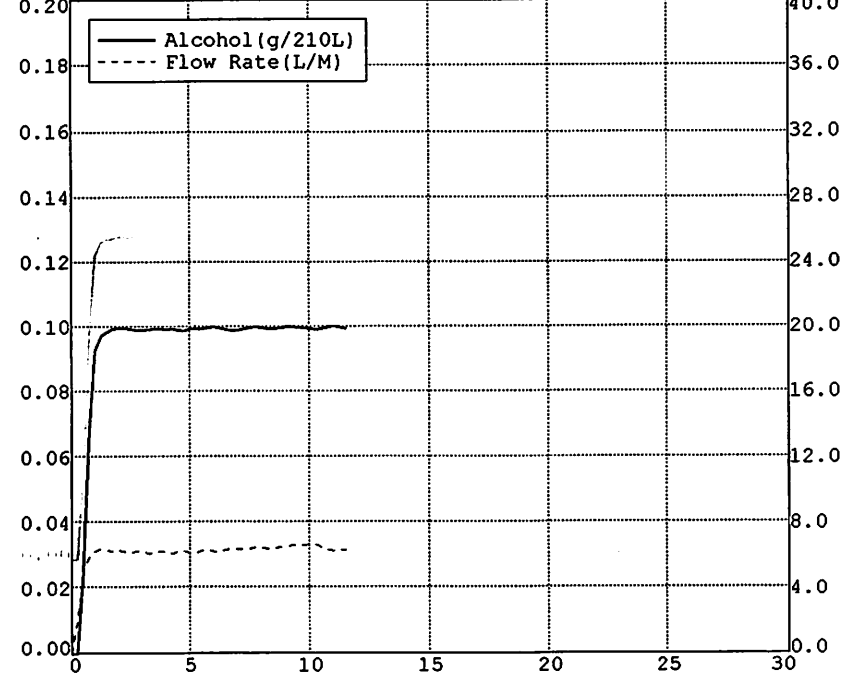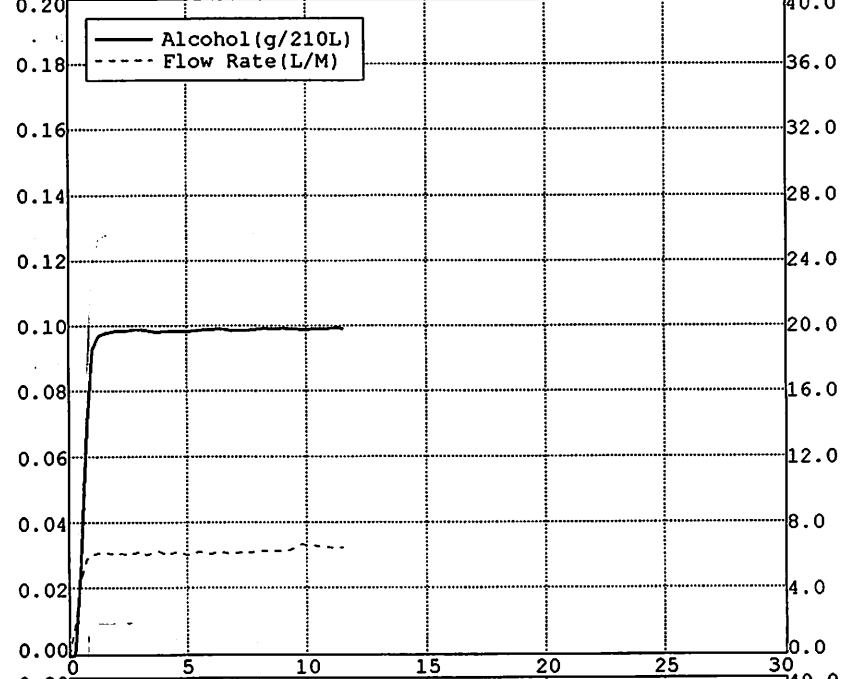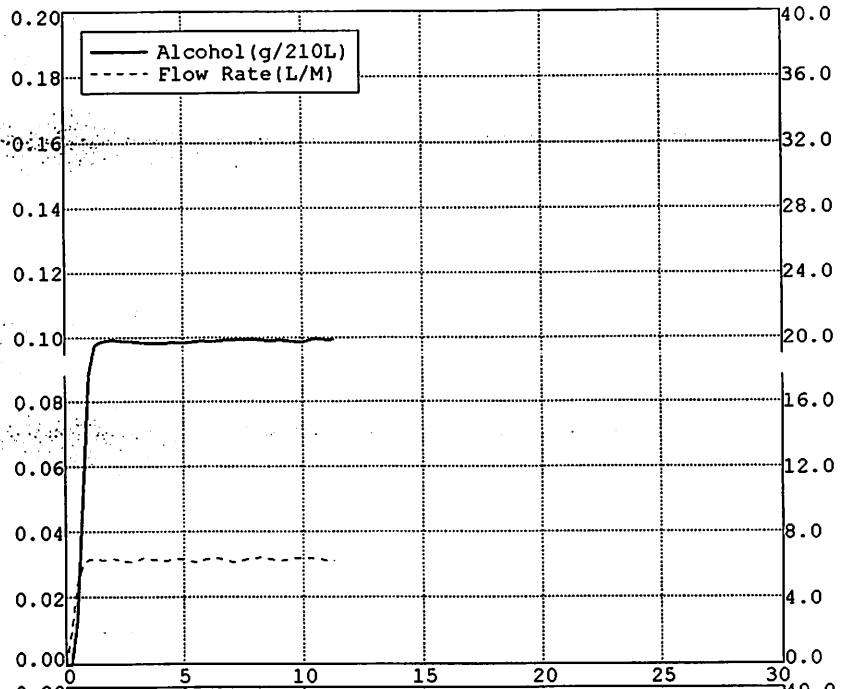

ONEIDA CO. SO

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:18
INTERNAL STANDARD	VERIFIED	18:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:18
BLANK TEST	0.00	18:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:20
BLANK TEST	0.00	18:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:21
BLANK TEST	0.00	18:22

SOLUTION CHANGE

LEB

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 12/02/2019

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19250




Nominal = 0.10 g/210L

BLANK TEST	0.00	22:40
INTERNAL STANDARD	VERIFIED	22:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	22:41
BLANK TEST	0.00	22:41
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	22:42
BLANK TEST	0.00	22:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	22:43
BLANK TEST	0.00	22:44

C#.

NAME:
GRABELDINGER

		22:40
INTERNAL STANDARD	VERIFIED	22:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	22:41
BLANK TEST	0.00	22:41
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	22:43
BLANK TEST	0.00	22:44

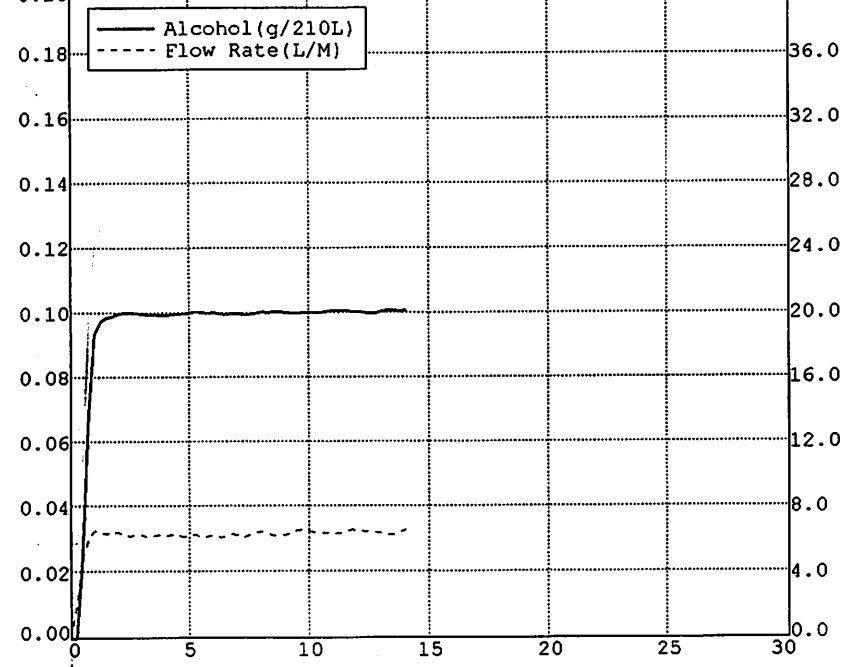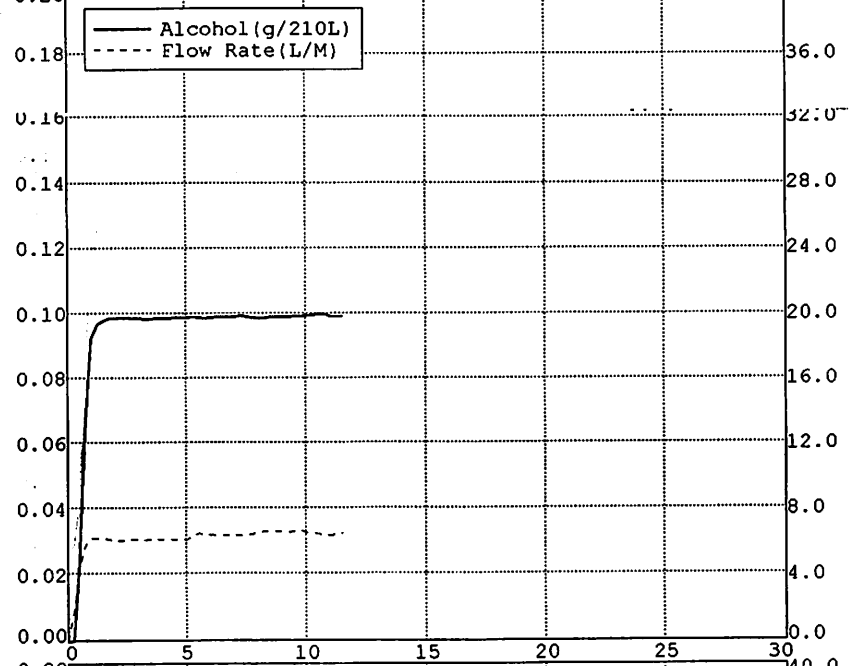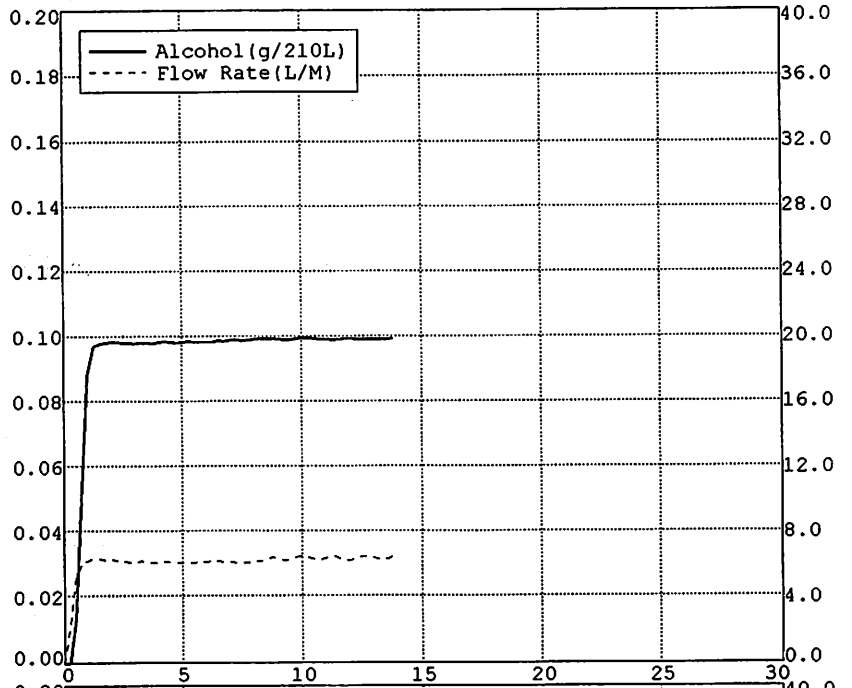

SUPERVISOR TEST




ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 12/05/2019

OPERATOR NAME:
EMRAH LATIC
Permit #: 46908
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:48
INTERNAL STANDARD	VERIFIED	01:48
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:48
BLANK TEST	0.00	01:49
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:49
BLANK TEST	0.00	01:50
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:50
BLANK TEST dmt: 113606	0.00	01:51

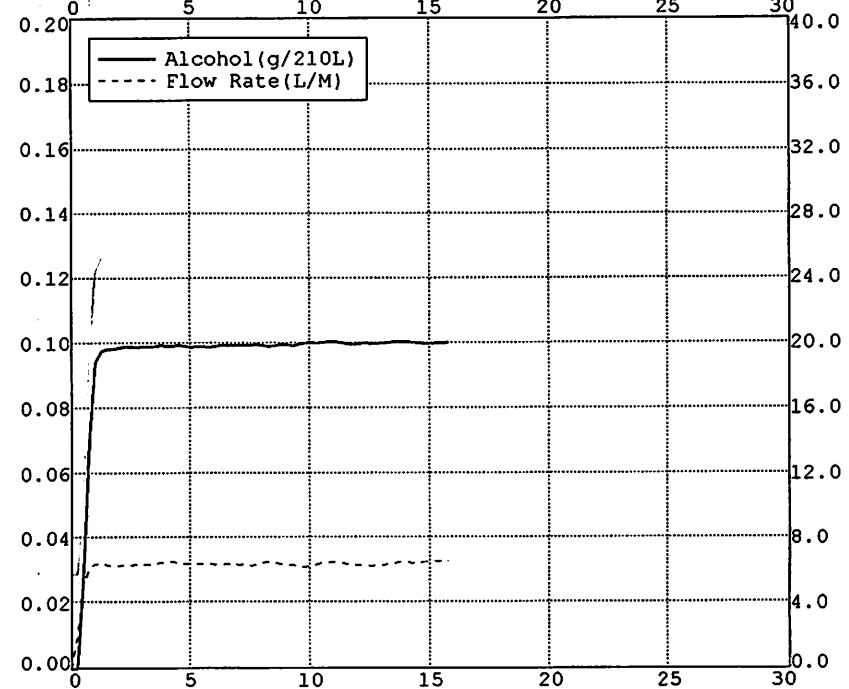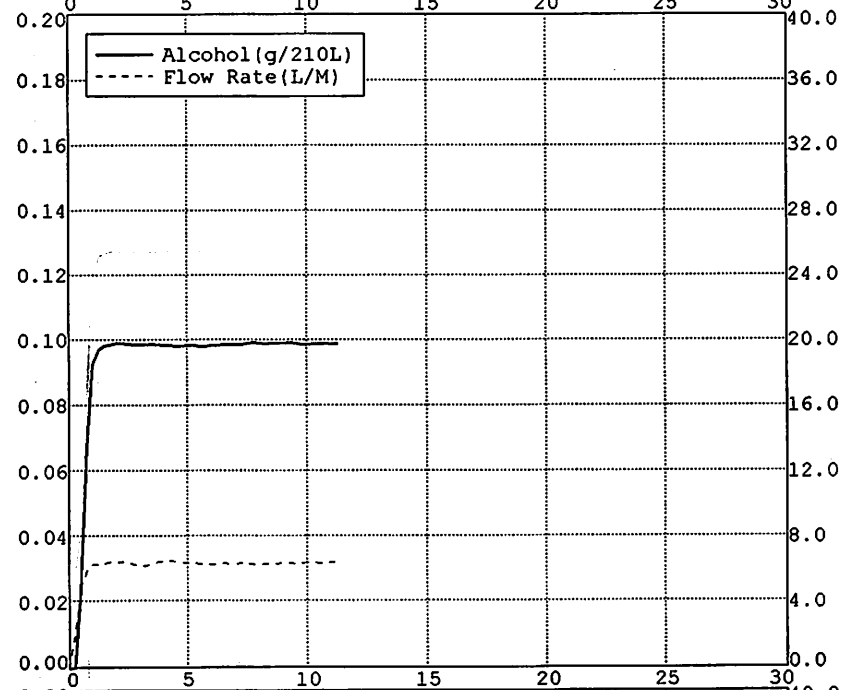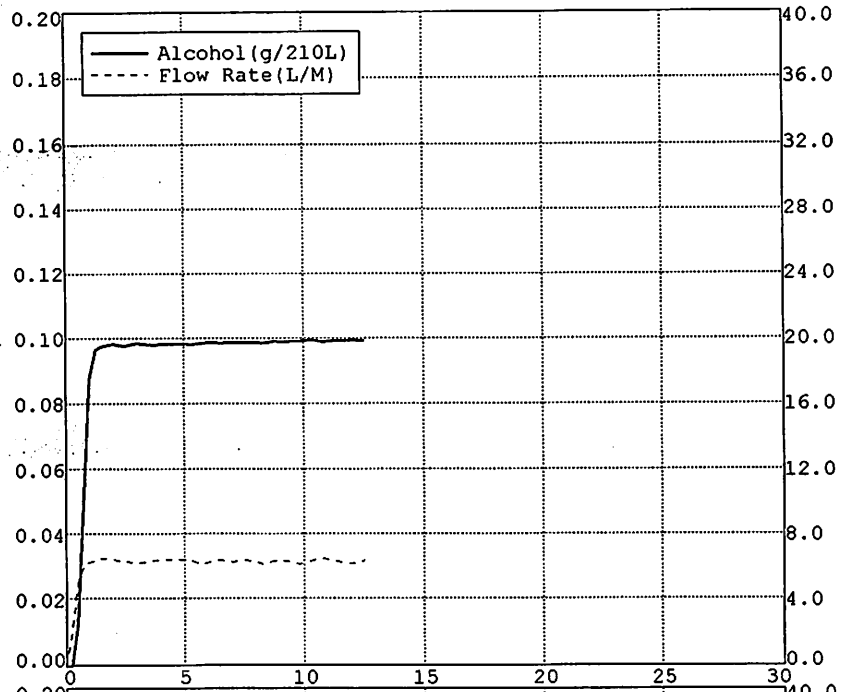

SUPERVISOR TEST

LEB




ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 12/11/2019

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:59
INTERNAL STANDARD	VERIFIED	17:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:00
BLANK TEST	0.00	18:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:01
BLANK TEST	0.00	18:02
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:02
BLANK TEST	0.00	18:03

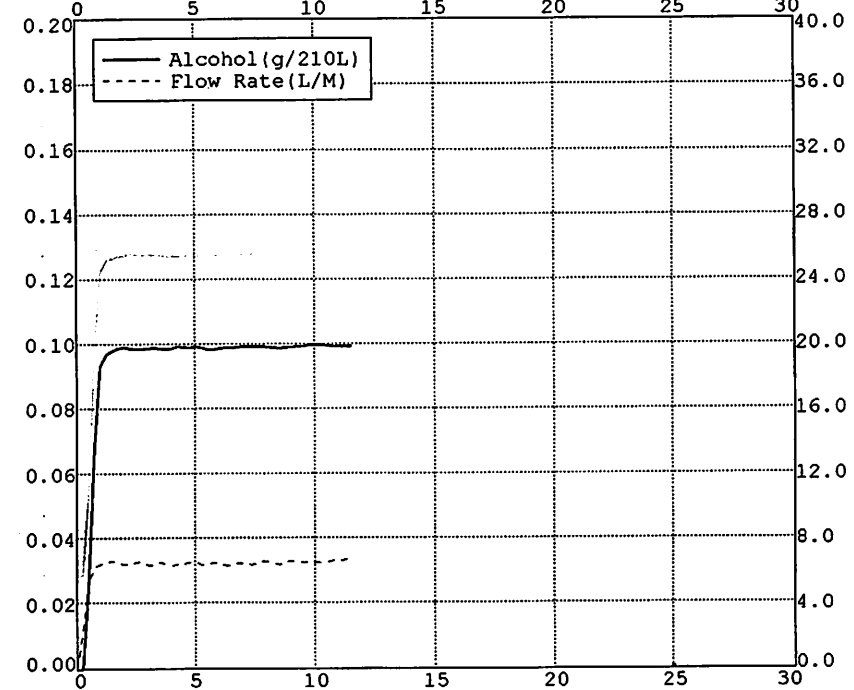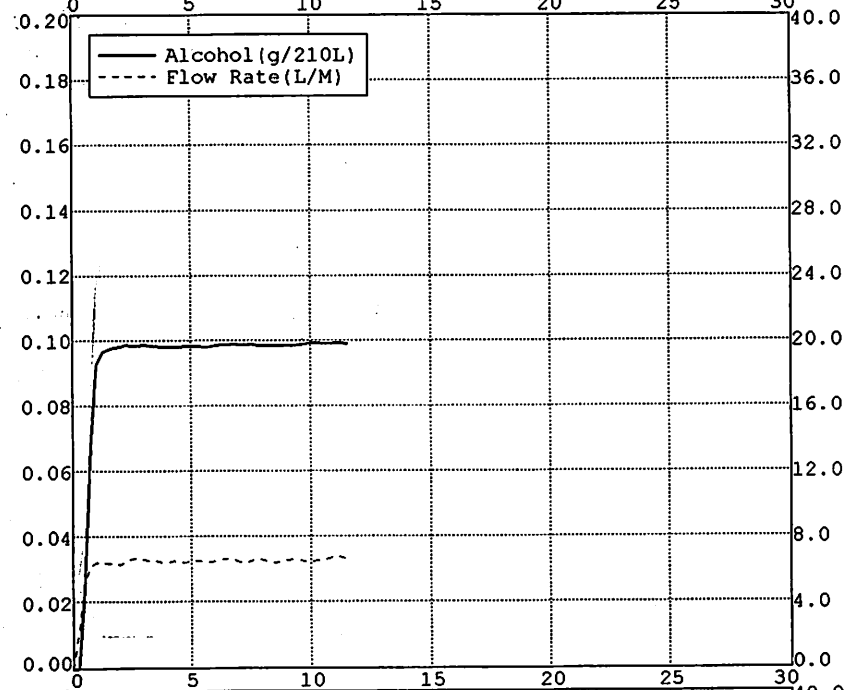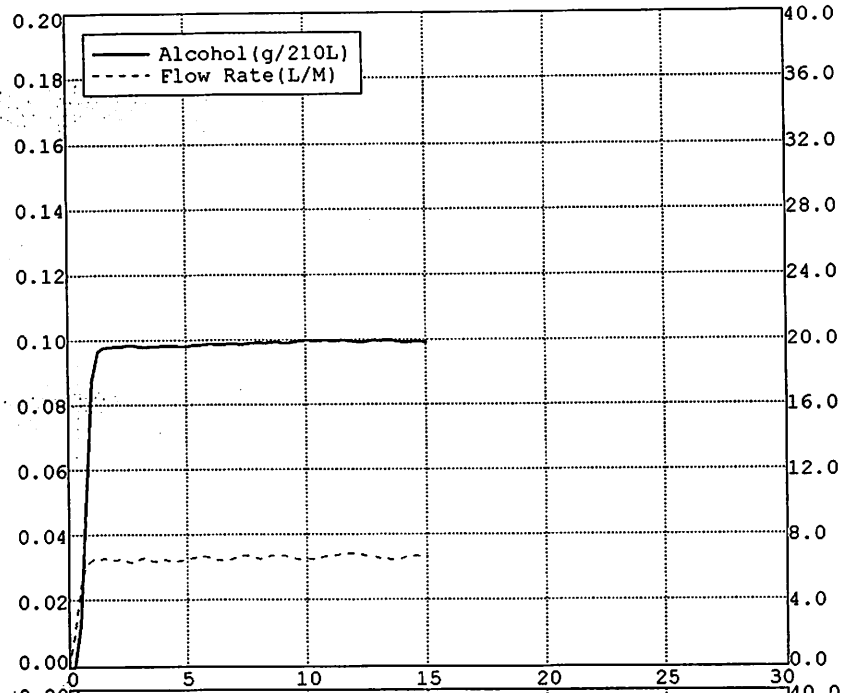

SUPERVISOR TEST

CEB
LATIC

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606




Date: 12/18/2019

OPERATOR NAME:
EMRAH LATIC
Permit #: 46908
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:58
INTERNAL STANDARD	VERIFIED	18:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:58
BLANK TEST	0.00	18:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:59
BLANK TEST	0.00	19:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	19:01
BLANK TEST	0.00	19:01

Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19250

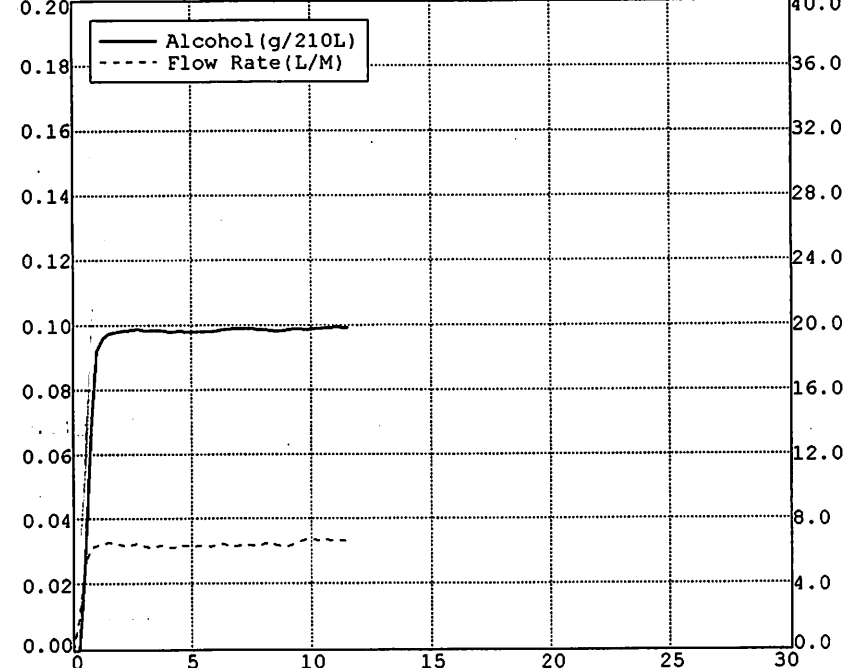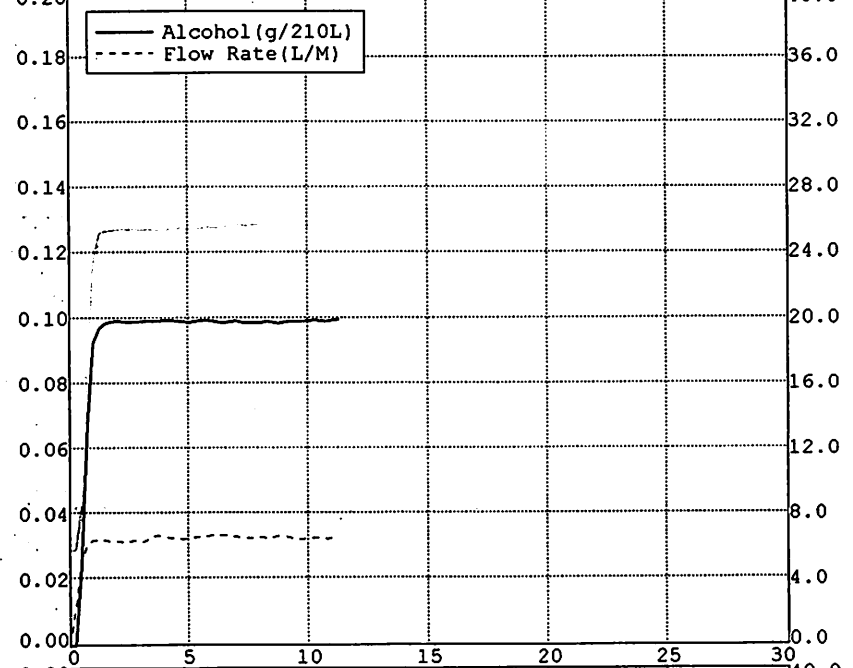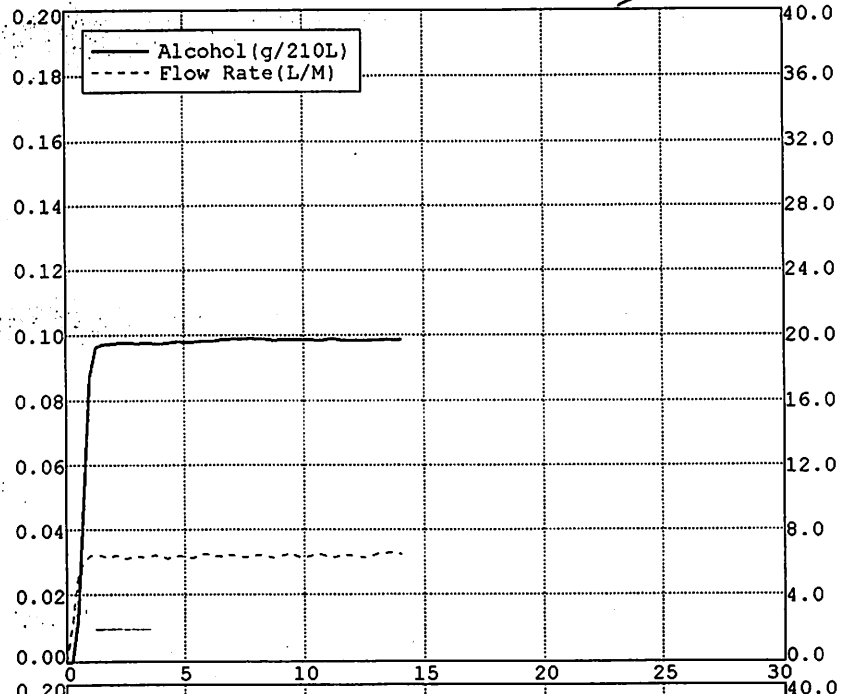

BLANK TEST	0.00	18:58
INTERNAL STANDARD	VERIFIED	18:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:58
BLANK TEST	0.00	18:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:59
BLANK TEST	0.00	19:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	19:01
BLANK TEST	0.00	19:01

SUPERVISOR TEST

LEB

ONEIDA COUNTY
 SHERIFF'S OFFICE
 DATAMASTER dmt: 113606

Date: 12/25/2019

OPERATOR NAME:
 BRETT A GRABELDINGER
 Permit #: 46896
 Operator Agency/Dept: ONEIDA CO. SO
 Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:55
INTERNAL STANDARD	VERIFIED	17:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:55
BLANK TEST	0.00	17:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:57
BLANK TEST	0.00	17:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:58
BLANK TEST	0.00	17:59

ONEIDA CO. SO
 Reference #: 19250

		17:55
		17:56
	0.09	17:57
	0.00	17:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:58

