

SUPERVISOR TEST

CFO




ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 12/25/2019

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19250

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 21:02 |
| INTERNAL STANDARD | VERIFIED | 21:02 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 21:02 |
| BLANK TEST | 0.00 | 21:03 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 21:03 |
| BLANK TEST | 0.00 | 21:04 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 21:05 |
| BLANK TEST | 0.00 | 21:06 |

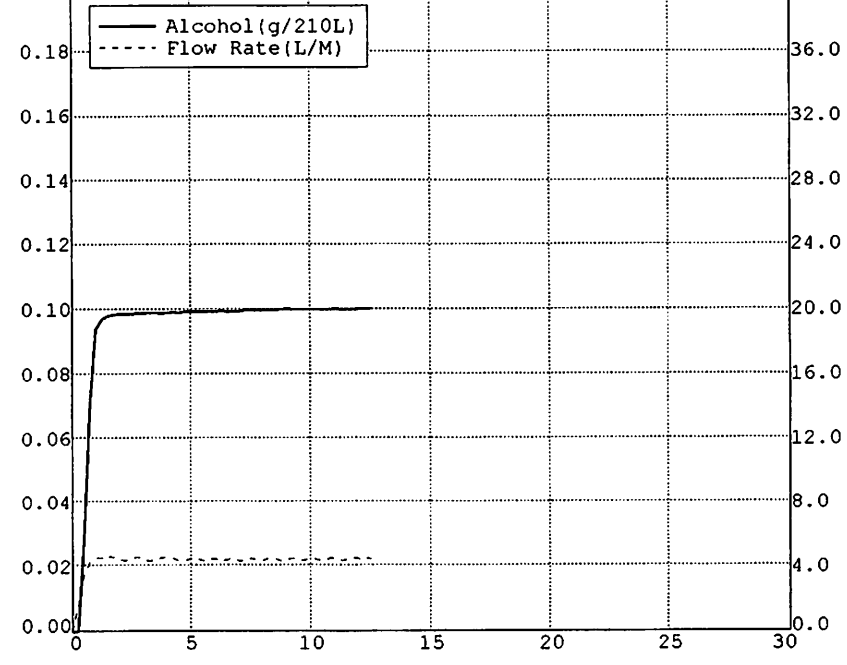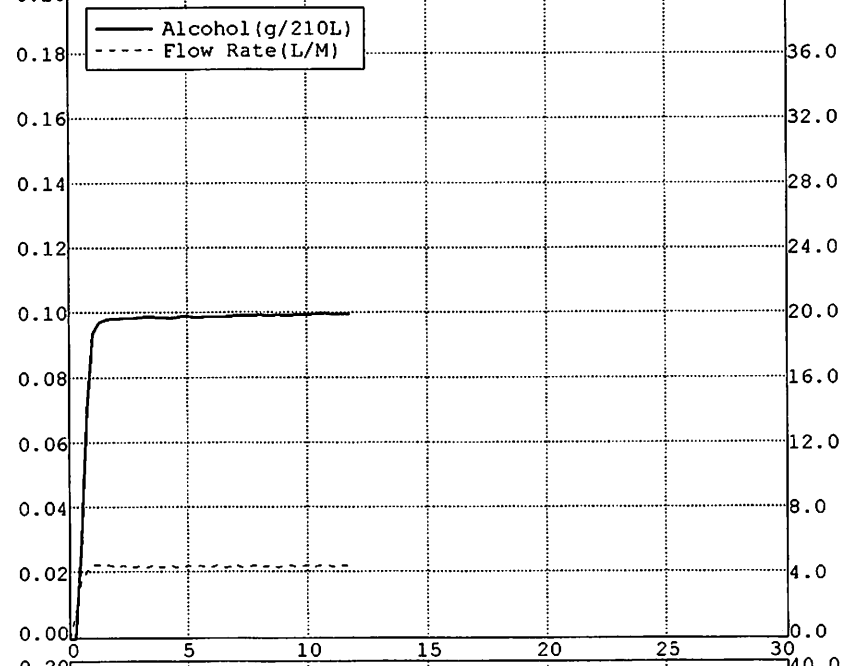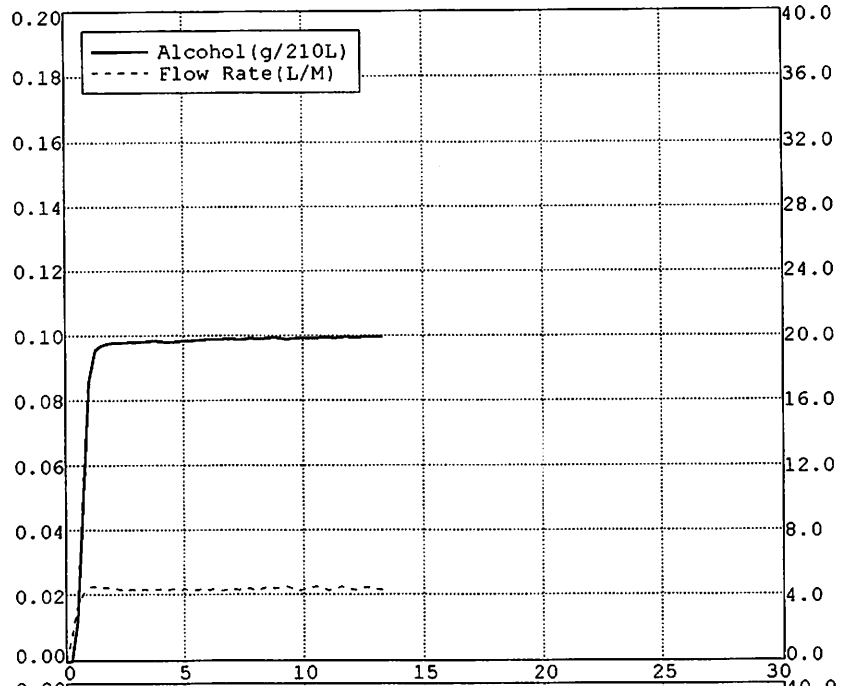

SUPERVISOR TEST

CFO




ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 01/05/2020

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19250

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 21:44 |
| INTERNAL STANDARD | VERIFIED | 21:44 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 21:44 |
| BLANK TEST | 0.00 | 21:45 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 21:46 |
| BLANK TEST | 0.00 | 21:47 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 21:47 |
| BLANK TEST | 0.00 | 21:48 |

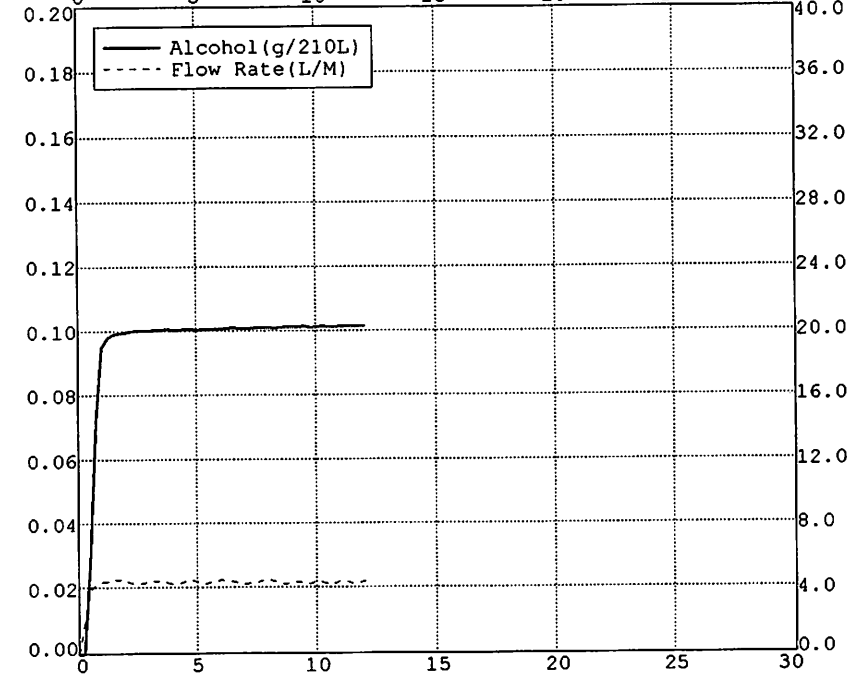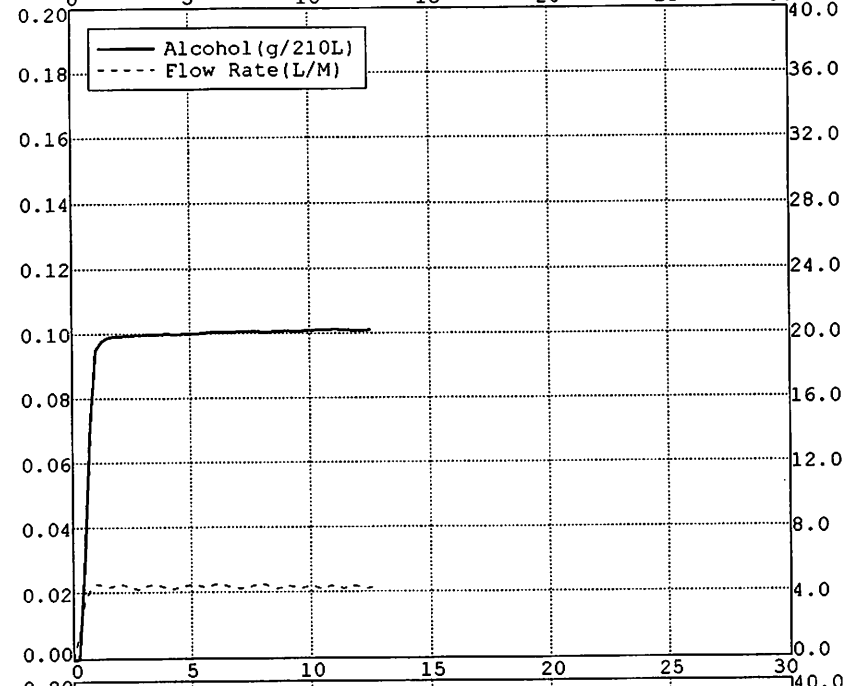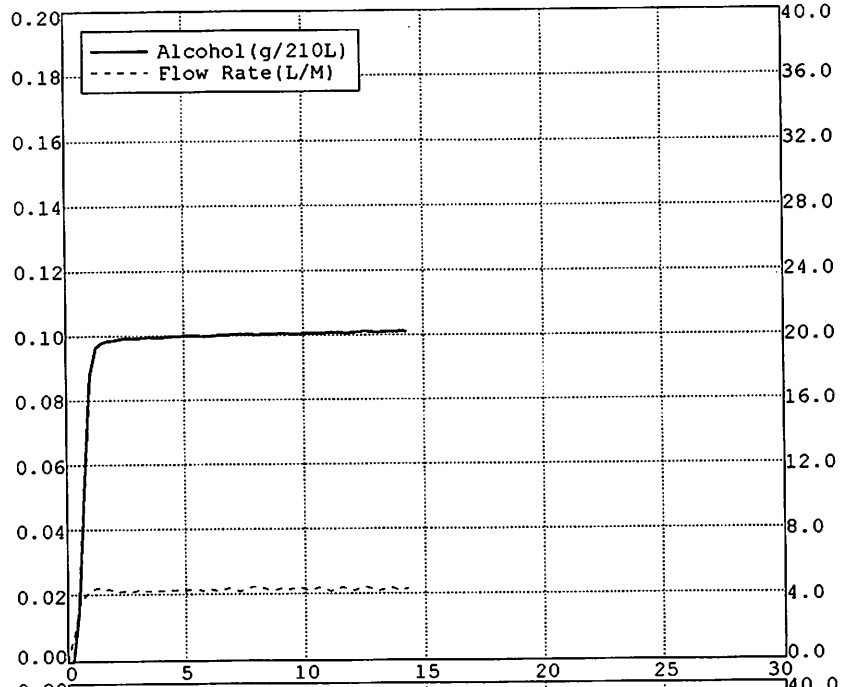

SUPERVISOR TEST

CF0

ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 01/08/2020

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 19250

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 21:17 |
| INTERNAL STANDARD | VERIFIED | 21:17 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 21:18 |
| BLANK TEST | 0.00 | 21:18 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 21:19 |
| BLANK TEST | 0.00 | 21:20 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 21:20 |
| BLANK TEST | 0.00 | 21:21 |

