

SOLUTION CHANGE




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

ate: 07/01/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:34
INTERNAL STANDARD	VERIFIED	15:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:34
BLANK TEST	0.00	15:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:35
BLANK TEST	0.00	15:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:37
BLANK TEST	0.00	15:37

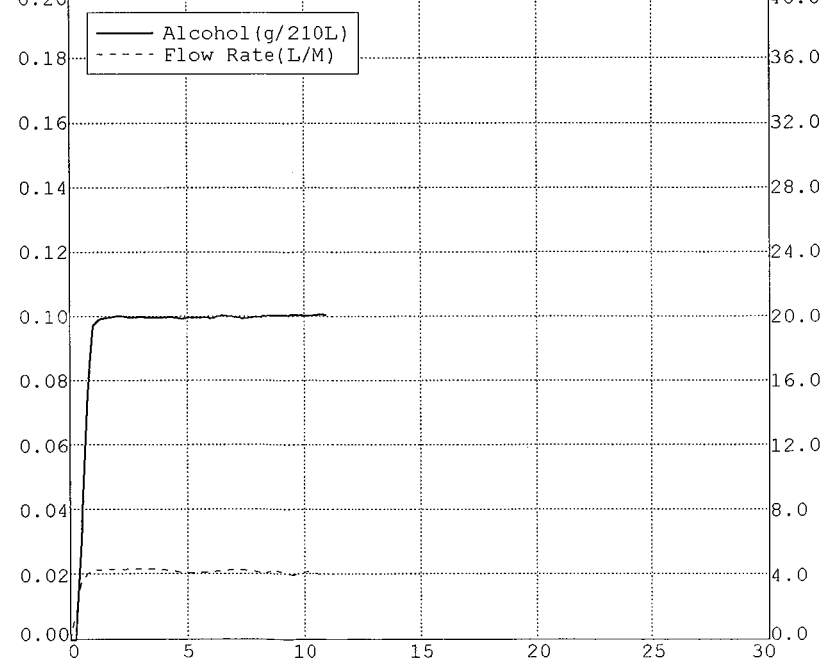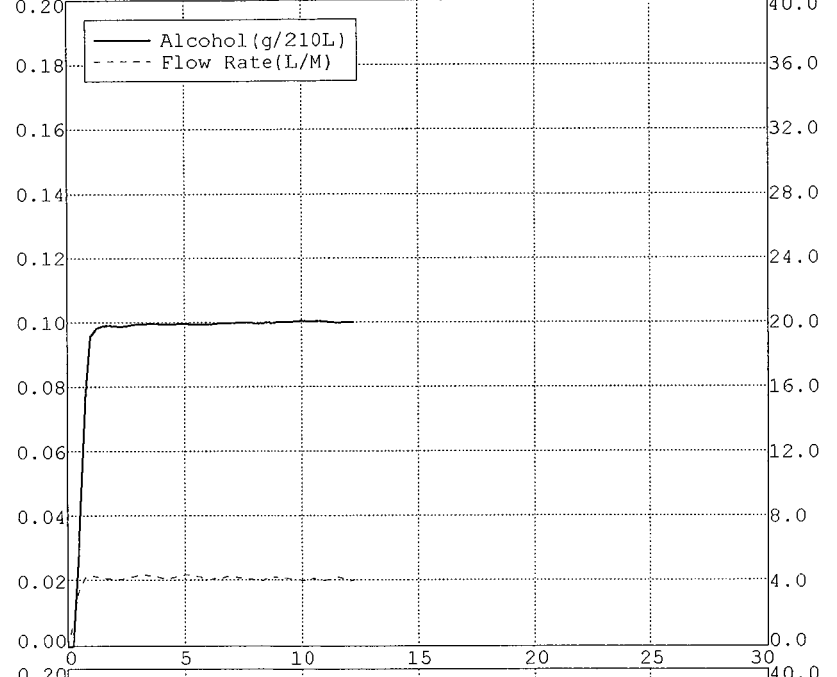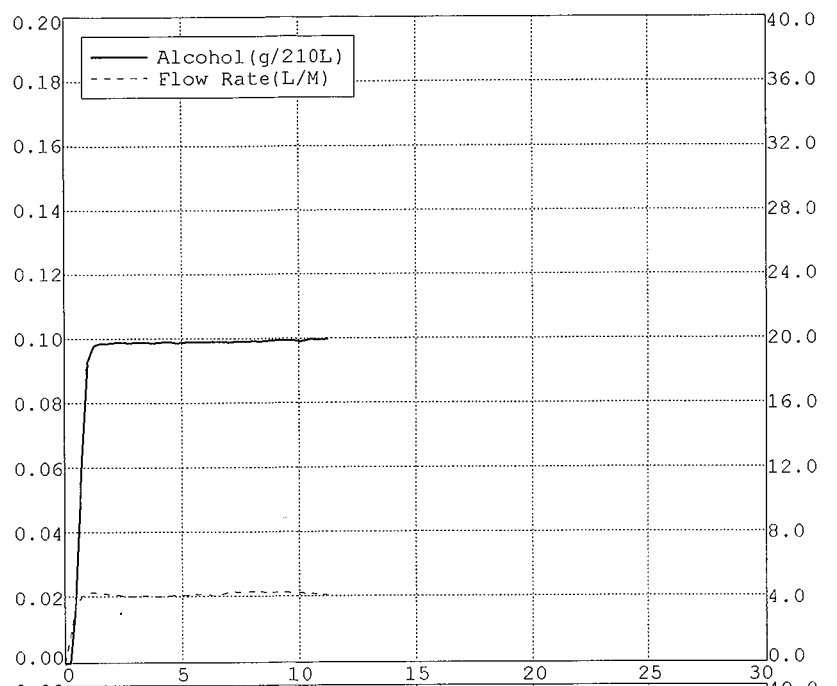

Hollie B Kennedy
Hollie B Kennedy 1085

SUPERVISOR TEST




ROME CITY
 POLICE DEPT
 DATAMASTER dmt: 106106

Date: 07/05/2019

OPERATOR NAME:
 HOLLIE B KENNEDY
 Permit #: 39044
 Operator Agency/Dept: ROME CITY PD
 Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:17
INTERNAL STANDARD	VERIFIED	15:17
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:18
BLANK TEST	0.00	15:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:19
BLANK TEST	0.00	15:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:20
BLANK TEST	0.00	15:21

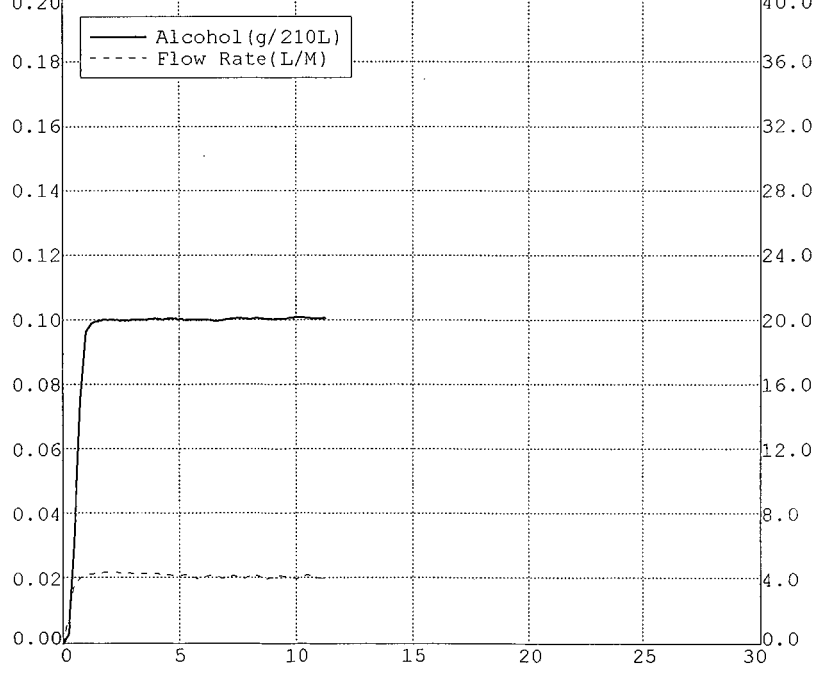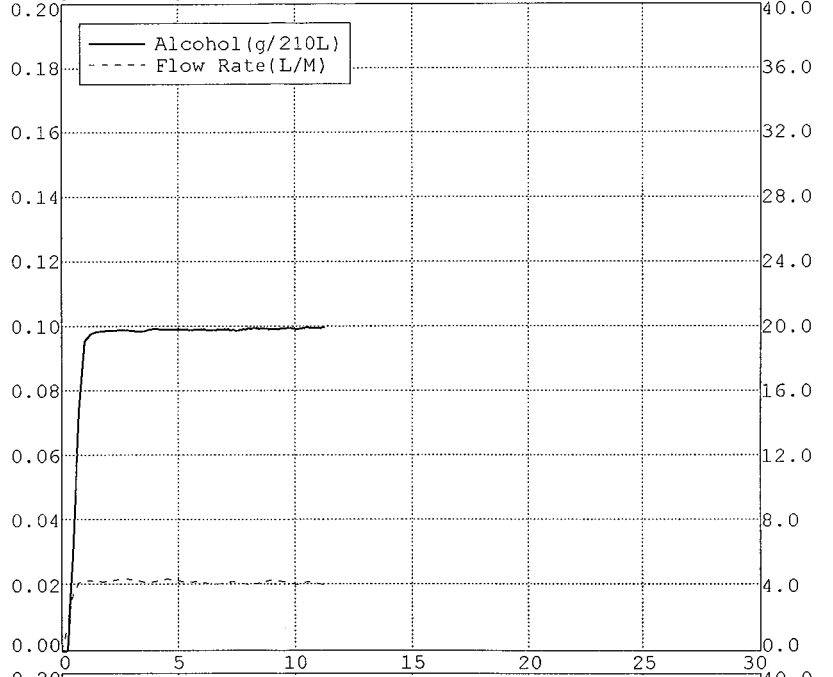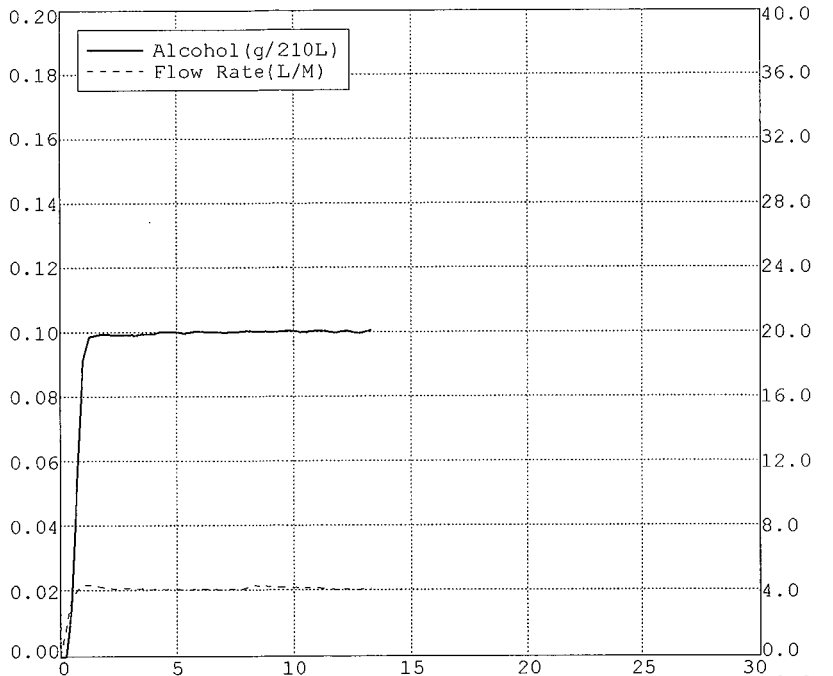

Hollie B Kennedy
 Hollie B Kennedy 10/05

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 07/12/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:42
INTERNAL STANDARD	VERIFIED	10:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:43
BLANK TEST	0.00	10:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:44
BLANK TEST	0.00	10:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:45
BLANK TEST	0.00	10:46

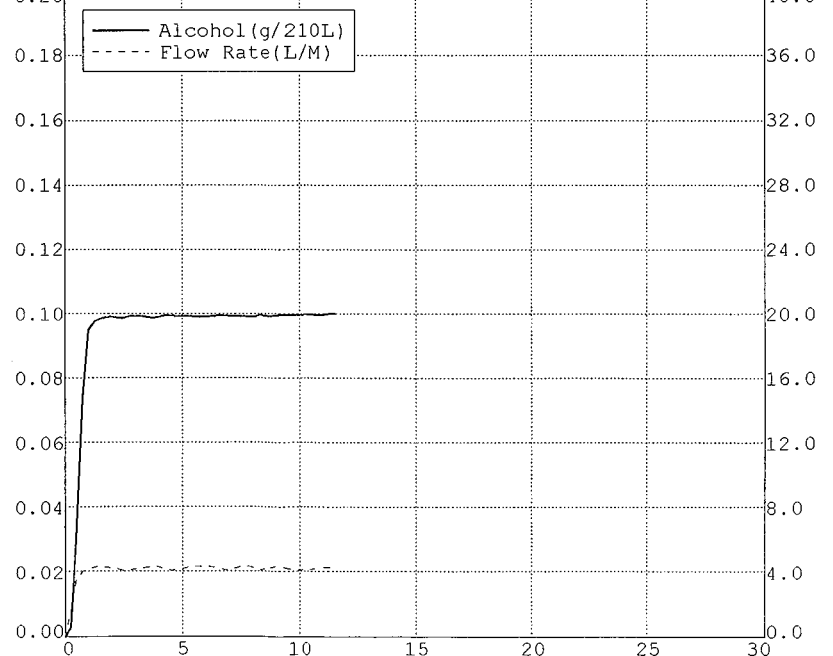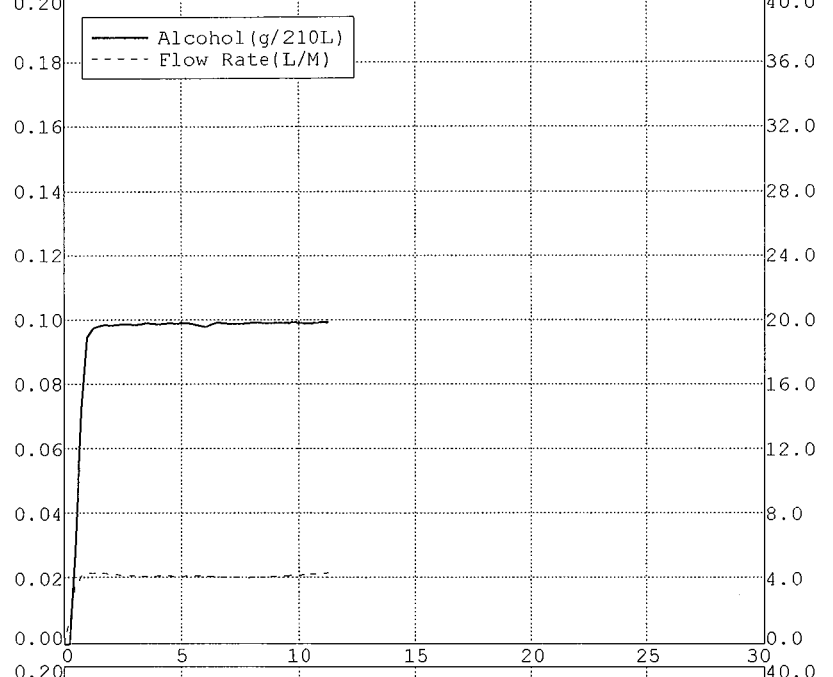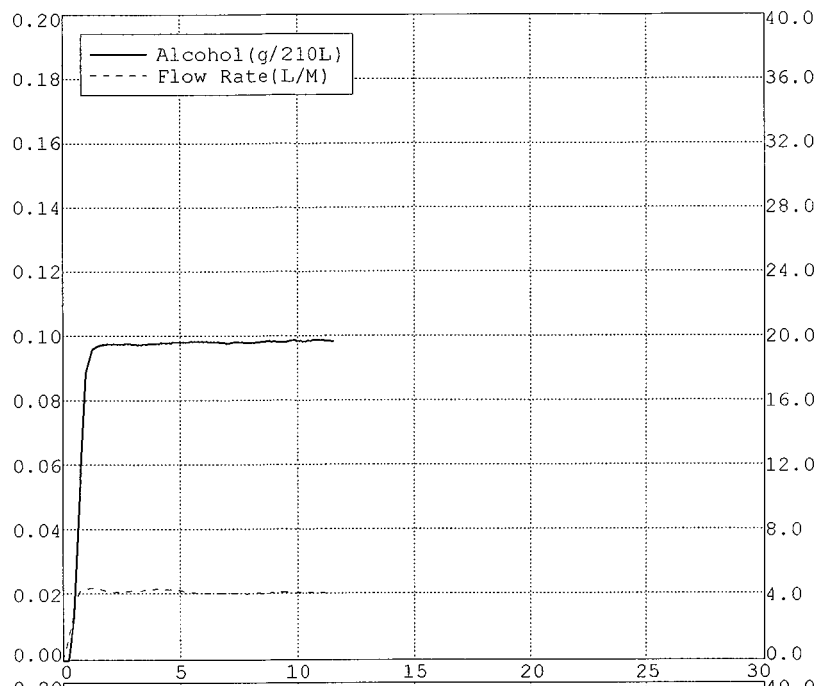

Hollie B Kennedy
Rome PD 07/12/19
10:05

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

ate: 07/19/2019

OPERATOR NAME:
HOLLIE B KENNEDYH
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:40
INTERNAL STANDARD	VERIFIED	15:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:41
BLANK TEST	0.00	15:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:42
BLANK TEST	0.00	15:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:43
BLANK TEST	0.00	15:44

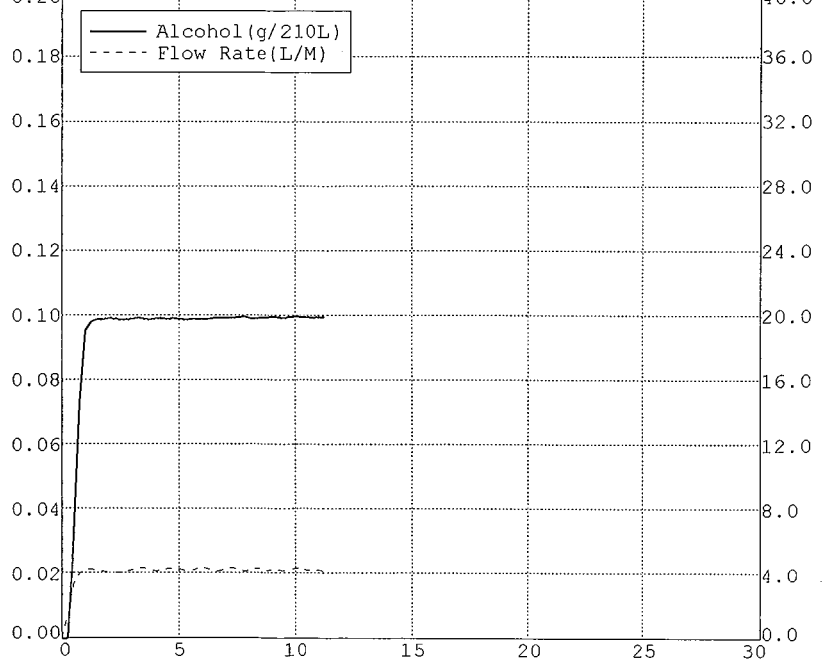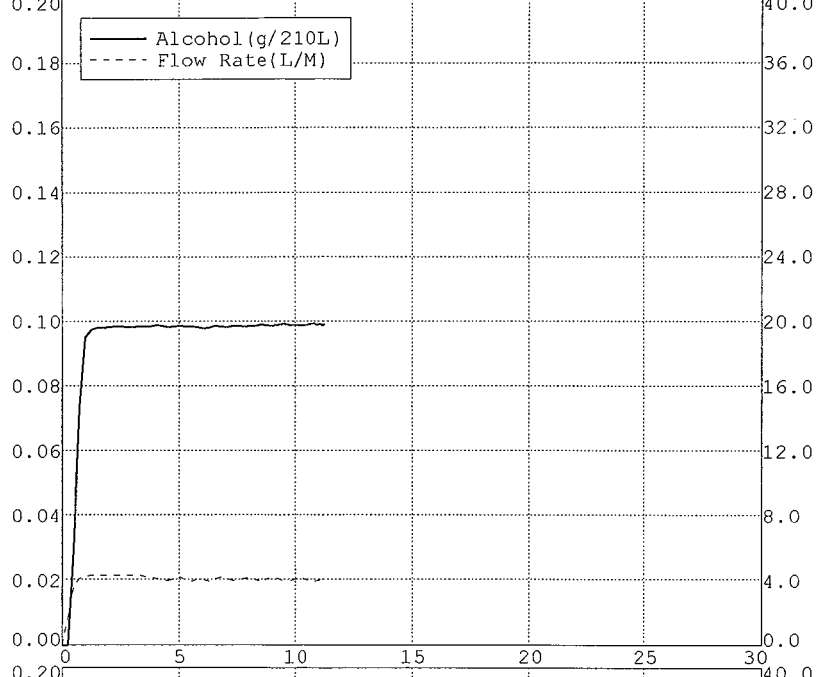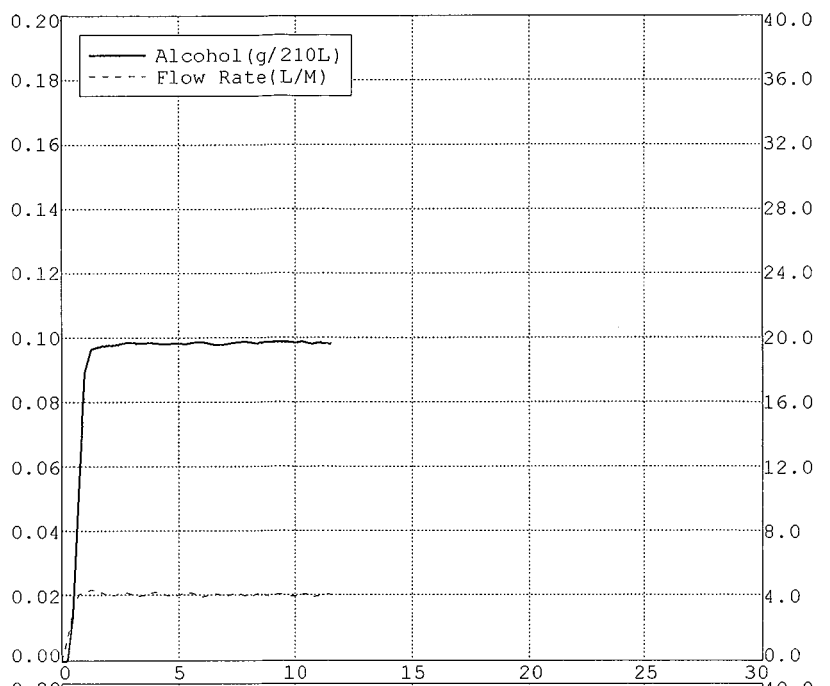

Hollie B Kennedy 07/19/19
Hollie B Kennedy was

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 07/27/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:14
INTERNAL STANDARD	VERIFIED	15:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:14
BLANK TEST	0.00	15:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:15
BLANK TEST	0.00	15:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:16
BLANK TEST	0.00	15:17

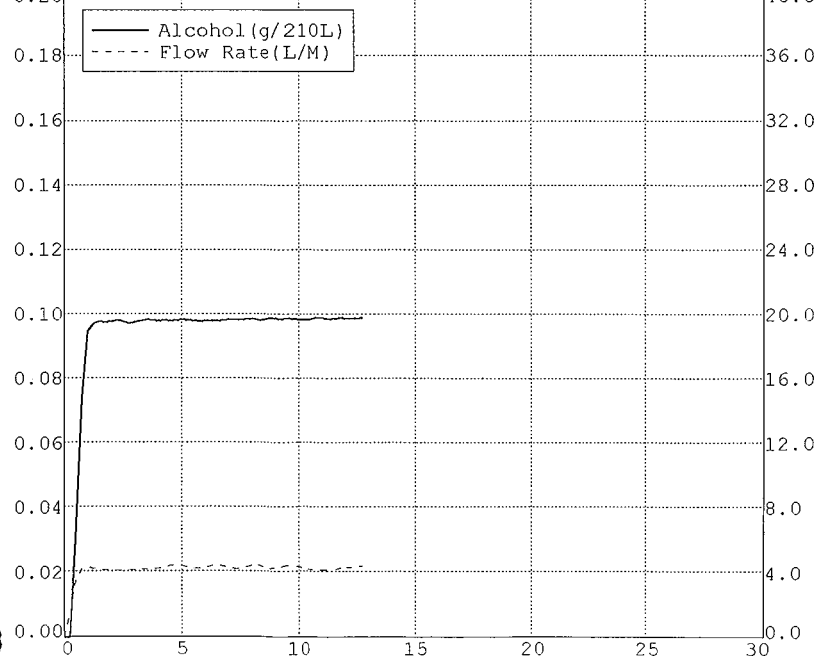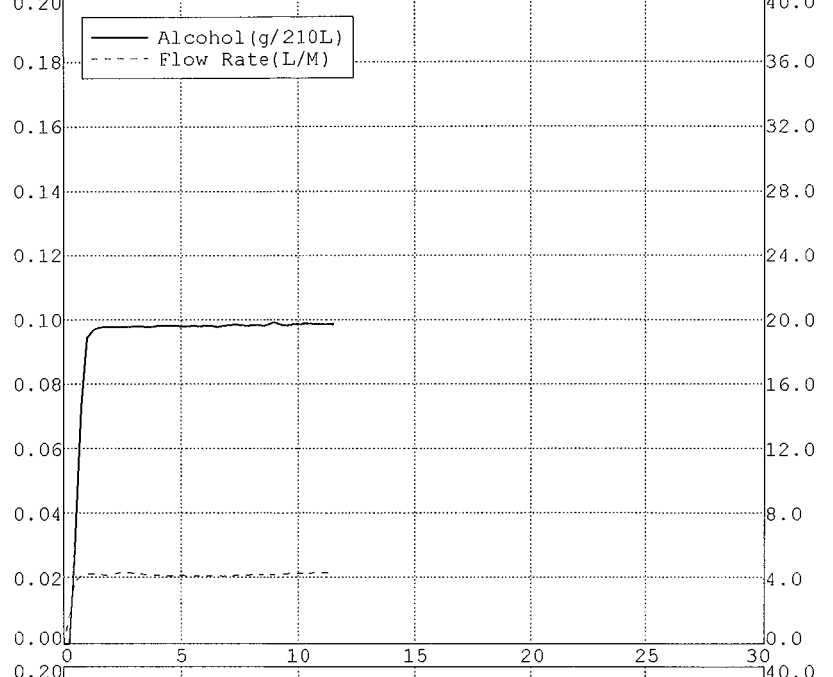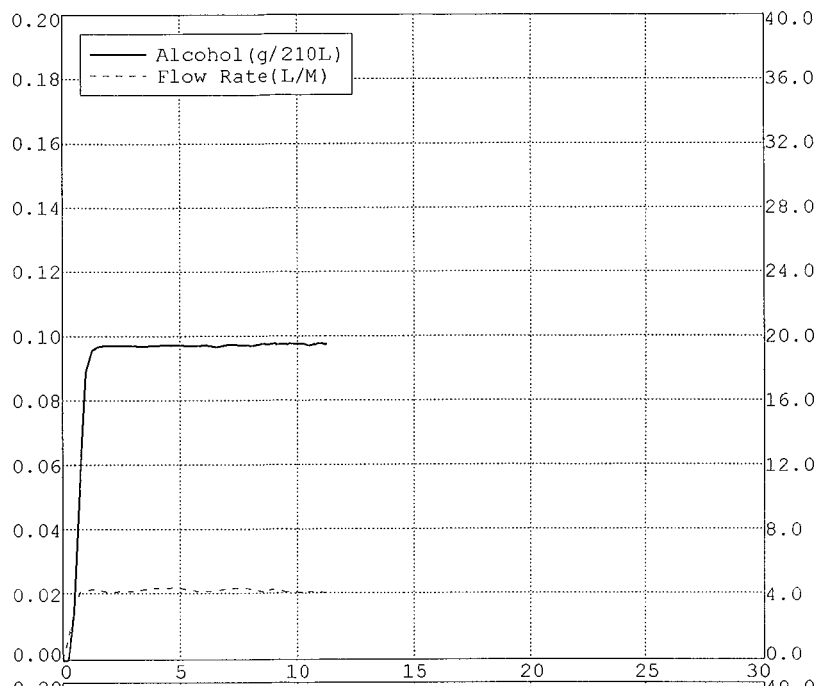

Huntbill Silverman RomCPD 07/29/19
D. Silverman 108cs