

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 04/03/2020

OPERATOR NAME:
HOLLIE B SILVERMAN
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:34
INTERNAL STANDARD	VERIFIED	15:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:34
BLANK TEST	0.00	15:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:36
BLANK TEST	0.00	15:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:37
BLANK TEST	0.00	15:38

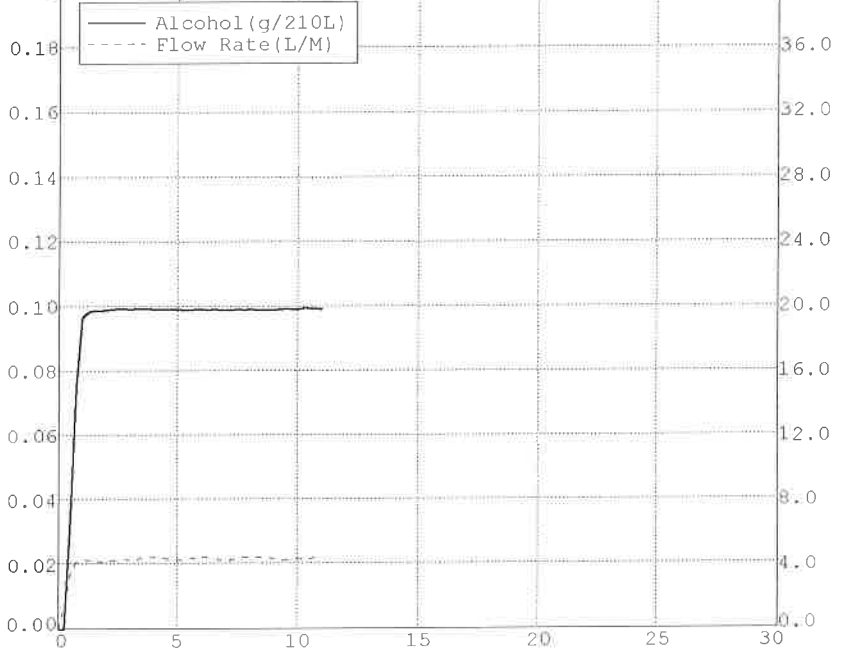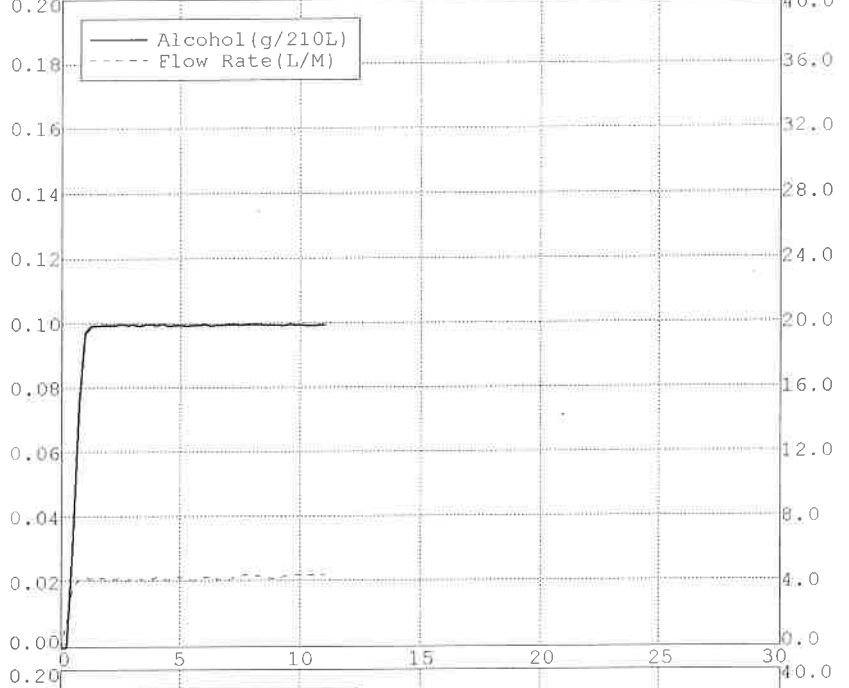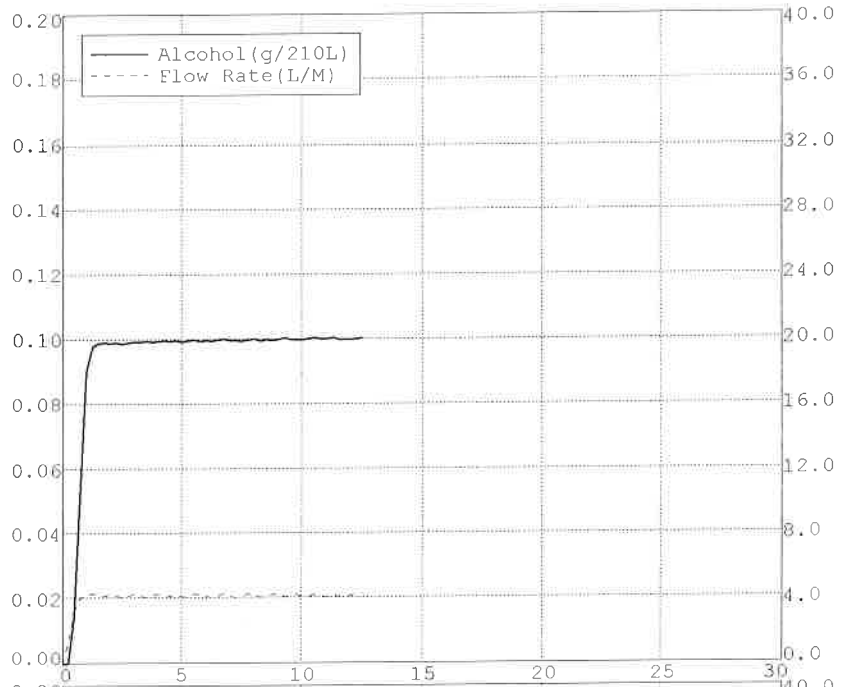

Hollie B. Silverman Rome PD 04/03/2020
Hollie B. Silverman