

SUPERVISOR TEST




ROME CITY  
POLICE DEPT  
DATAMASTER dmt: 106106

Date: 06/12/2020

OPERATOR NAME:  
HOLLIE B SILVERMAN  
Permit #: 39044  
Operator Agency/Dept: ROME CITY PD  
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:17
INTERNAL STANDARD	VERIFIED	16:17
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:18
BLANK TEST	0.00	16:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:19
BLANK TEST	0.00	16:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:20
BLANK TEST	0.00	16:21

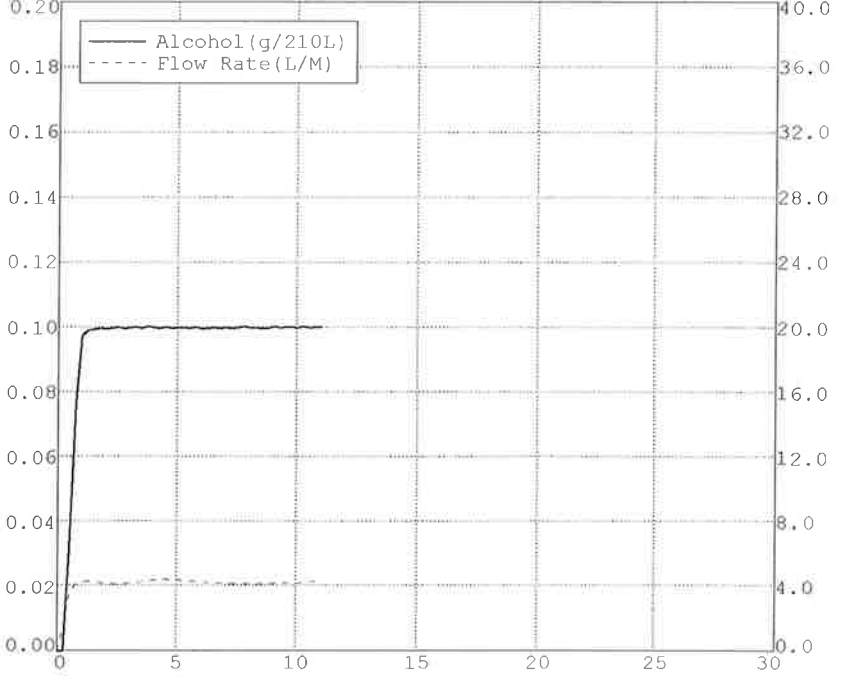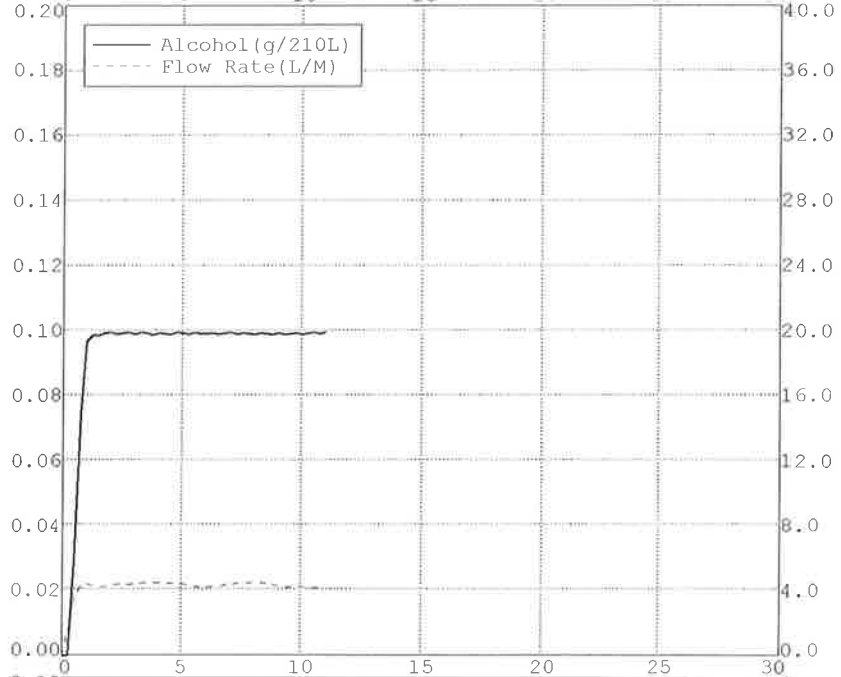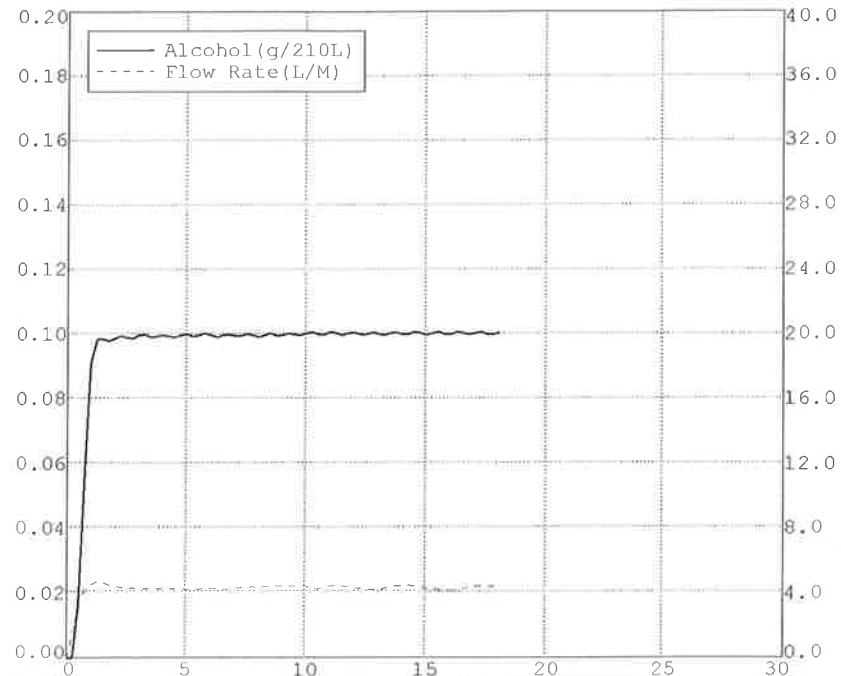

Hollie Silverman Rome PD 06/12/2020

Hollie Silverman 10105