

SUPERVISOR TEST

UTICA CITY
 POLICE DEPT
 DATAMASTER dmt: 107308




Date: 10/29/2019

OPERATOR NAME:
 MICHAEL J CLIVE
 Permit #: 36682
 Operator Agency/Dept: UTICA CITY PD
 Reference Standard #: 19180

RM
19-11-201

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:10
INTERNAL STANDARD	VERIFIED	15:10
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	15:10
BLANK TEST	0.00	15:11
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	15:11
BLANK TEST	0.00	15:12
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	15:13
BLANK TEST	0.00	15:13

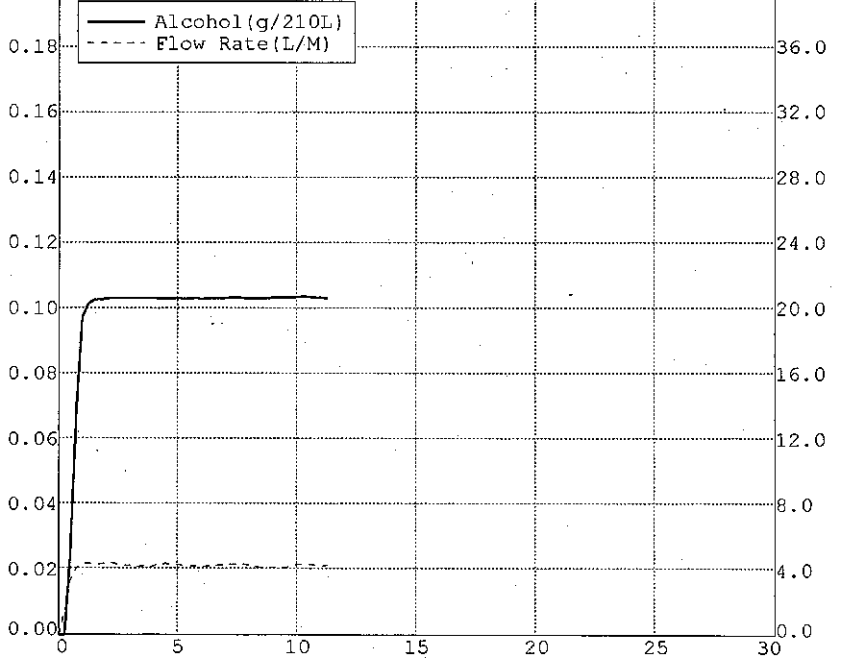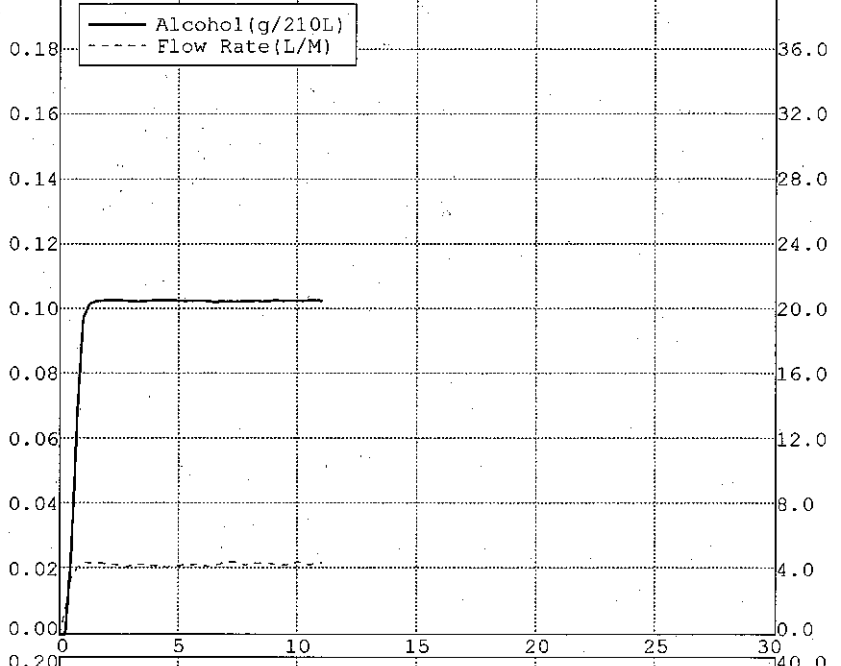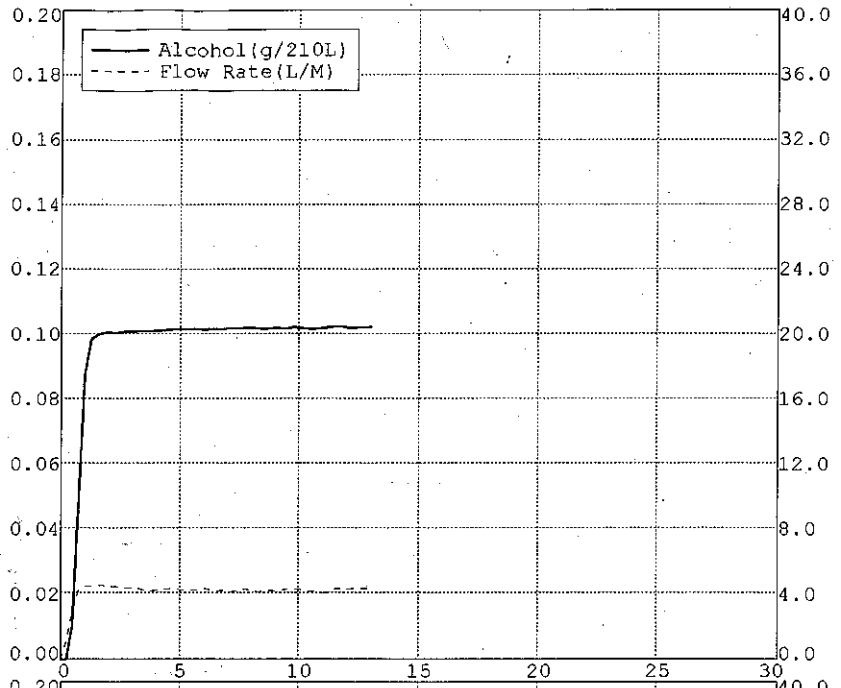

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282

Date: 10/29/2019

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 19180

RMS
19-11701

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:09
INTERNAL STANDARD	VERIFIED	15:09
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	15:10
BLANK TEST	0.00	15:10
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	15:11
BLANK TEST	0.00	15:11
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	15:12
BLANK TEST	0.00	15:13

