

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308




Date: 12/03/2019

*AMS
19-45908*

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:39
INTERNAL STANDARD	VERIFIED	13:39
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	13:39
BLANK TEST	0.00	13:40
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	13:40
BLANK TEST	0.00	13:41
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	13:41
BLANK TEST	0.00	13:42

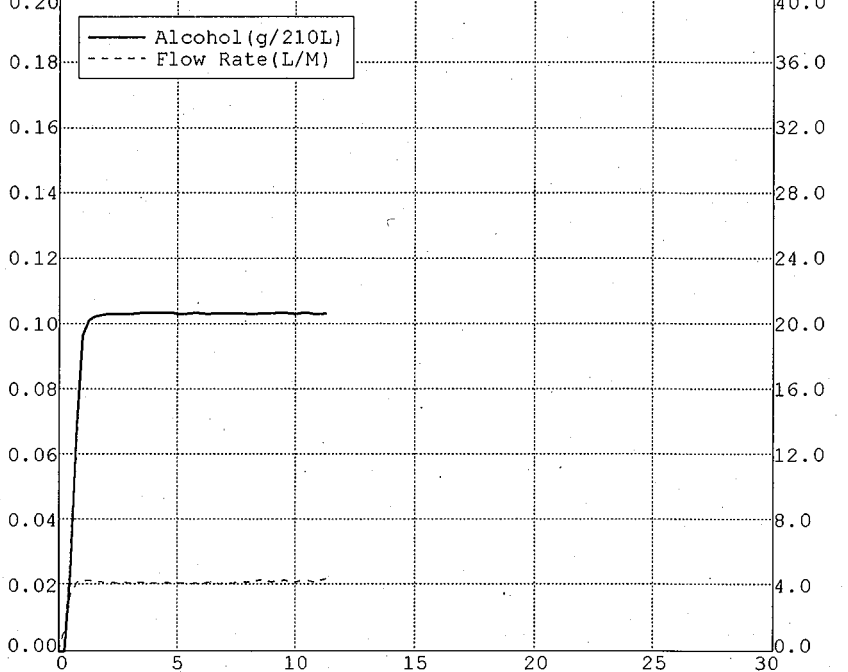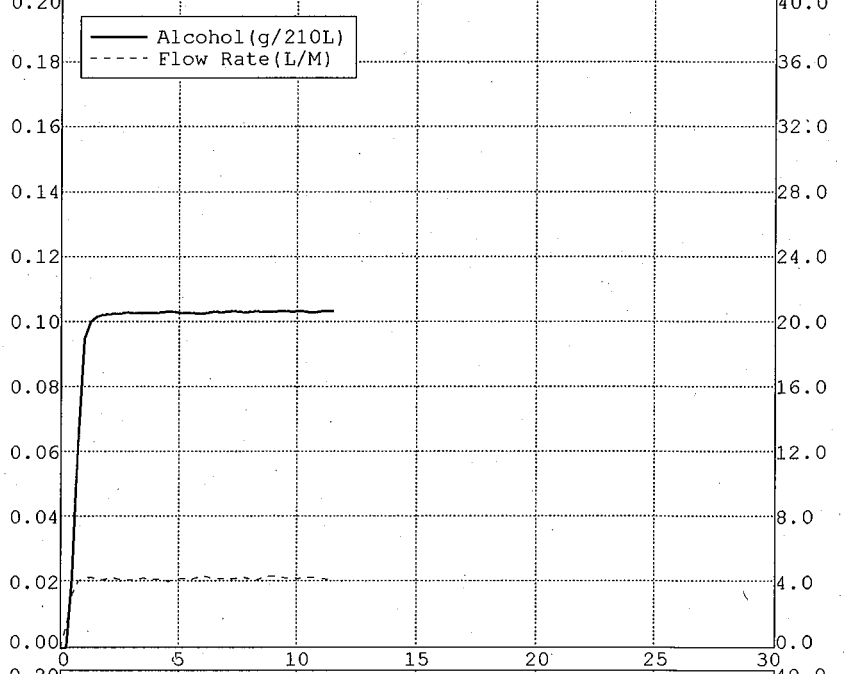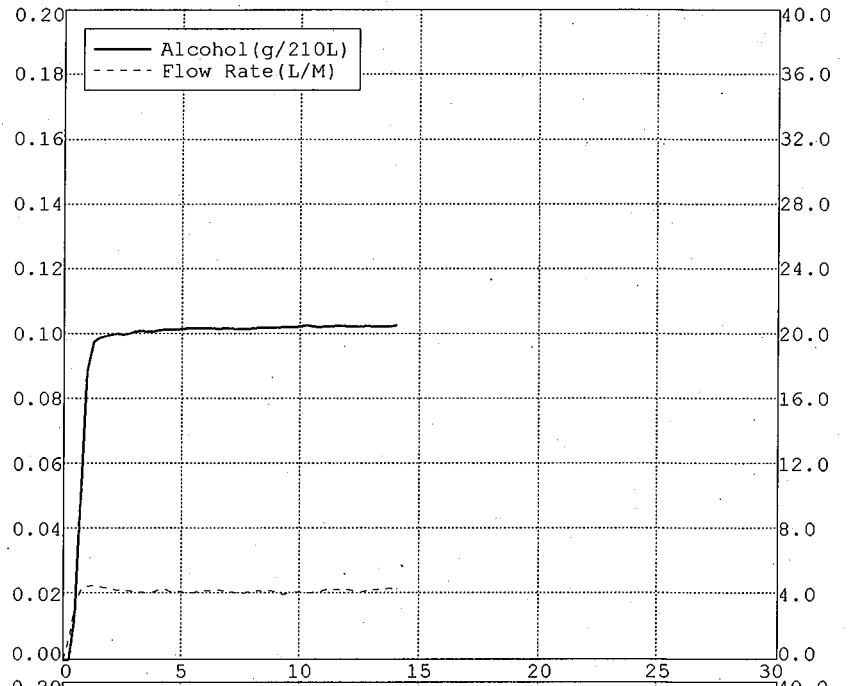

SUPERVISOR TEST

UTICA CITY
 POLICE DEPT
 DATAMASTER dmt: 100282

Date: 12/03/2019

RMS
19-45908

OPERATOR NAME:
 MICHAEL J CLIVE
 Permit #: 366682
 Operator Agency/Dept: UTICA CITY PD
 Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:54
INTERNAL STANDARD	VERIFIED	12:54
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	12:55
BLANK TEST	0.00	12:56
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	12:56
BLANK TEST	0.00	12:57
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	12:57
BLANK TEST	0.00	12:58

