

SUPERVISOR TEST

UTICA CITY
 POLICE DEPT
 DATAMASTER dmt: 107308




Date: 02/11/2020

*PLS
 20-4806*

OPERATOR NAME:
 MICHAEL J CLIVE
 Permit #: 36682
 Operator Agency/Dept: UTICA CITY PD
 Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:57
INTERNAL STANDARD	VERIFIED	11:57
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:57
BLANK TEST	0.00	11:58
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:58
BLANK TEST	0.00	11:59
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:59
BLANK TEST	0.00	12:00

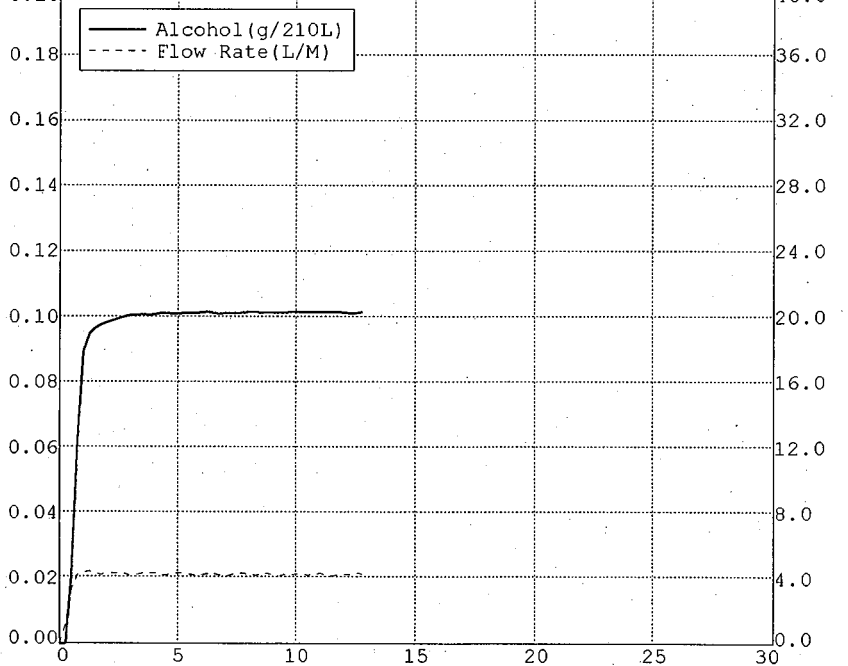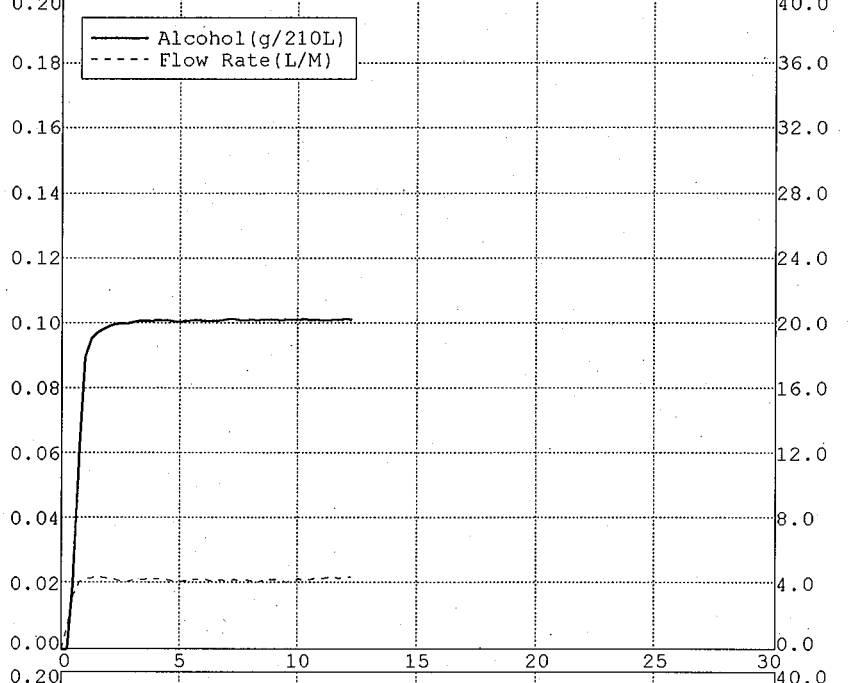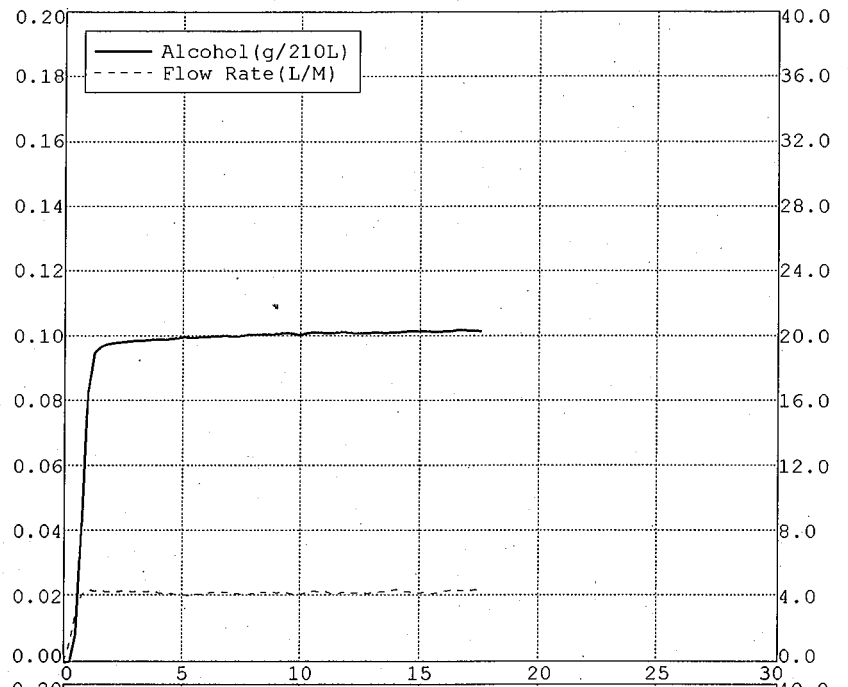

SUPERVISOR TEST

UTICA CITY
 POLICE DEPT
 DATAMASTER dmt: 100282

Date: 02/11/2020

ZMS
20-4806

OPERATOR NAME:
 MICHAEL J CLIVE
 Permit #: 36682
 Operator Agency/Dept: UTICA CITY PD
 Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:37
INTERNAL STANDARD	VERIFIED	09:37
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	09:37
BLANK TEST	0.00	09:38
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	09:38
BLANK TEST	0.00	09:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:40
BLANK TEST	0.00	09:40

