

SUPERVISOR TEST




-----  
WHITESTOWN TOWN  
POLICE DEPT.  
DATAMASTER dmt: 100231  
-----

Date: 12/28/2019

OPERATOR NAME:  
D J HUMPHRIES II  
Permit #: 40440  
Operator Agency/Dept: WHITESTOWN TOWN PD  
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:48
INTERNAL STANDARD	VERIFIED	20:48
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	20:48
BLANK TEST	0.00	20:49
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	20:50
BLANK TEST	0.00	20:50
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	20:51
BLANK TEST	0.00	20:52

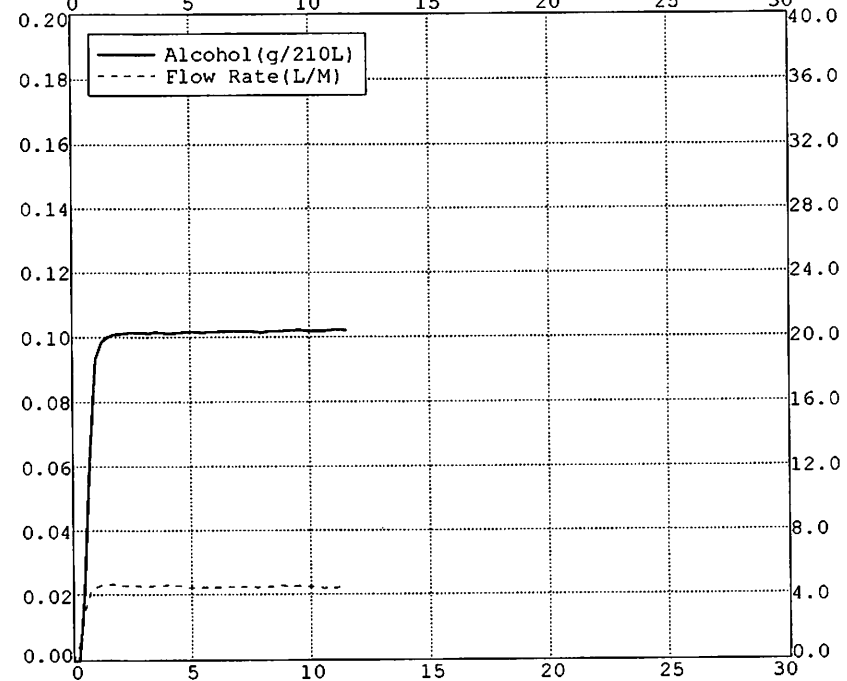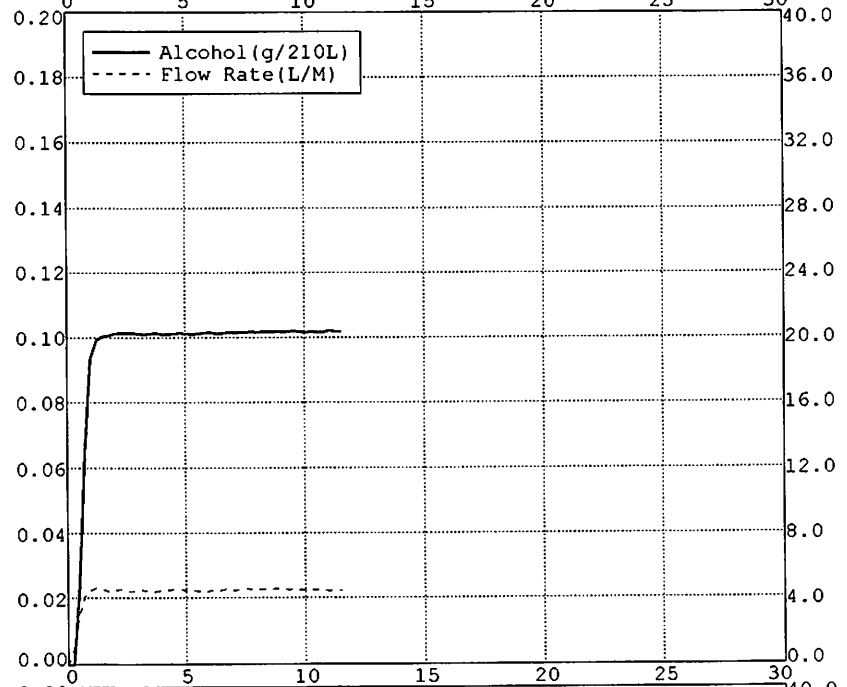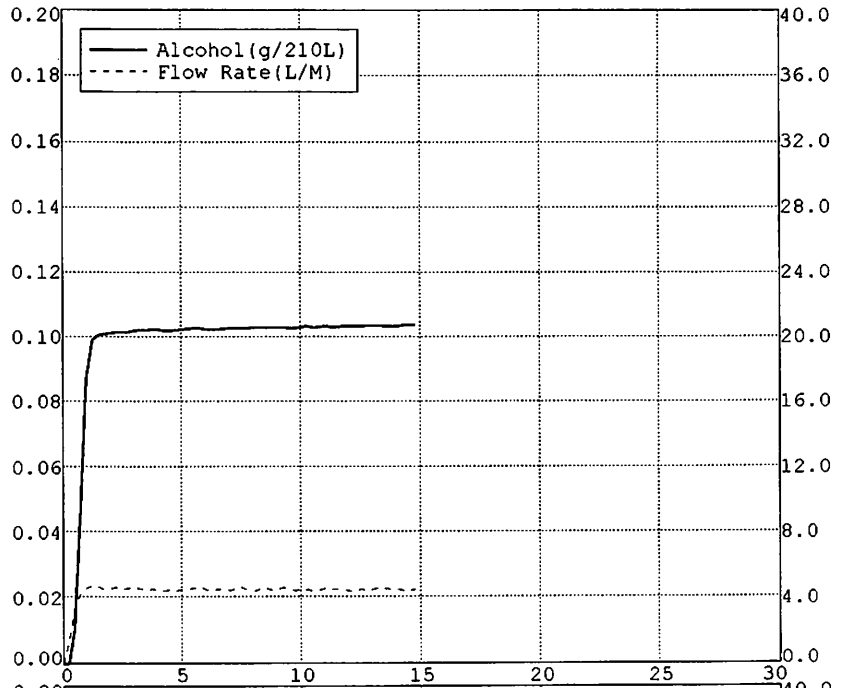

SUPERVISOR TEST




WHITESTOWN TOWN  
POLICE DEPT.  
DATAMASTER dmt: 100231

ate: 12/12/2019

OPERATOR NAME:  
D J HUMPHRIES II  
Permit #: 40440  
Operator Agency/Dept: WHITESTOWN TOWN PD  
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:42
INTERNAL STANDARD	VERIFIED	20:42
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	20:43
BLANK TEST	0.00	20:44
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	20:44
BLANK TEST	0.00	20:45
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	20:45
BLANK TEST	0.00	20:46

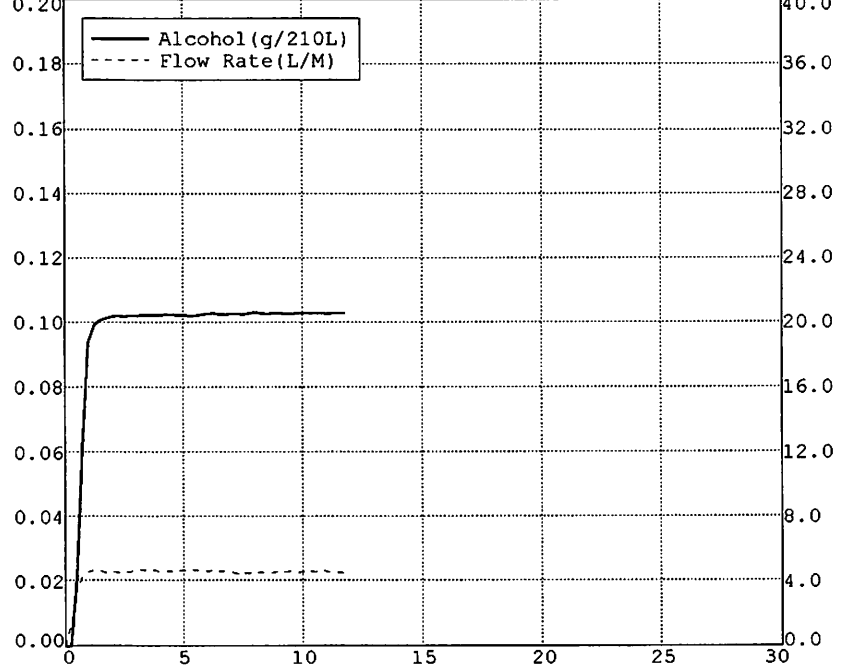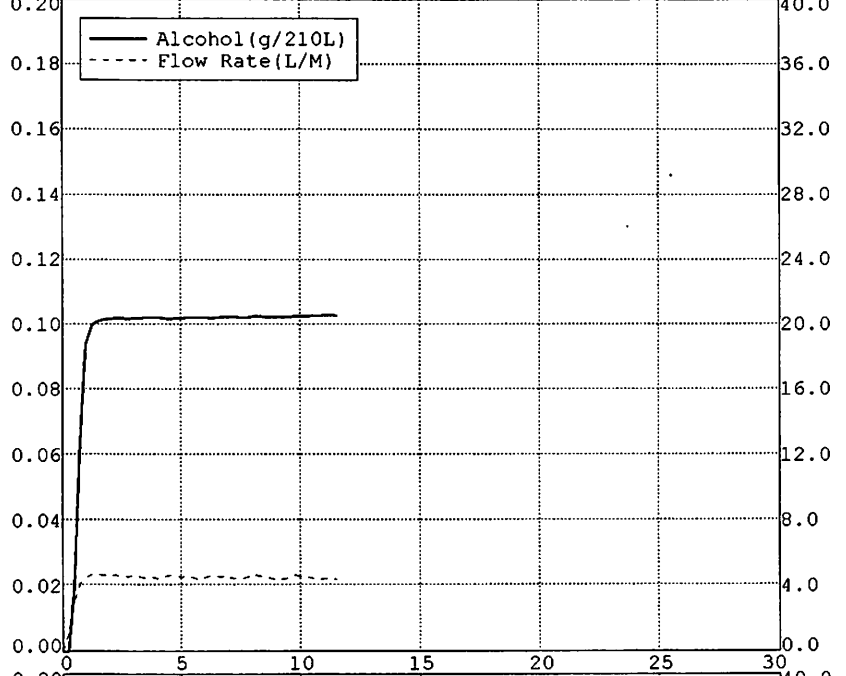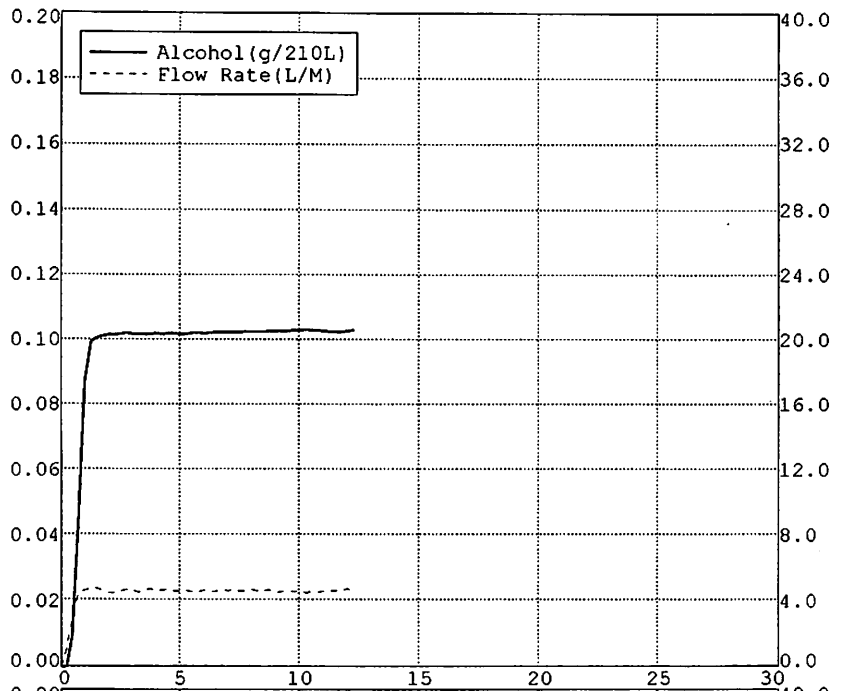

SOLUTION CHANGE

-----  
WHITESTOWN TOWN  
POLICE DEPT.  
DATAMASTER dmt: 100231  
-----

Date: 12/01/2019

OPERATOR NAME:  
D J HUMPHRIES II  
Permit #: 40440  
Operator Agency/Dept: WHITESTOWN TOWN PD  
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:17
INTERNAL STANDARD	VERIFIED	19:17
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	19:18
BLANK TEST	0.00	19:19
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	19:19
BLANK TEST	0.00	19:20
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	19:20
BLANK TEST	0.00	19:21

