

SOLUTION CHANGE

LEB




ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 04/01/2020

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 20040

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 18:35 |
| INTERNAL STANDARD | VERIFIED | 18:35 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 18:35 |
| BLANK TEST | 0.00 | 18:36 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 18:36 |
| BLANK TEST | 0.00 | 18:37 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 18:38 |
| BLANK TEST | 0.00 | 18:38 |

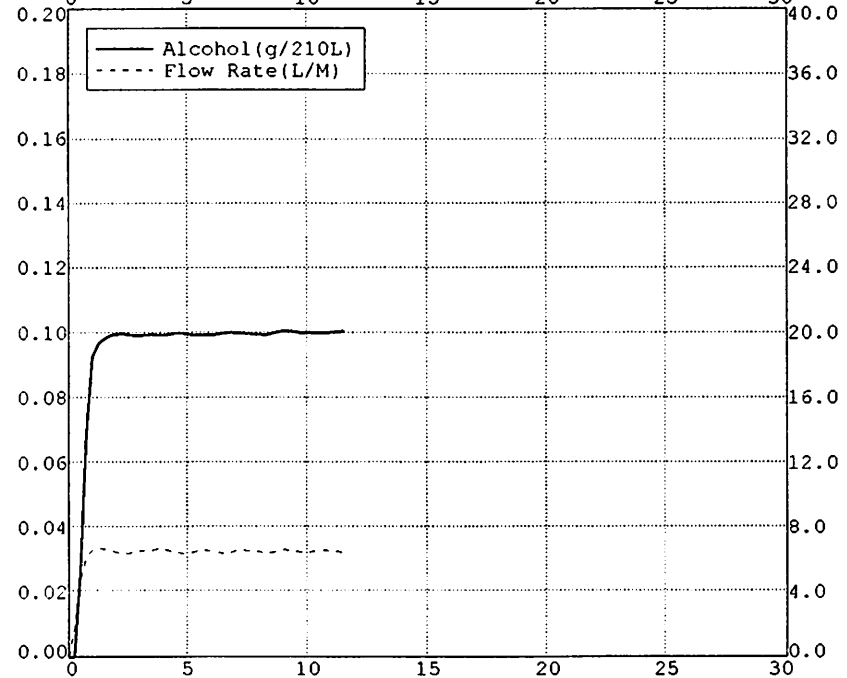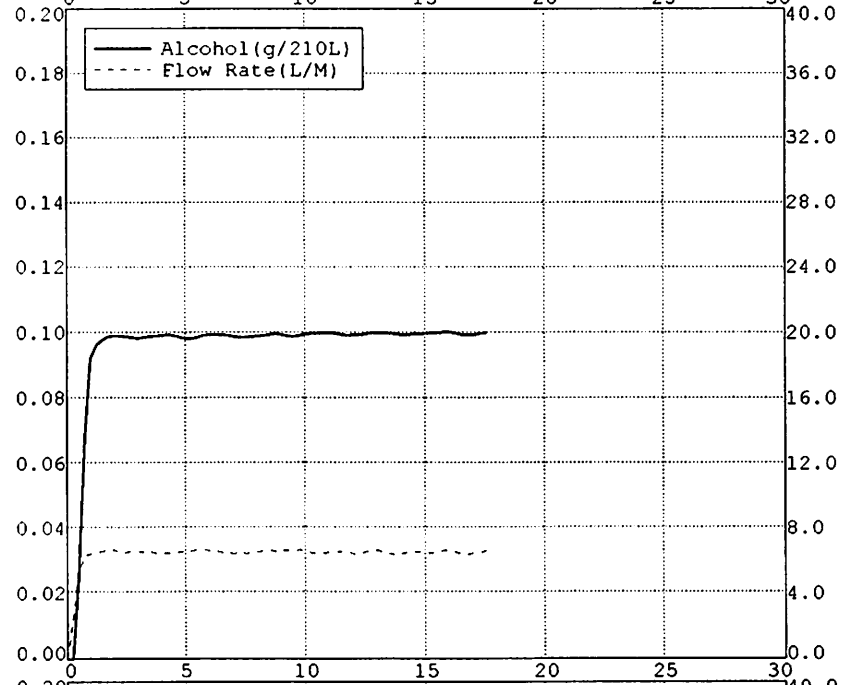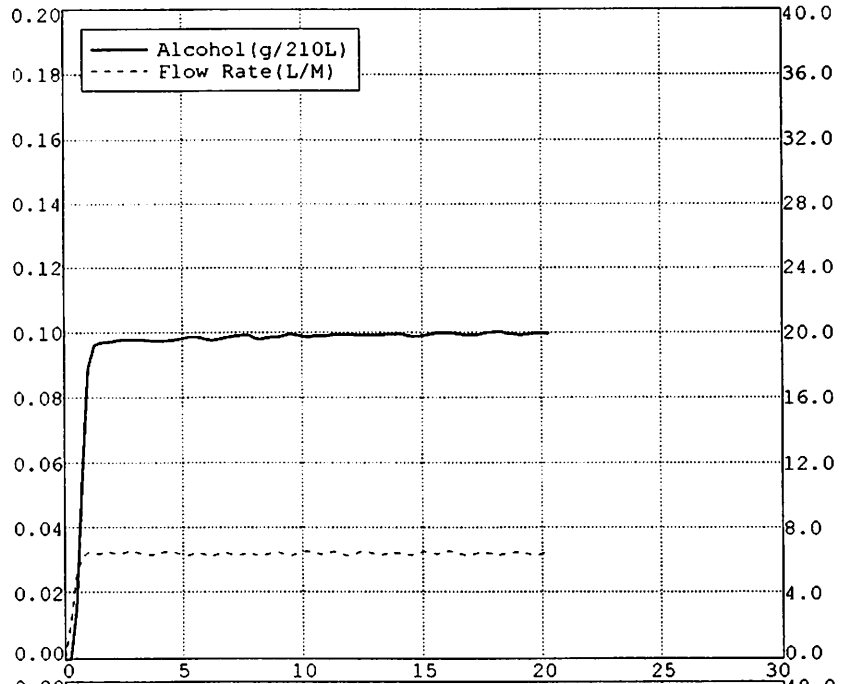

SUPERVISOR TEST

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 04/08/2020

OPERATOR NAME:
BRANDON J RUTLEDGE
Permit #: 43762
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 20040

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 20:27 |
| INTERNAL STANDARD | VERIFIED | 20:27 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 20:28 |
| BLANK TEST | 0.00 | 20:28 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 20:29 |
| BLANK TEST | 0.00 | 20:30 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 20:30 |
| BLANK TEST | 0.00 | 20:31 |

LER

