

SOLUTION CHANGE




ROME CITY  
 POLICE DEPT  
 DATAMASTER dmt: 106106

Date: 06/01/2020

OPERATOR NAME:  
 HOLLIE B SILVERMAN  
 Permit #: 39044  
 Operator Agency/Dept: ROME CITY PD  
 Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:34
INTERNAL STANDARD	VERIFIED	22:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	22:35
BLANK TEST	0.00	22:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	22:36
BLANK TEST	0.00	22:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	22:37
BLANK TEST	0.00	22:38

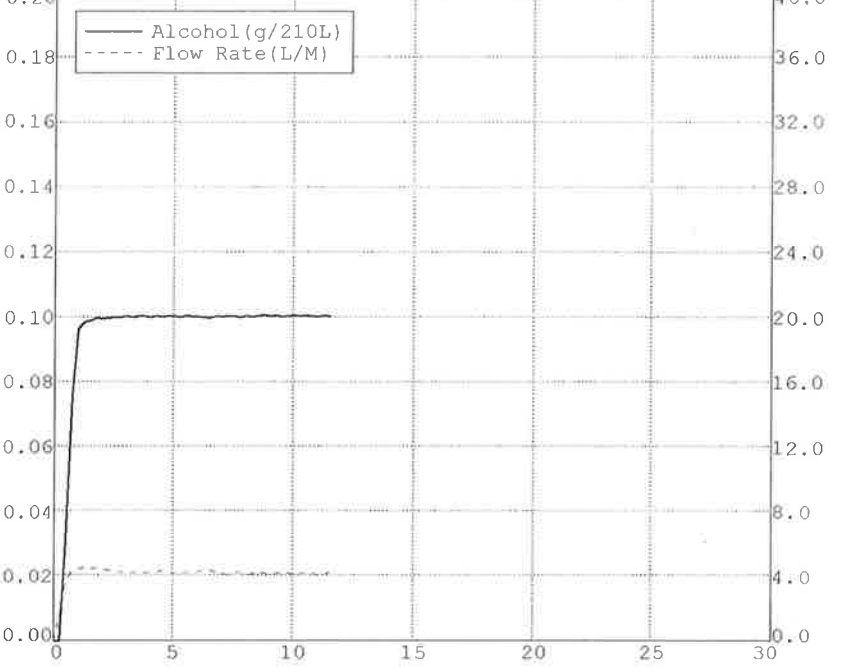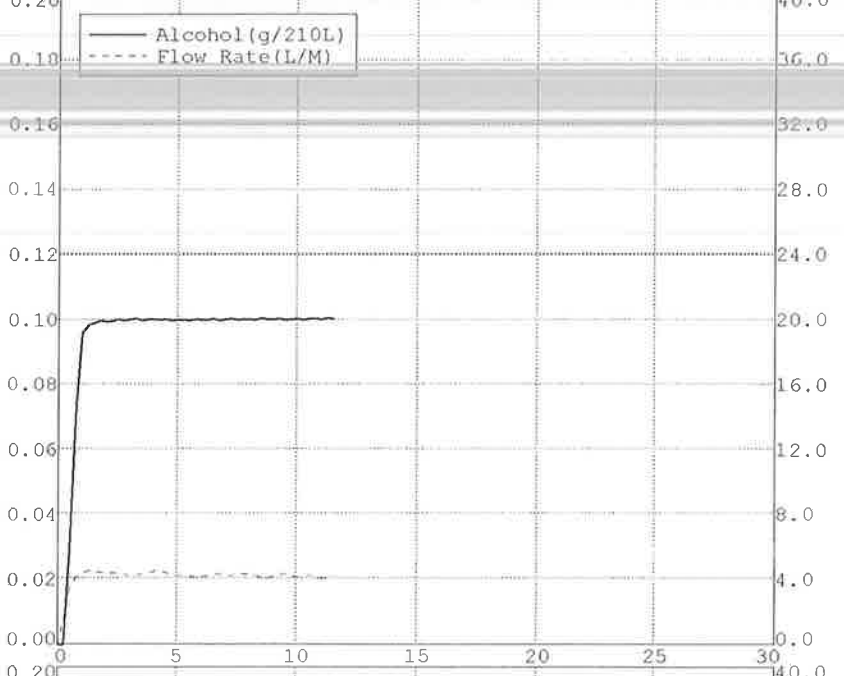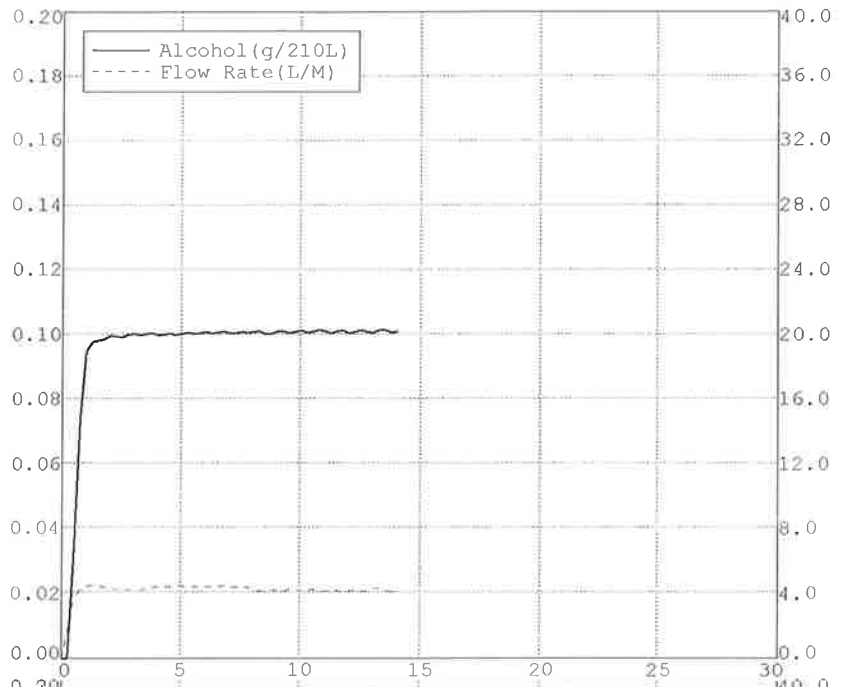

Hollie B. Silverman Rome PD 06/01/2020  
 Hollie B. Silverman 106106