

SOLUTION CHANGE




ROME CITY  
POLICE DEPT  
DATAMASTER dmt: 106106

Date: 01/01/2019

OPERATOR NAME:  
HOLLIE B KENNEDY  
Permit #: 39044  
Operator Agency/Dept: ROME CITY PD  
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:04
INTERNAL STANDARD	VERIFIED	16:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:05
BLANK TEST	0.00	16:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:06
BLANK TEST	0.00	16:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:07
BLANK TEST	0.00	16:08

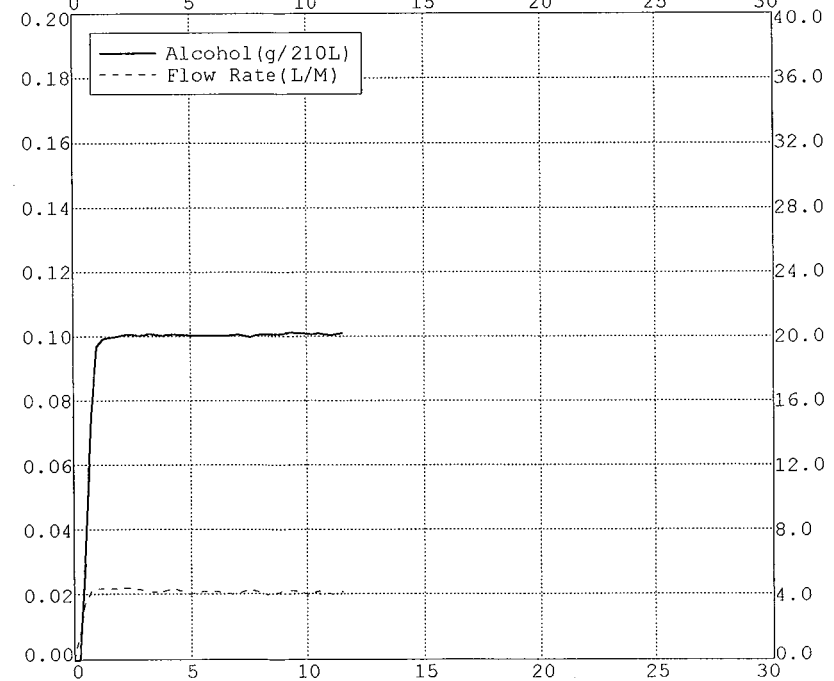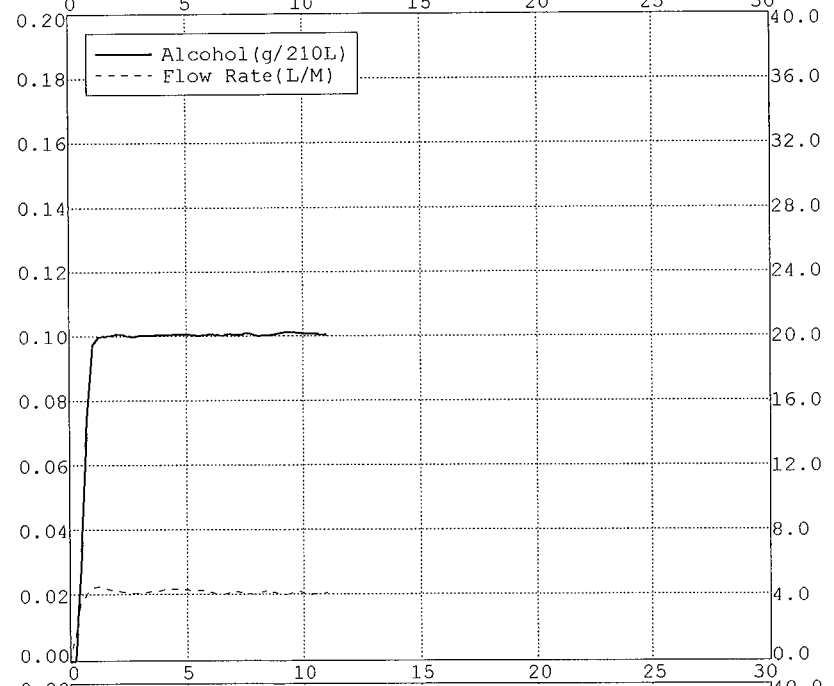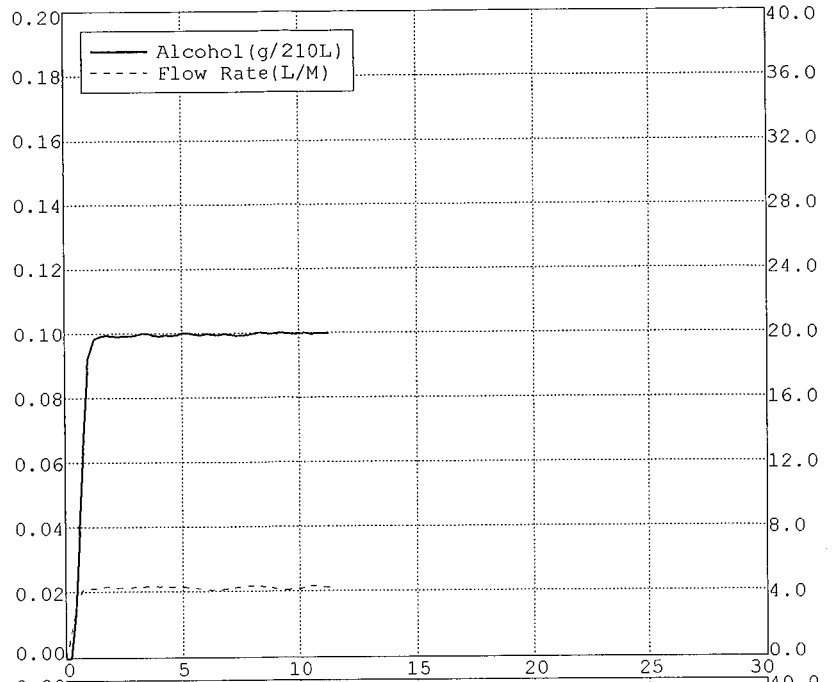

*Hollie B Kennedy* Rome PD 01/01/19  
*Hollie B Kennedy* 10805

SUPERVISOR TEST

ROME CITY  
POLICE DEPT  
DATAMASTER dmt: 106106




Date: 01/04/2019

OPERATOR NAME:  
HOLLIE B KENNEDY  
Permit #: 39044  
Operator Agency/Dept: ROME CITY PD  
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:27
INTERNAL STANDARD	VERIFIED	15:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.08	15:28
BLANK TEST	0.00	15:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.08	15:29
BLANK TEST	0.00	15:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.08	15:30

Blank Error

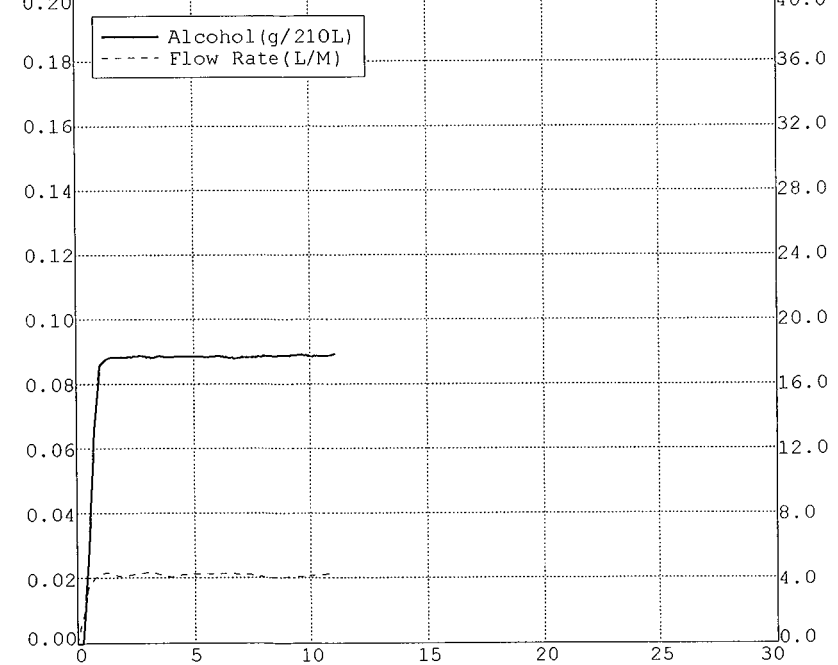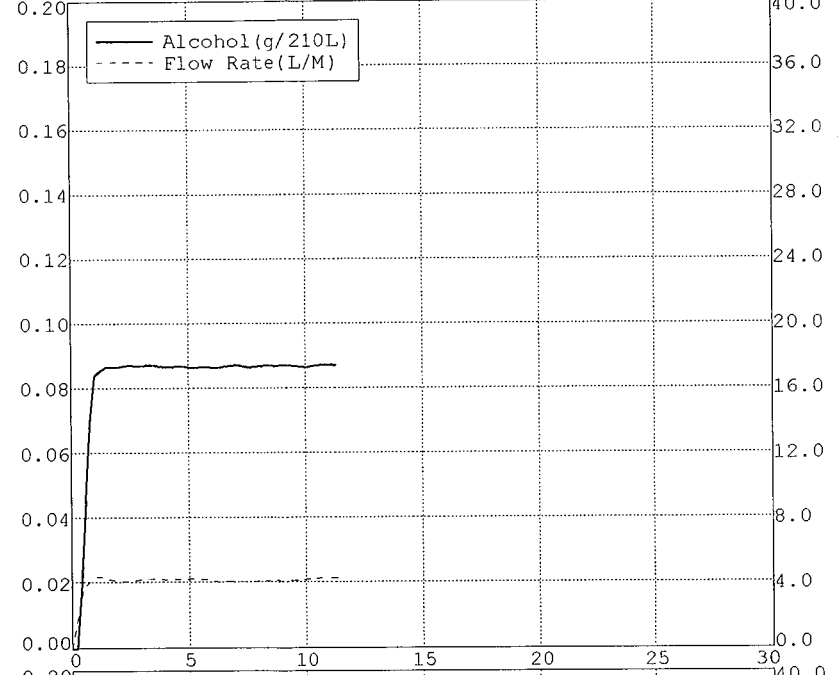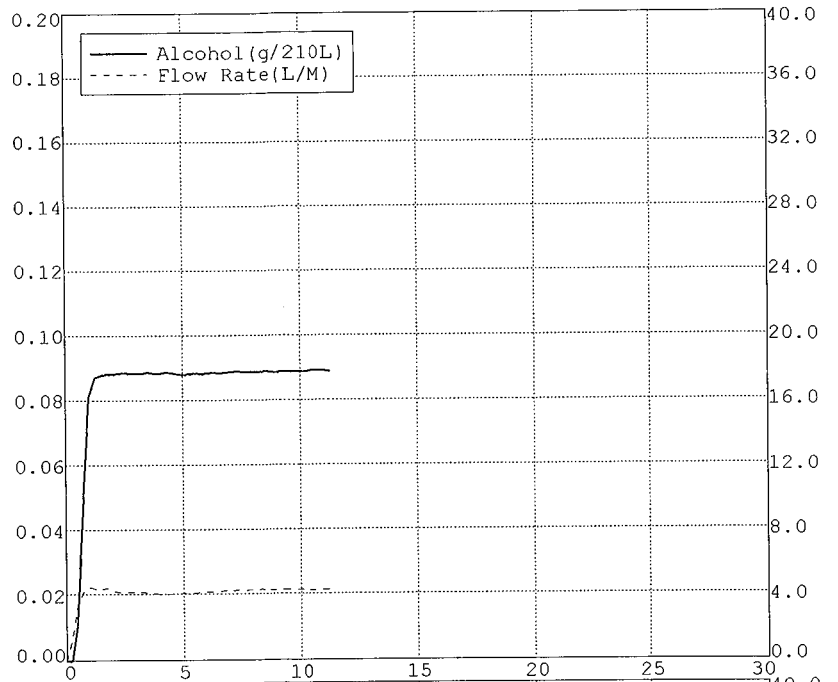

*Hollie Kennedy Rome PD 01/04/19*  
*Hollie Kennedy 10805*

SUPERVISOR TEST




ROME CITY  
POLICE DEPT  
DATAMASTER dmt: 106106

Date: 01/04/2019

OPERATOR NAME:  
HOLLIE B KENNEDY  
Permit #: 39044  
Operator Agency/Dept: ROME CITY PD  
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:08
INTERNAL STANDARD	VERIFIED	20:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	20:08
BLANK TEST	0.00	20:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	20:09
BLANK TEST	0.00	20:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	20:11
BLANK TEST	0.00	20:11

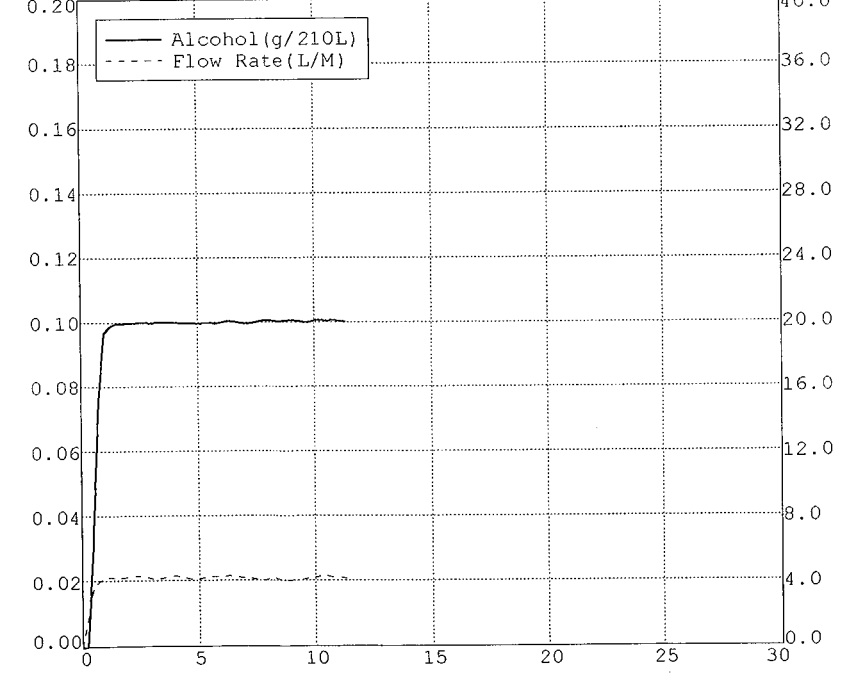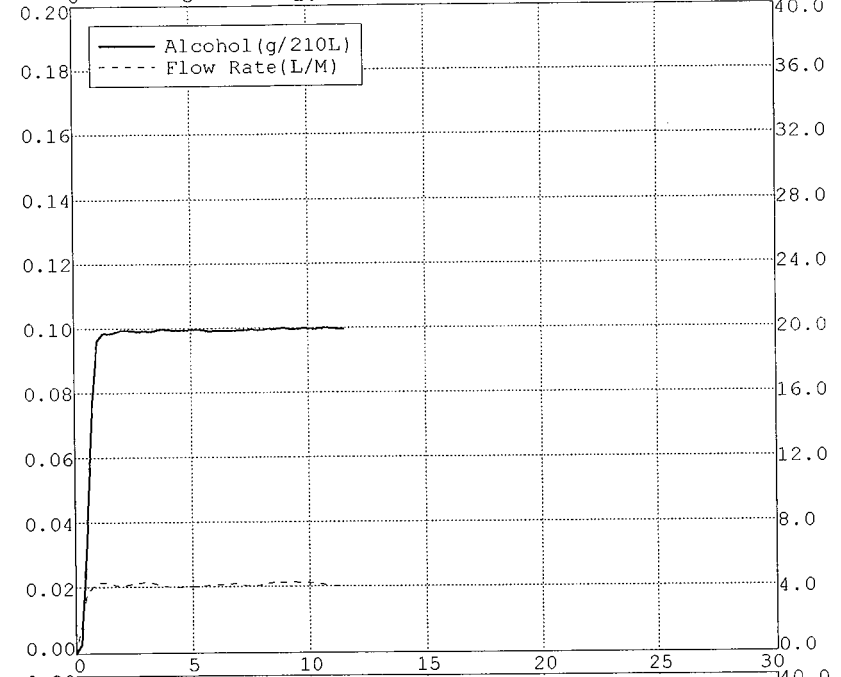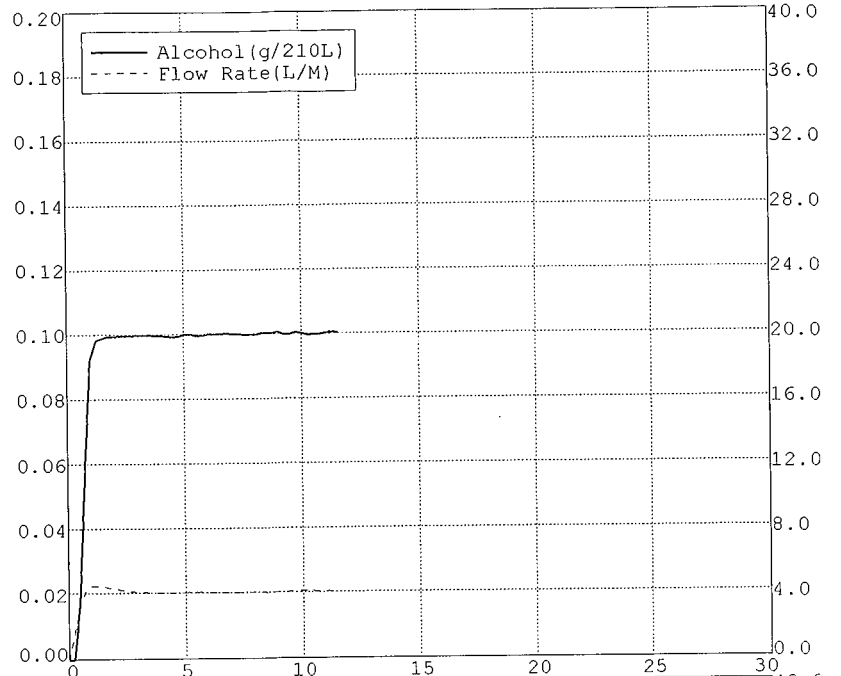

*Hollie Kennedy Rome PD 01/04/19*  
*Hollie Kennedy 106106*

SUPERVISOR TEST




ROME CITY  
POLICE DEPT  
DATAMASTER dmt: 106106

Date: 01/11/2019

OPERATOR NAME:  
HOLLIE B KENNEDY  
Permit #: 39044  
Operator Agency/Dept: ROME CITY PD  
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:35
INTERNAL STANDARD	VERIFIED	19:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	19:35
BLANK TEST	0.00	19:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	19:36
BLANK TEST	0.00	19:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	19:37
BLANK TEST	0.00	19:38

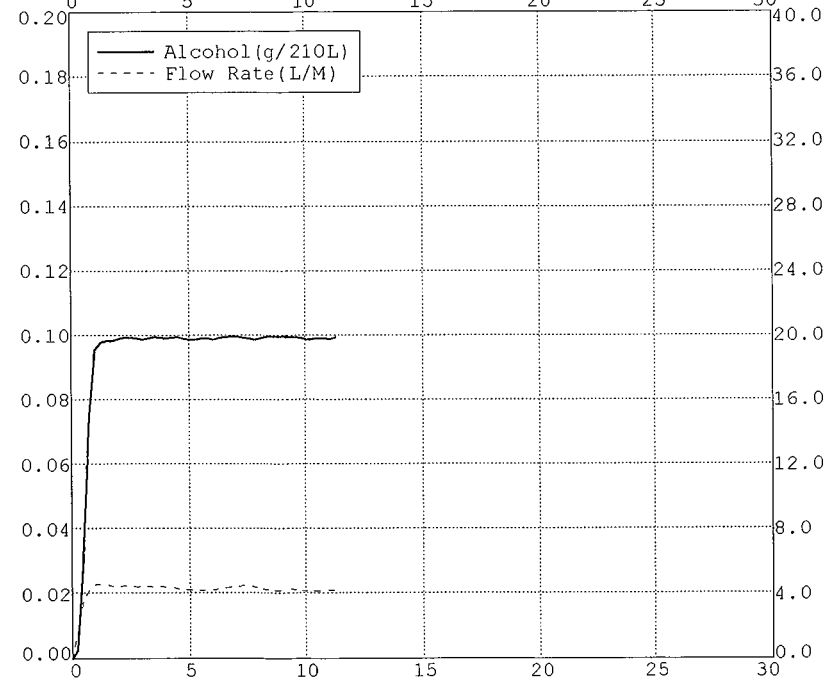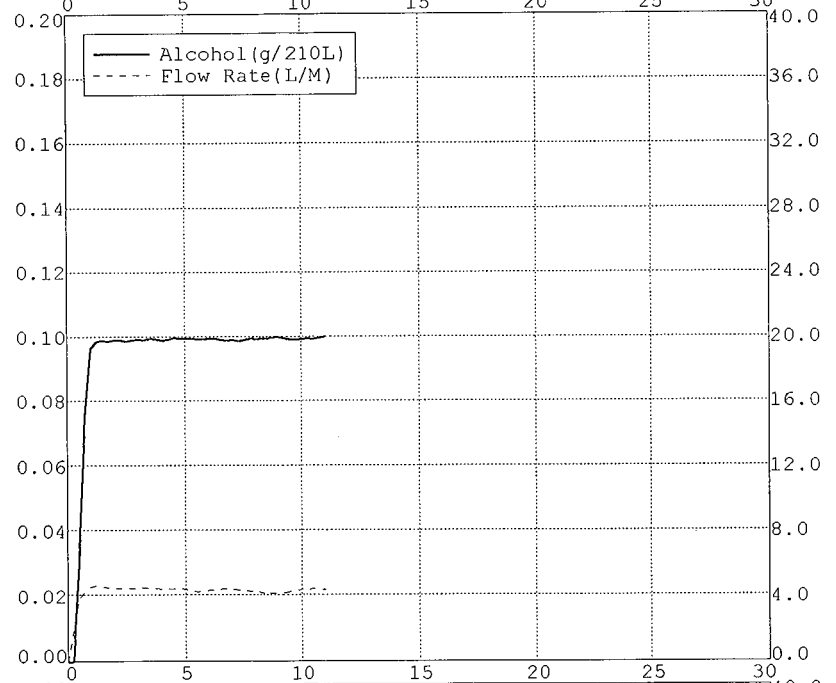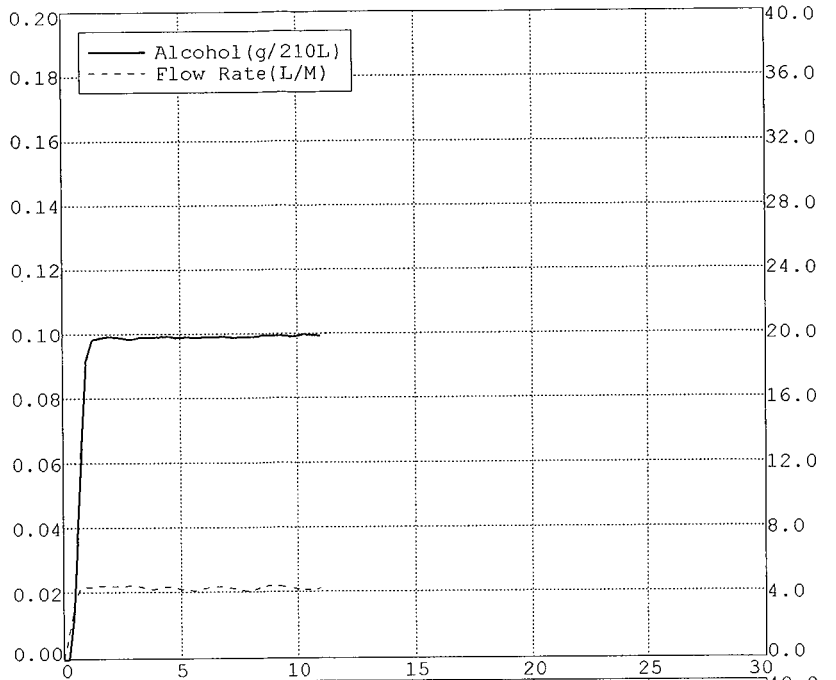

*Hollie B Kennedy, Rome PD 01/11/19*  
*Hollie B Kennedy*

SUPERVISOR TEST



ROME CITY  
POLICE DEPT  
DATAMASTER dmt: 106106

Date: 01/14/2019

OPERATOR NAME:  
HOLLIE B KENNEDY  
Permit #: 39044  
Operator Agency/Dept: ROME CITY PD  
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:18
INTERNAL STANDARD	VERIFIED	14:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:19
BLANK TEST	0.00	14:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:20
BLANK TEST	0.00	14:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:21
BLANK TEST	0.00	14:22

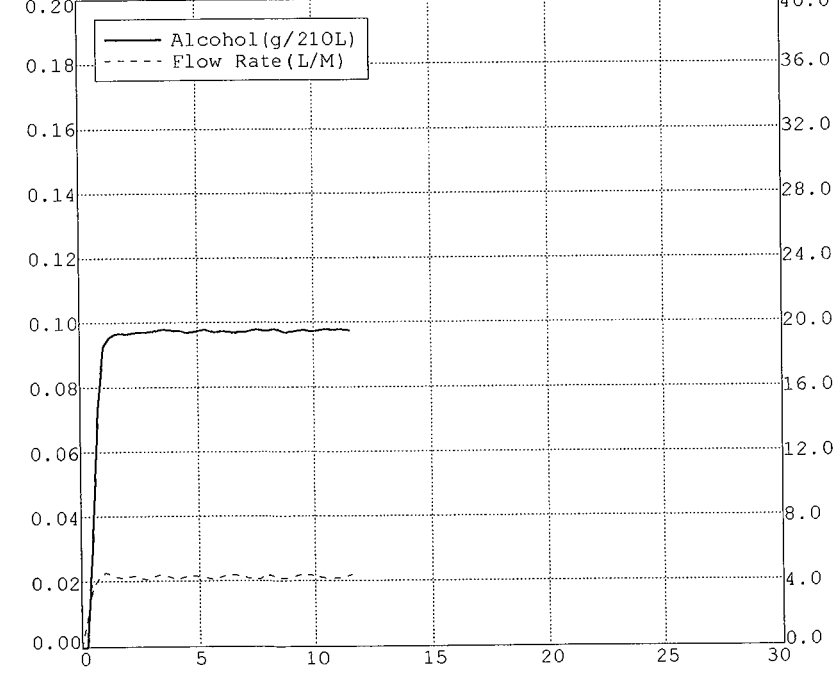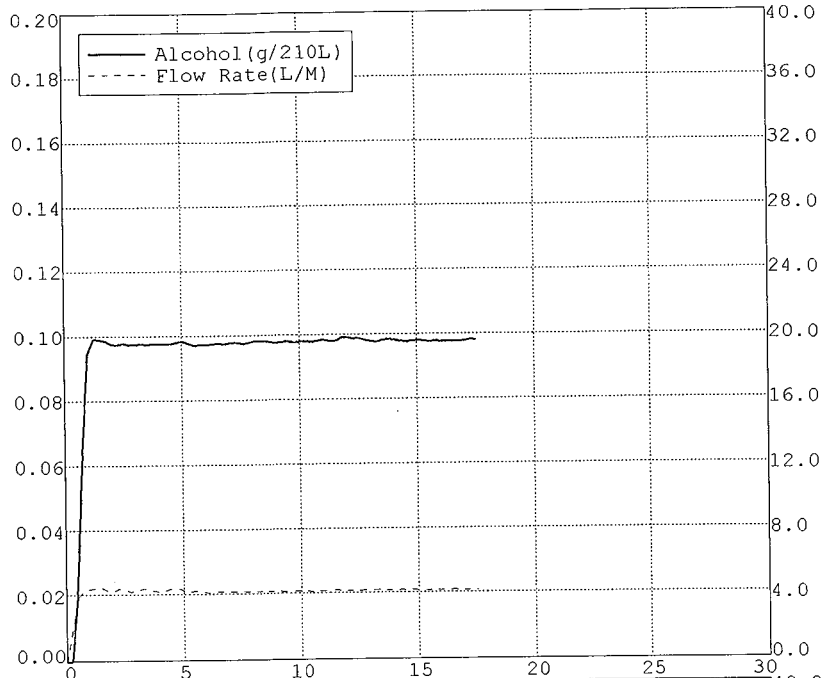

Hollie Kennedy Rome PD 01/14/19  
Hollie Kennedy 106106

SUPERVISOR TEST



ROME CITY  
POLICE DEPT  
DATAMASTER dmt: 106106

Date: 01/18/2019

OPERATOR NAME:  
HOLLIE B KENNEDY  
Permit #: 39044  
Operator Agency/Dept: ROME CITY PD  
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:35
INTERNAL STANDARD	VERIFIED	19:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:35
BLANK TEST	0.00	19:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:36
BLANK TEST	0.00	19:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:38
BLANK TEST	0.00	19:38

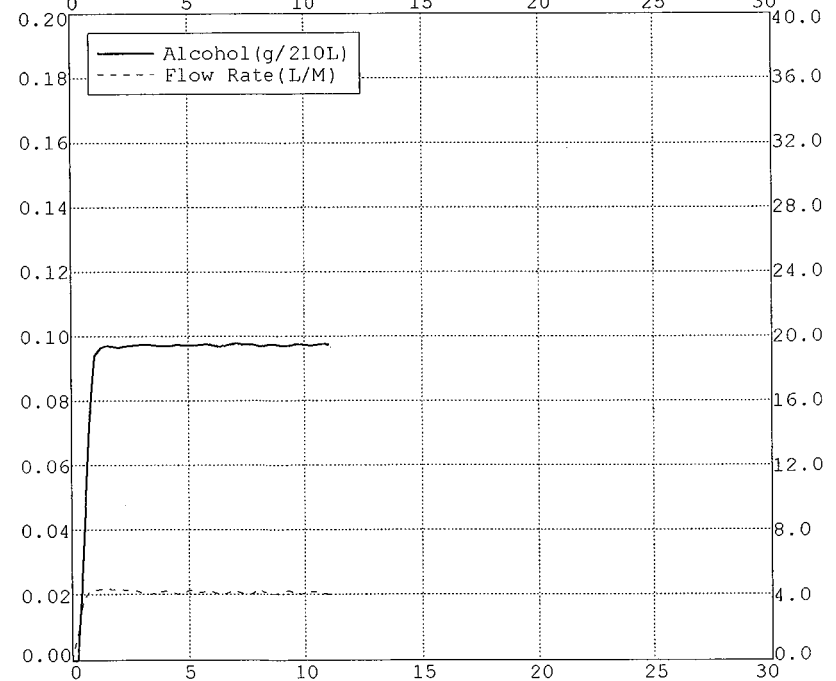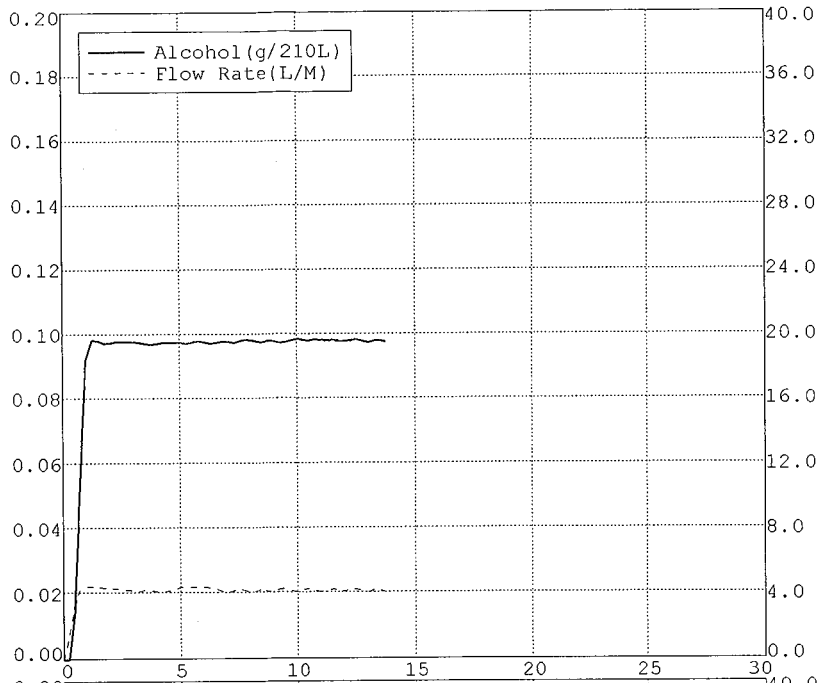

*Hollie Kennedy Rome PD 01/18/19*  
*Amelia 1085*

SUPERVISOR TEST




ROME CITY  
 POLICE DEPT  
 DATAMASTER dmt: 106106

Date: 01/25/2019

OPERATOR NAME:  
 HOLLIE B KENNEDY  
 Permit #: 39044  
 Operator Agency/Dept: ROME CITY PD  
 Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:02
INTERNAL STANDARD	VERIFIED	16:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:02
BLANK TEST	0.00	16:03
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:03
BLANK TEST	0.00	16:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:04
BLANK TEST	0.00	16:05

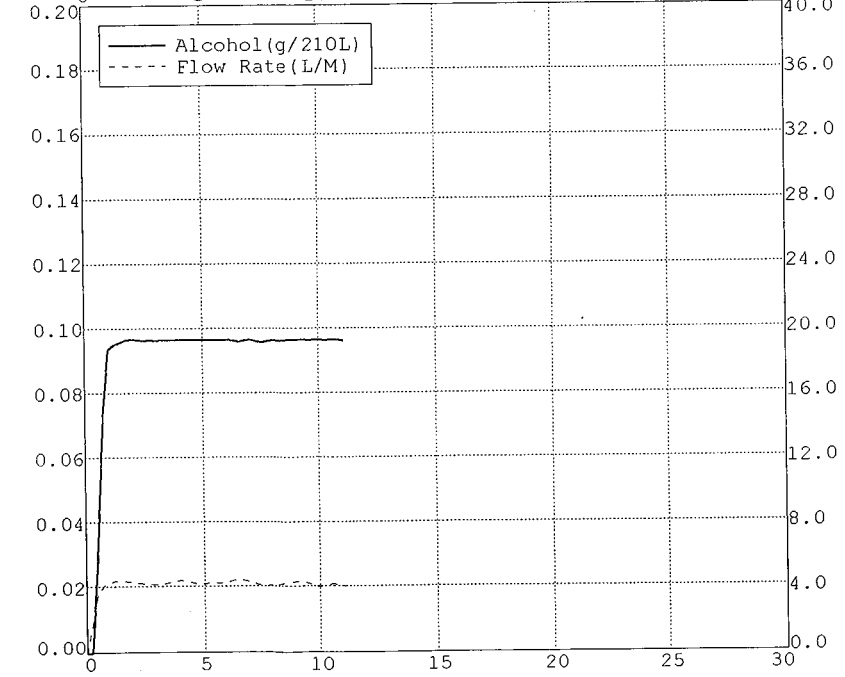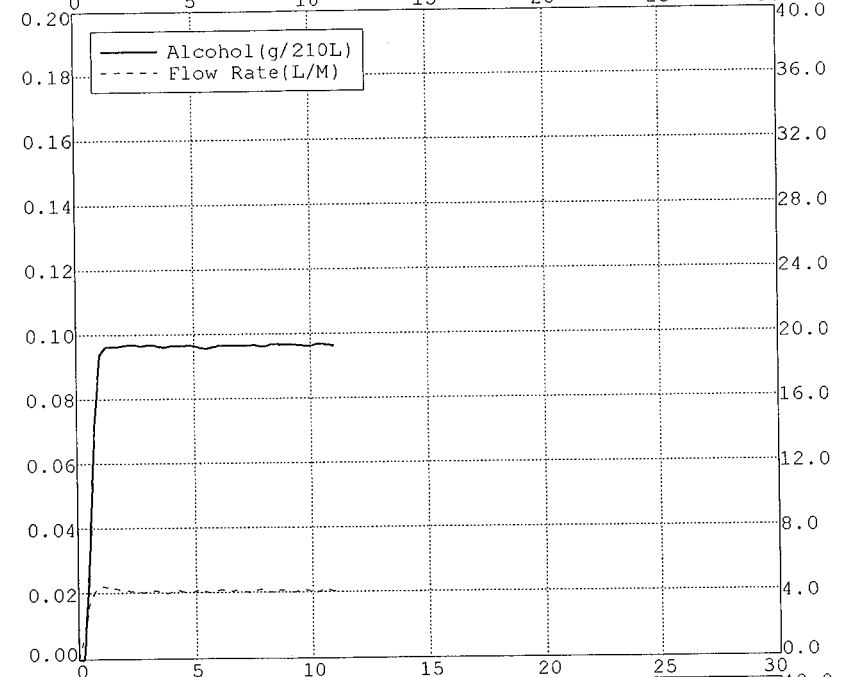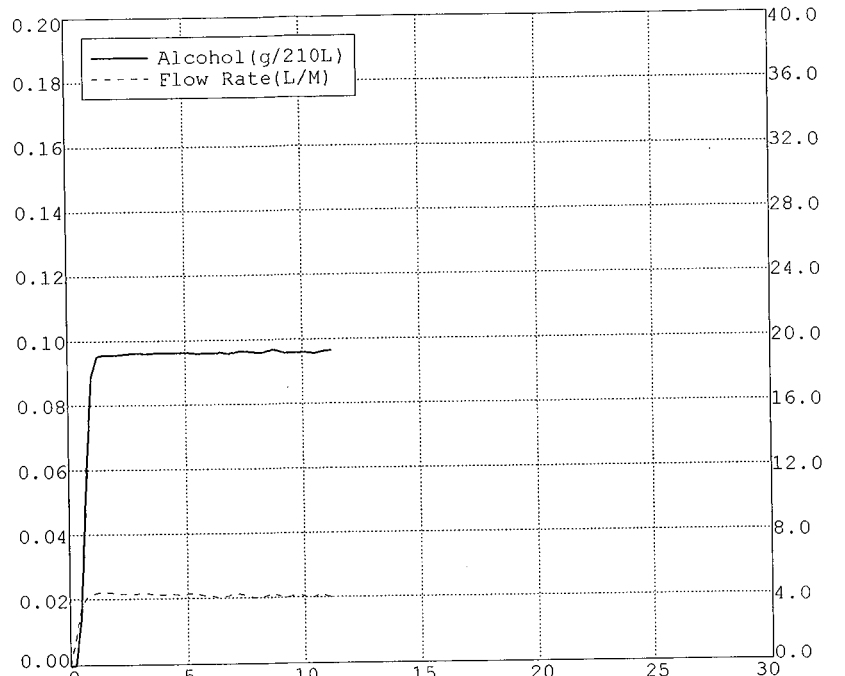

*Hollie Kennedy Rome PD 01/25/19*  
*Hollie Kennedy 16:05*