

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 02/07/2020

OPERATOR NAME:
HOLLIE B SILVERMAN
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:05
INTERNAL STANDARD	VERIFIED	16:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:05
BLANK TEST	0.00	16:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:06
BLANK TEST	0.00	16:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:07
BLANK TEST	0.00	16:08

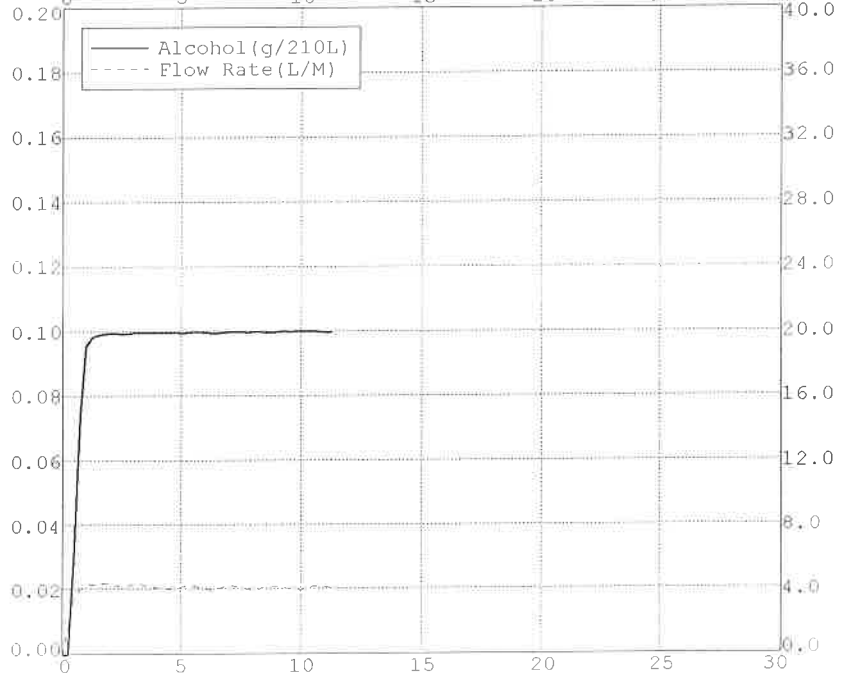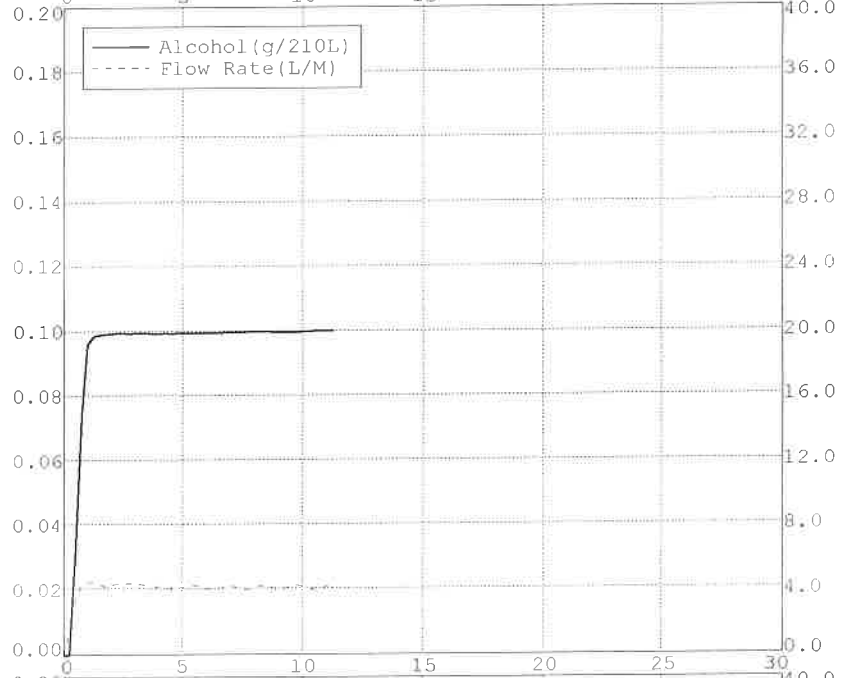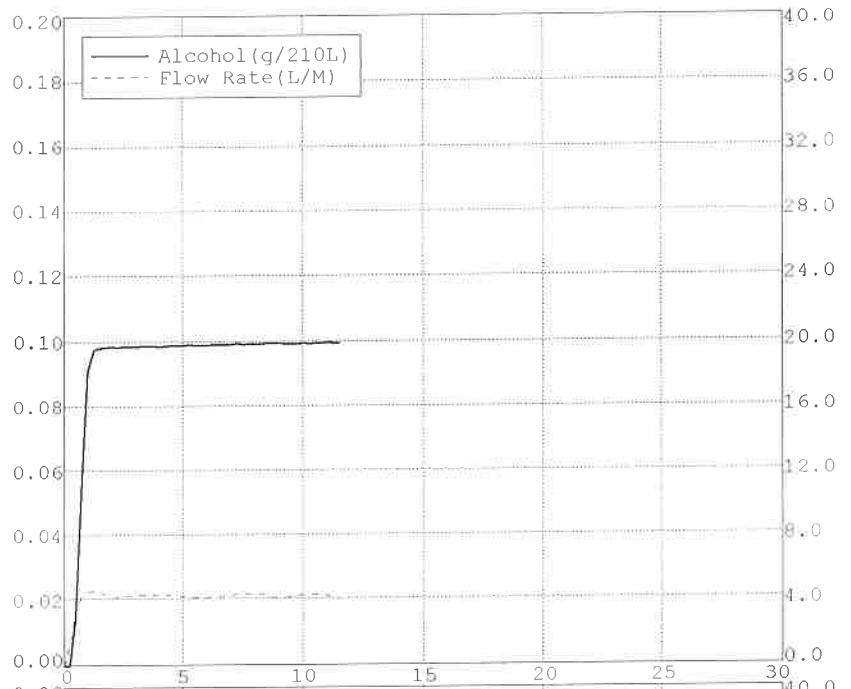

RH Hollie B Silverman Rome PD 02/07/2020

~~RH Hollie B Silverman~~ 10805