

SOLUTION CHANGE

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308




Date: 12/02/2019

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 19250

RM
19-45792

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:24
INTERNAL STANDARD	VERIFIED	13:24
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	13:25
BLANK TEST	0.00	13:26
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	13:26
BLANK TEST	0.00	13:27
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	13:27
BLANK TEST	0.00	13:28

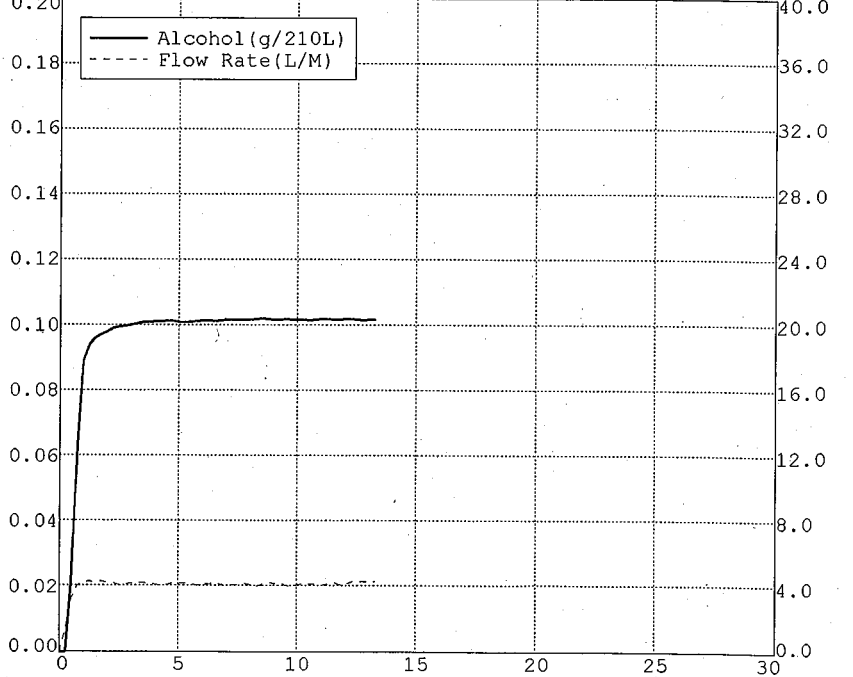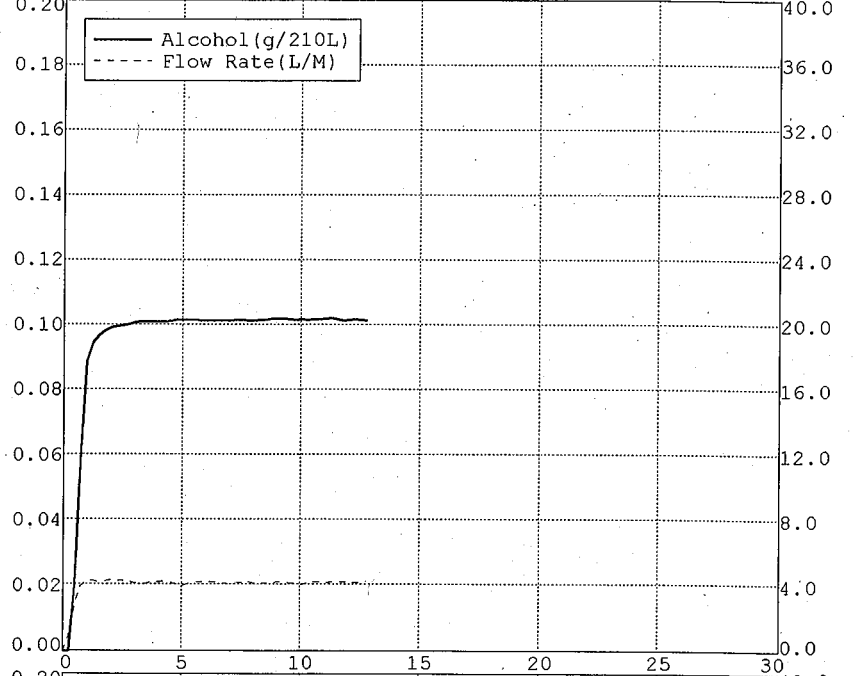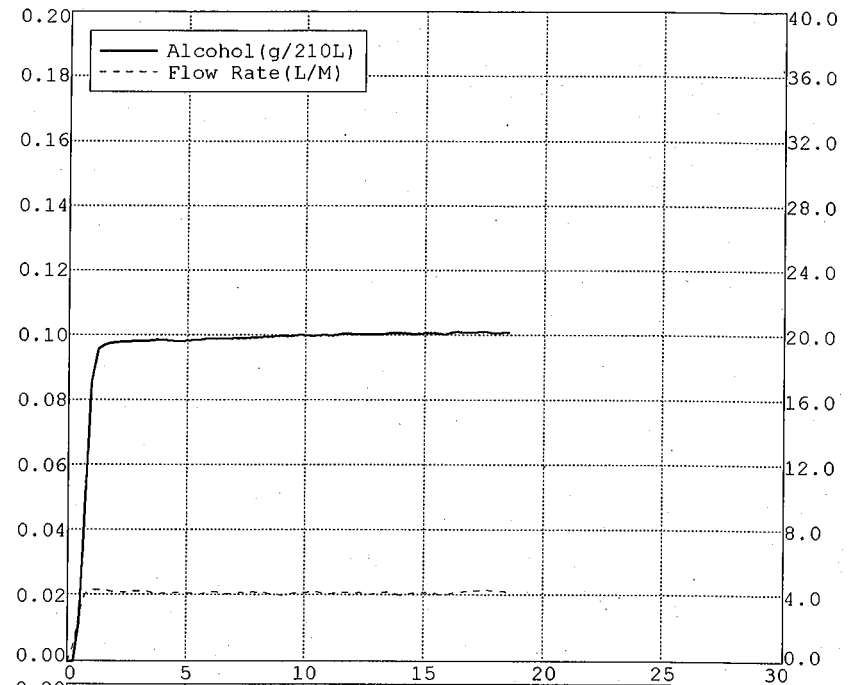

SOLUTION CHANGE

UTICA CITY
 POLICE DEPT
 DATAMASTER dmt: 100282

Date: 12/02/2019

OPERATOR NAME:
 MICHAEL J CLIVE
 Permit #: 36682
 Operator Agency/Dept: UTICA CITY PD
 Reference Standard #: 19250

RMJ
19-45792

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:44
INTERNAL STANDARD	VERIFIED	11:44
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	11:44
BLANK TEST	0.00	11:45
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	11:45
BLANK TEST	0.00	11:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:46
BLANK TEST	0.00	11:47

