

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308




Date: 11/19/2019

RMS
19-44319

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:23
INTERNAL STANDARD	VERIFIED	13:23
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	13:23
BLANK TEST	0.00	13:24
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	13:25
BLANK TEST	0.00	13:25
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	13:26
BLANK TEST	0.00	13:27

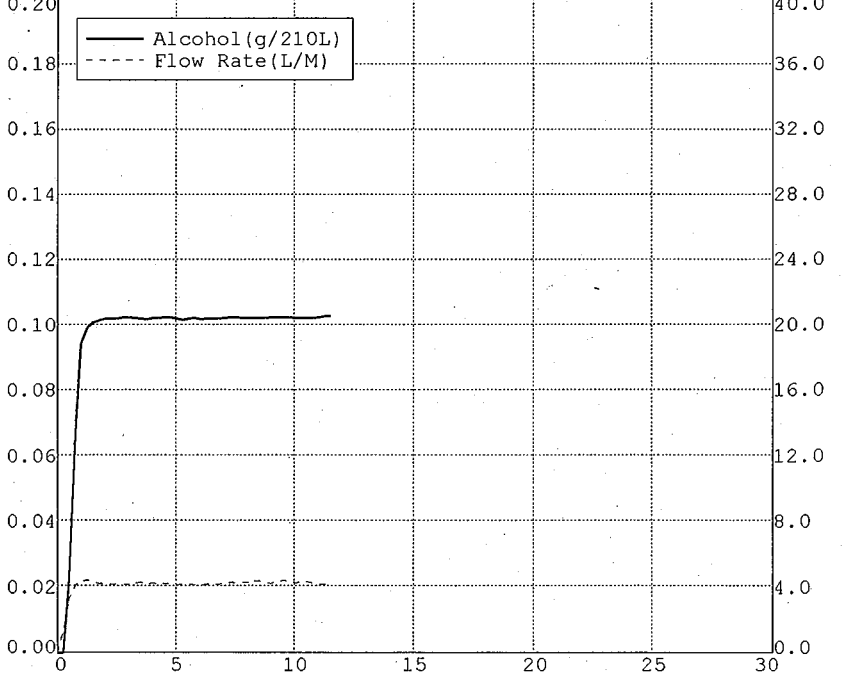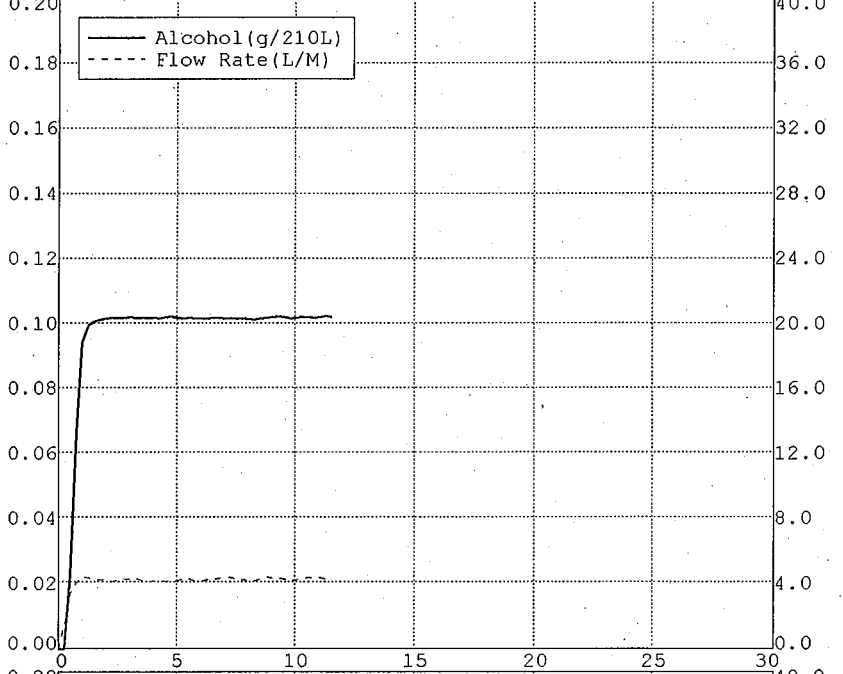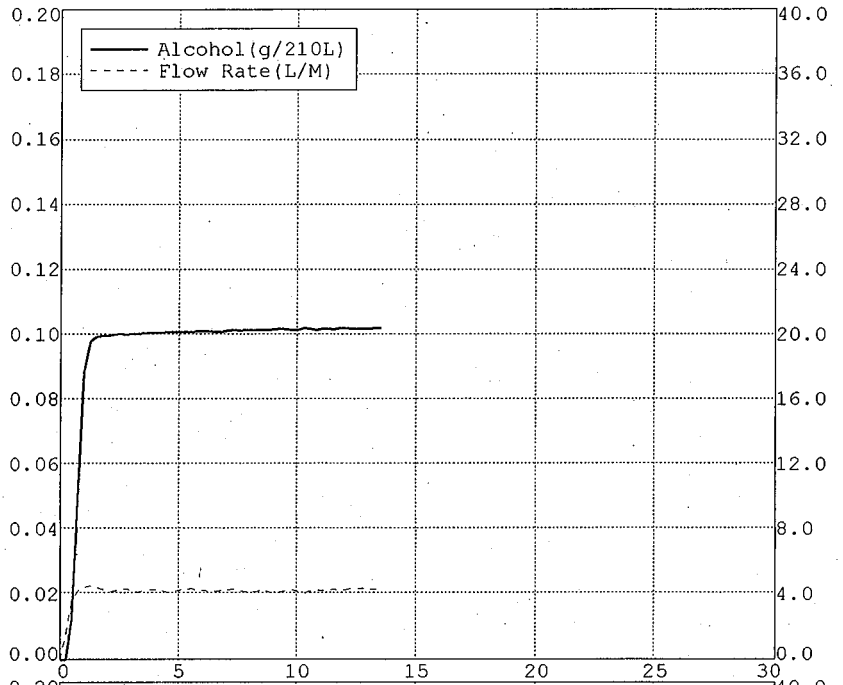

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282

Date: 11/19/2019

RMS
19-44319

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:26
INTERNAL STANDARD	VERIFIED	12:26
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	12:26
BLANK TEST	0.00	12:27
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	12:28
BLANK TEST	0.00	12:28
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	12:29
BLANK TEST	0.00	12:30

