

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308




Date: 12/17/2019

RMJ
19-47558

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:13
INTERNAL STANDARD	VERIFIED	11:14
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:14
BLANK TEST	0.00	11:15
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:15
BLANK TEST	0.00	11:16
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:16
BLANK TEST	0.00	11:17

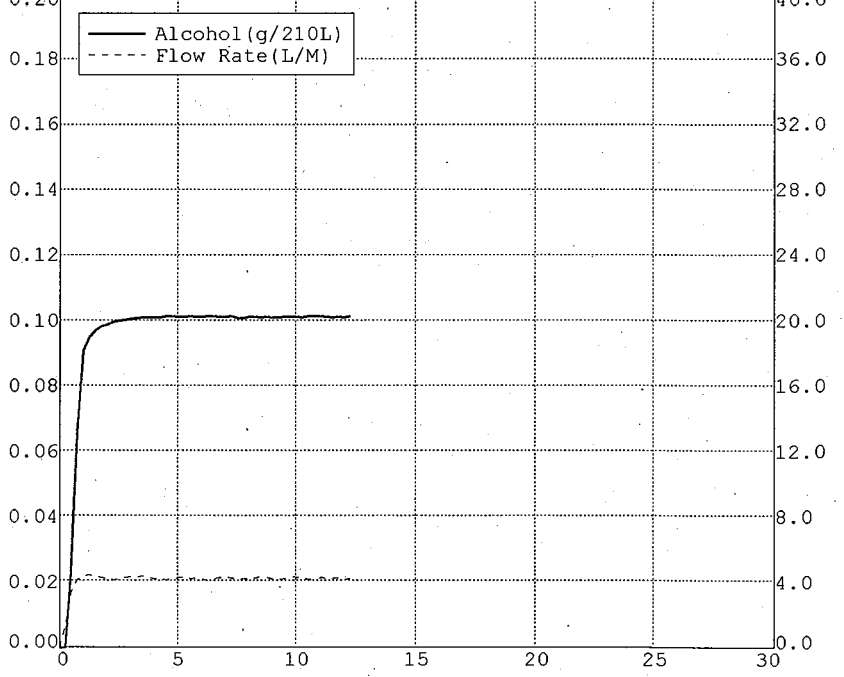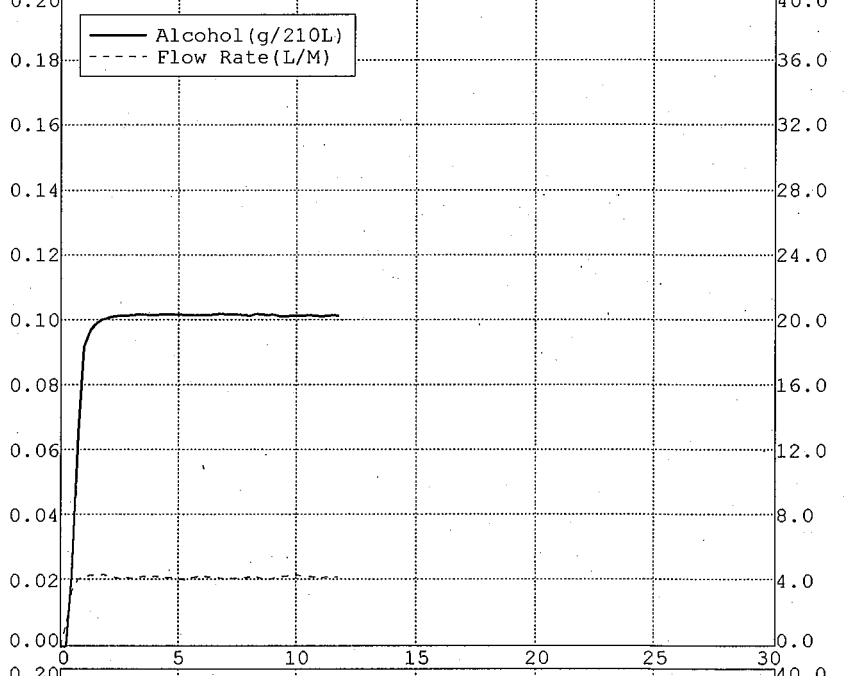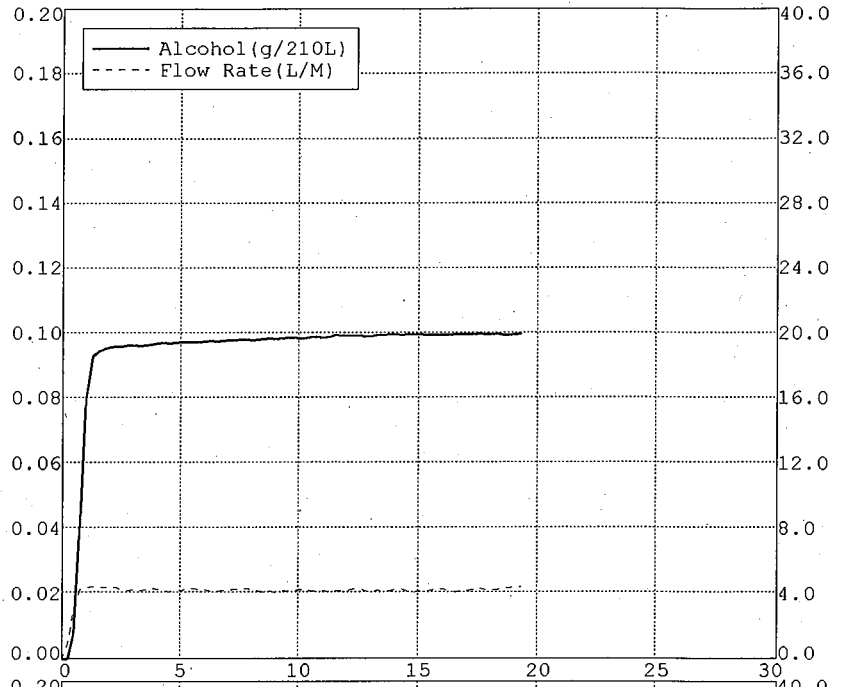

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282

Date: 12/17/2019

RMS
19-47558

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:09
INTERNAL STANDARD	VERIFIED	09:09
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	09:09
BLANK TEST	0.00	09:10
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	09:10
BLANK TEST	0.00	09:11
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	09:12
BLANK TEST	0.00	09:12

