

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308




Date: 01/28/2020

RM>
20-3024

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:06
INTERNAL STANDARD	VERIFIED	12:06
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:07
BLANK TEST	0.00	12:07
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:08
BLANK TEST	0.00	12:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:09
BLANK TEST	0.00	12:10

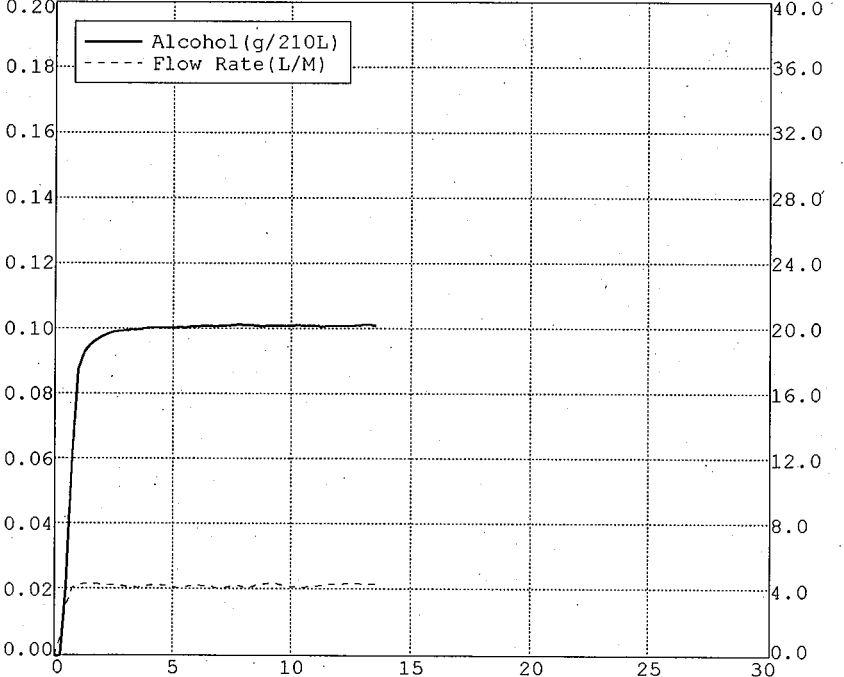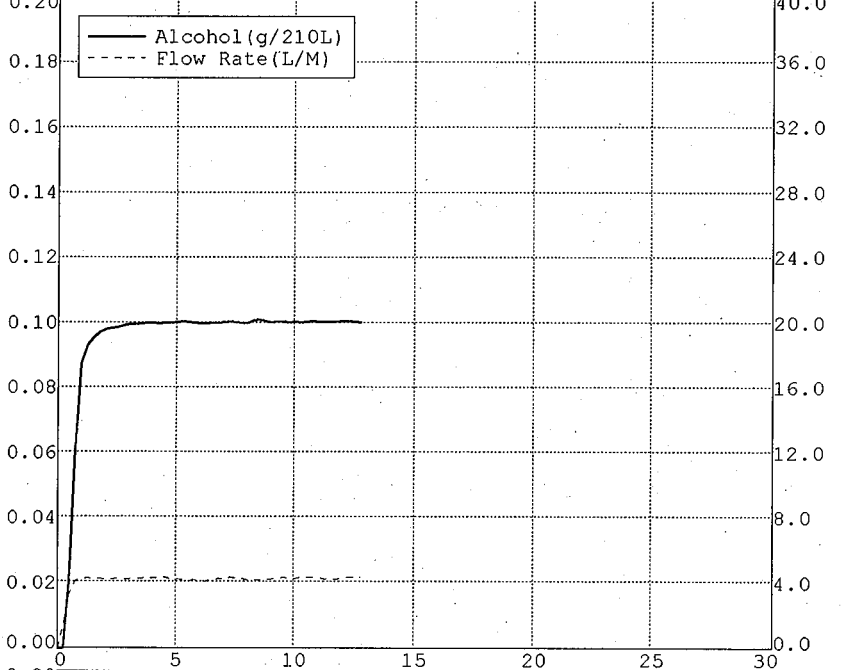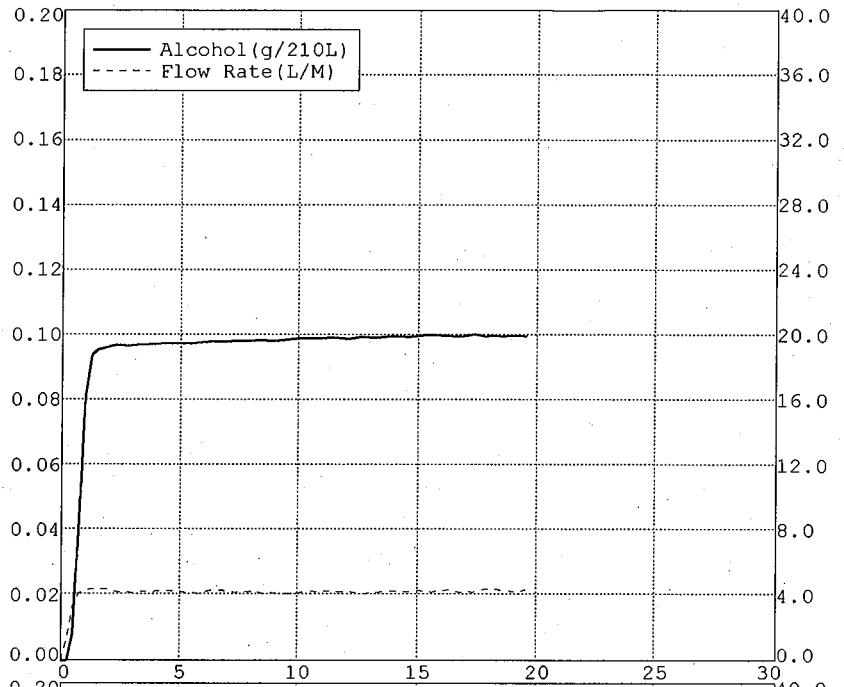

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282

Date: 01/28/2020

*RMS
20-3024*

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:31
INTERNAL STANDARD	VERIFIED	11:31
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	11:31
BLANK TEST	0.00	11:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:32
BLANK TEST	0.00	11:33
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	11:34
BLANK TEST	0.00	11:34

