

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308




Date: 05/05/2020

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 20040

RMS
20-14659

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:47
INTERNAL STANDARD	VERIFIED	12:47
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:47
BLANK TEST	0.00	12:48
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:48
BLANK TEST	0.00	12:49
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:49
BLANK TEST	0.00	12:50

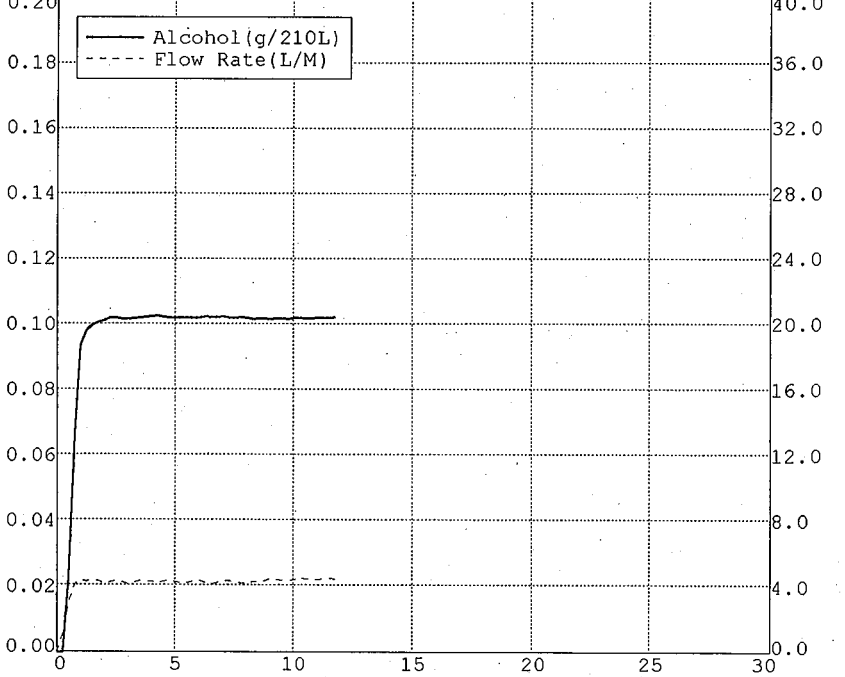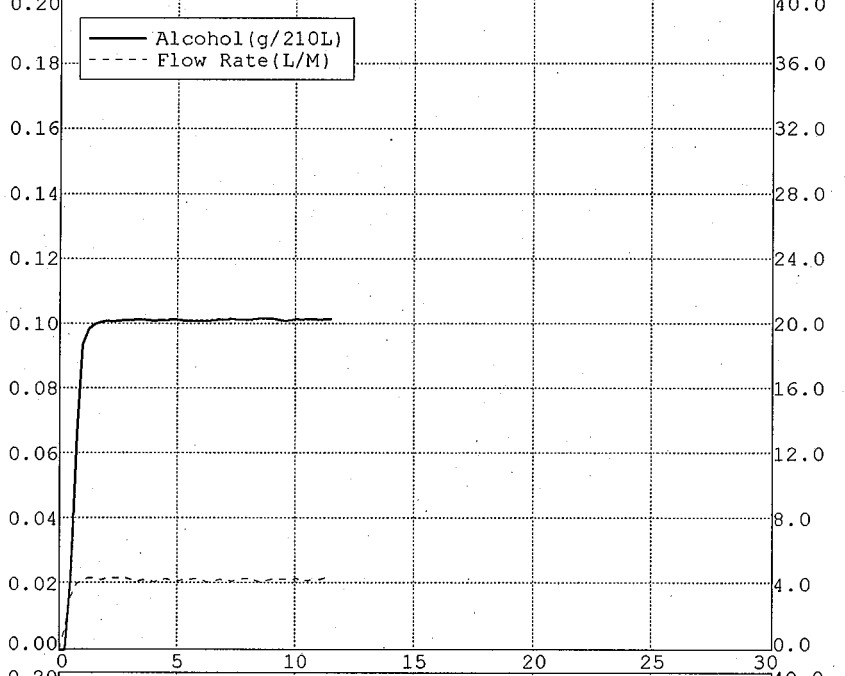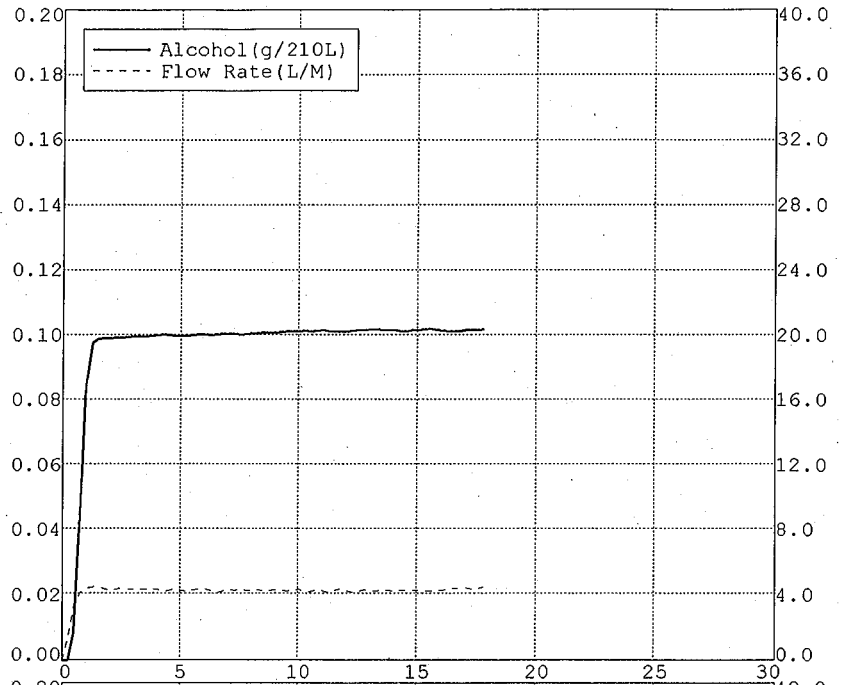

SUPERVISOR TEST

UTICA CITY
 POLICE DEPT
 DATAMASTER dmt: 100282

RMS
20-14659

Date: 05/05/2020

OPERATOR NAME:
 MICHAEL J CLIVE
 Permit #: 36682
 Operator Agency/Dept: UTICA CITY PD
 Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:50
INTERNAL STANDARD	VERIFIED	11:50
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	11:50
BLANK TEST	0.00	11:51
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	11:52
BLANK TEST	0.00	11:52
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	11:53
BLANK TEST	0.00	11:54

