

SUPERVISOR TEST

UTICA CITY
 POLICE DEPT
 DATAMASTER dmt: 107308




RM3
20-6505

Date: 02/25/2020

OPERATOR NAME:
 MICHAEL J CLIVE
 Permit #: 36682
 Operator Agency/Dept: UTICA CITY PD
 Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:24
INTERNAL STANDARD	VERIFIED	12:24
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:24
BLANK TEST	0.00	12:25
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:25
BLANK TEST	0.00	12:26
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:26
BLANK TEST	0.00	12:27

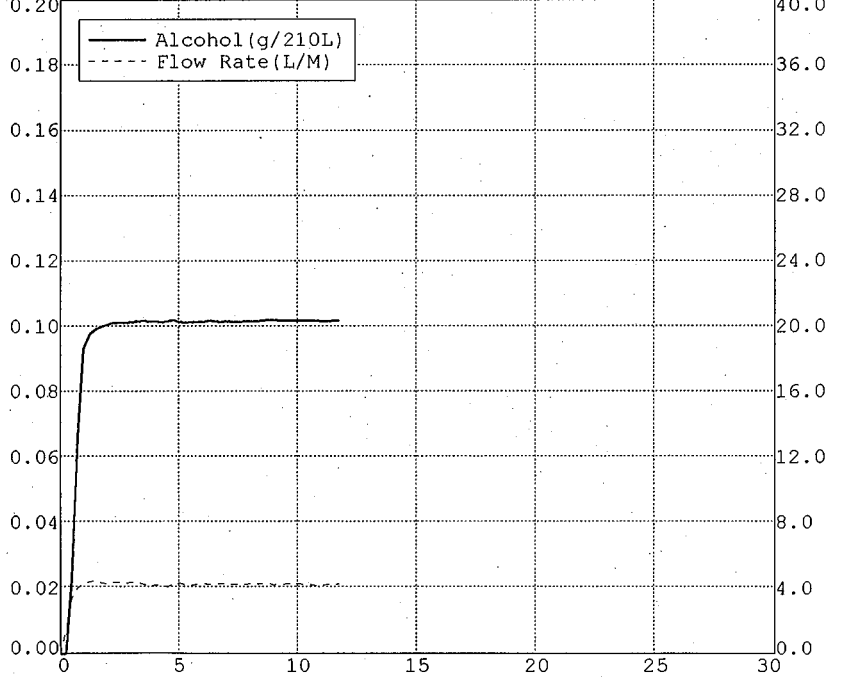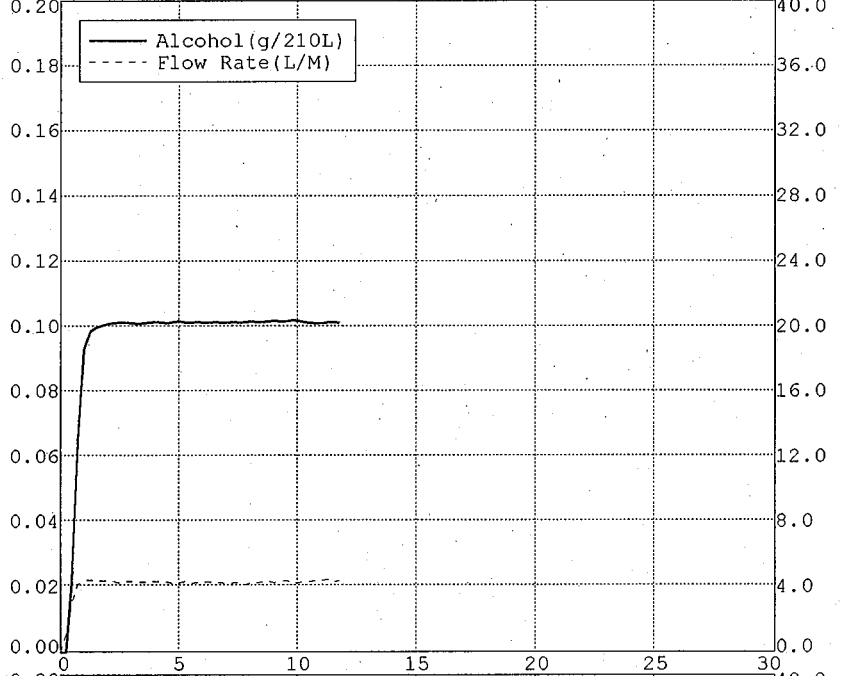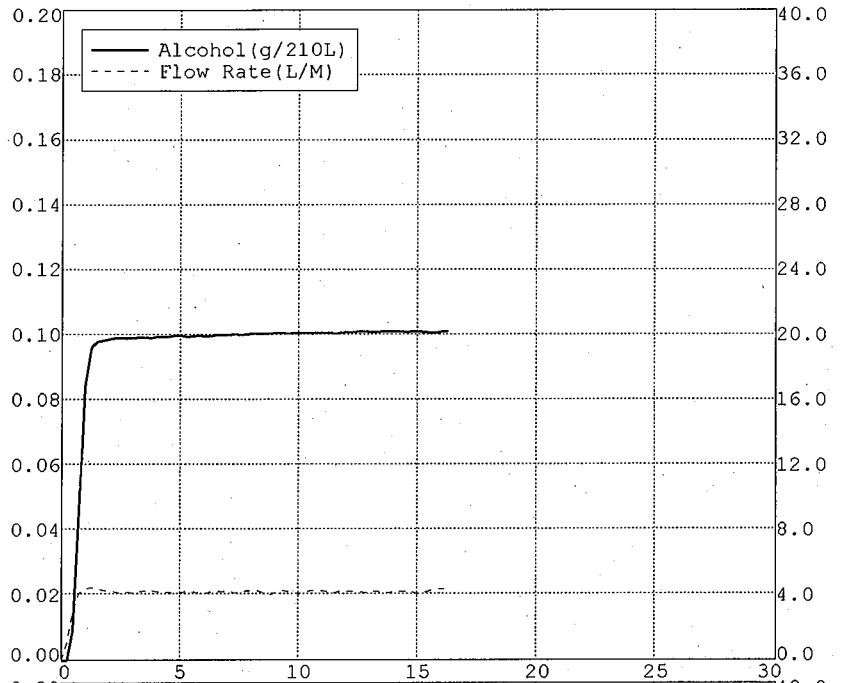

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282

Date: 02/25/2020

*RMS
20-6505*

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:04
INTERNAL STANDARD	VERIFIED	12:04
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	12:05
BLANK TEST	0.00	12:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:06
BLANK TEST	0.00	12:07
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	12:07
BLANK TEST	0.00	12:08

