

SUPERVISOR TEST




NEW HARTFORD TOWN
POLICE DEPT
DATAMASTER dmt: 127606

Date: 03/13/2020

OPERATOR NAME:
MICHAEL T KOWALSKI
Permit #: 31077
Operator Agency/Dept: NEW HARTFORD TOWN PD
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:24
INTERNAL STANDARD	VERIFIED	12:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:24
BLANK TEST	0.00	12:25
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:25
BLANK TEST	0.00	12:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:26
BLANK TEST	0.00	12:27

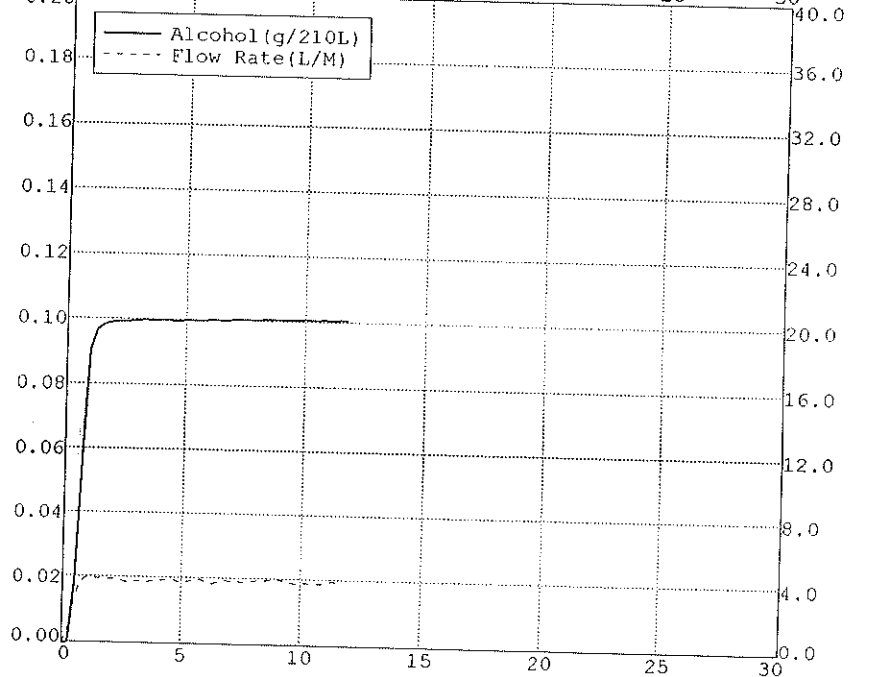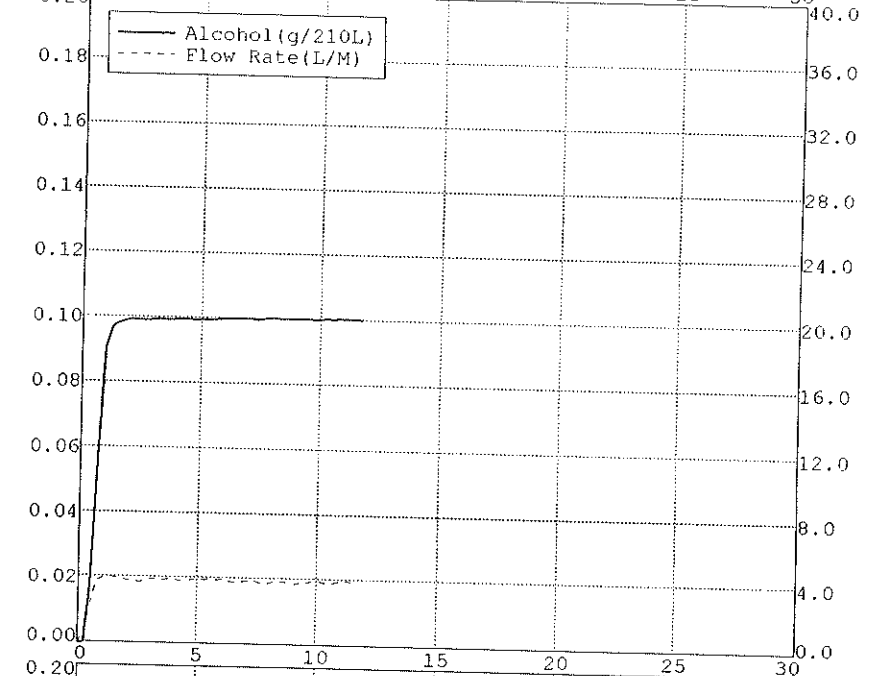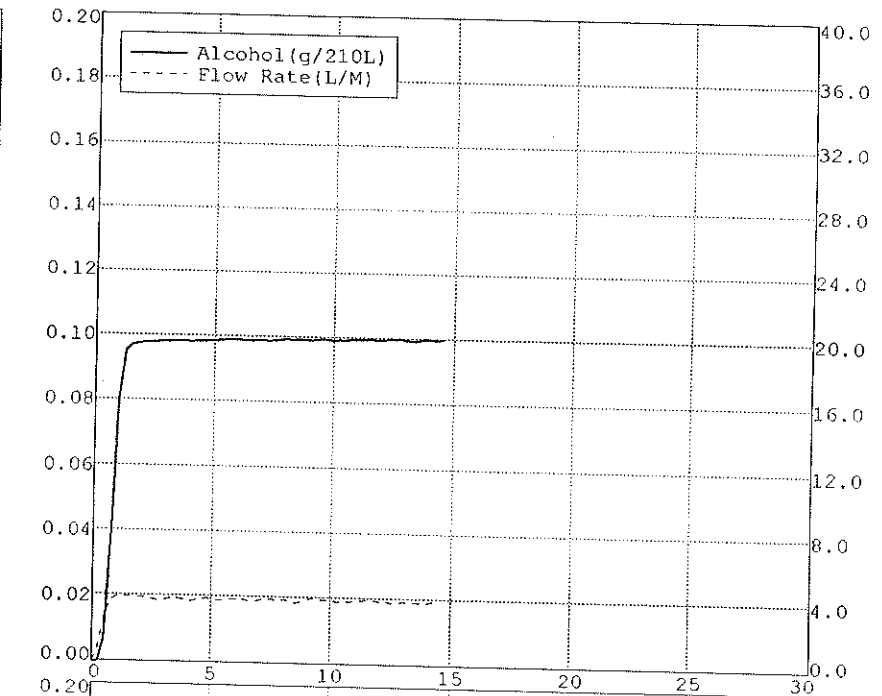

SUPERVISOR TEST




NEW HARTFORD TOWN
POLICE DEPT
DATAMASTER dmt: 127606

Date: 03/20/2020

OPERATOR NAME:
MICHAEL T KOWALSKI
Permit #: 31077
Operator Agency/Dept: NEW HARTFORD TOWN PD
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:20
INTERNAL STANDARD	VERIFIED	07:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:21
BLANK TEST	0.00	07:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:22
BLANK TEST	0.00	07:23
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:23
BLANK TEST	0.00	07:24

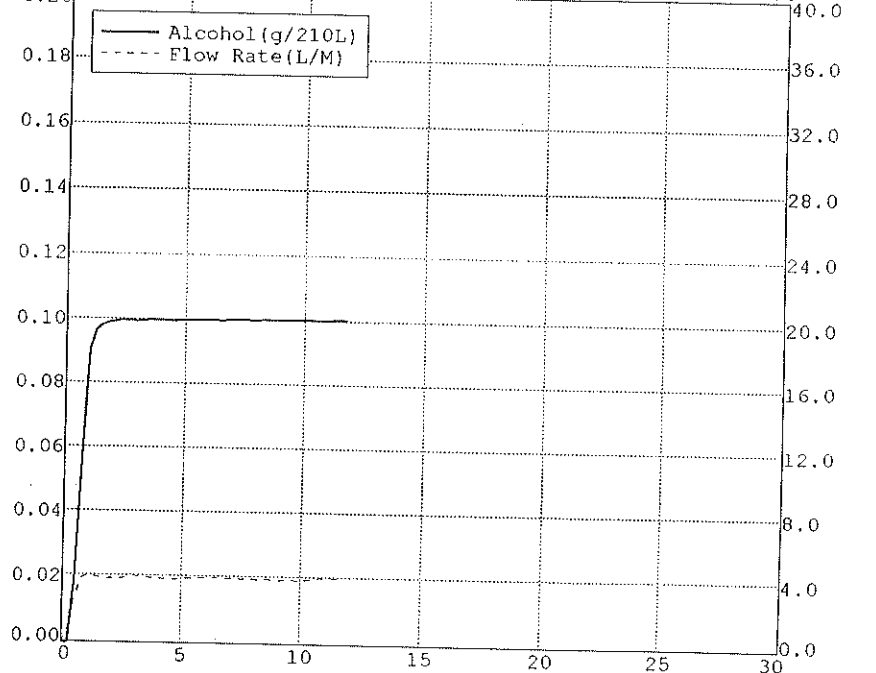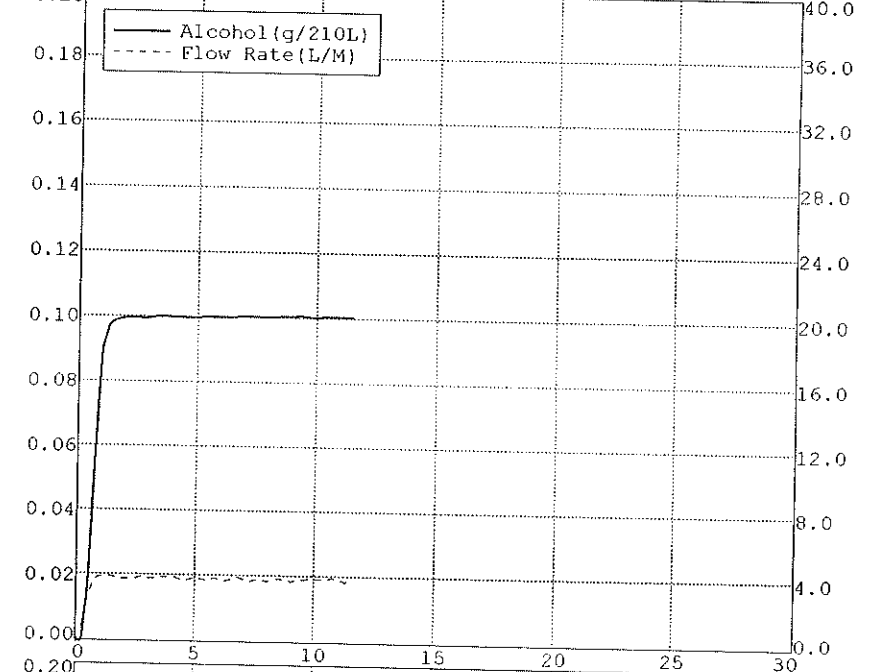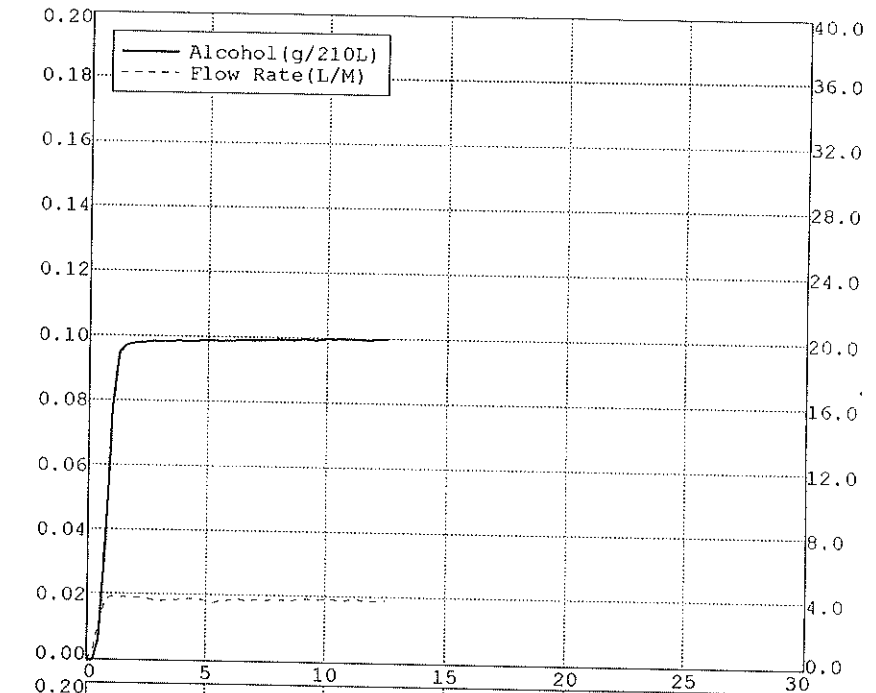

SUPERVISOR TEST




NEW HARTFORD TOWN
POLICE DEPT
DATAMASTER dmt: 127606

Date: 03/27/2020

OPERATOR NAME:
MICHAEL T KOWALSKI
Permit #: 31077
Operator Agency/Dept: NEW HARTFORD TOWN PD
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:34
INTERNAL STANDARD	VERIFIED	15:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:34
BLANK TEST	0.00	15:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:36
BLANK TEST	0.00	15:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:37
BLANK TEST	0.00	15:38

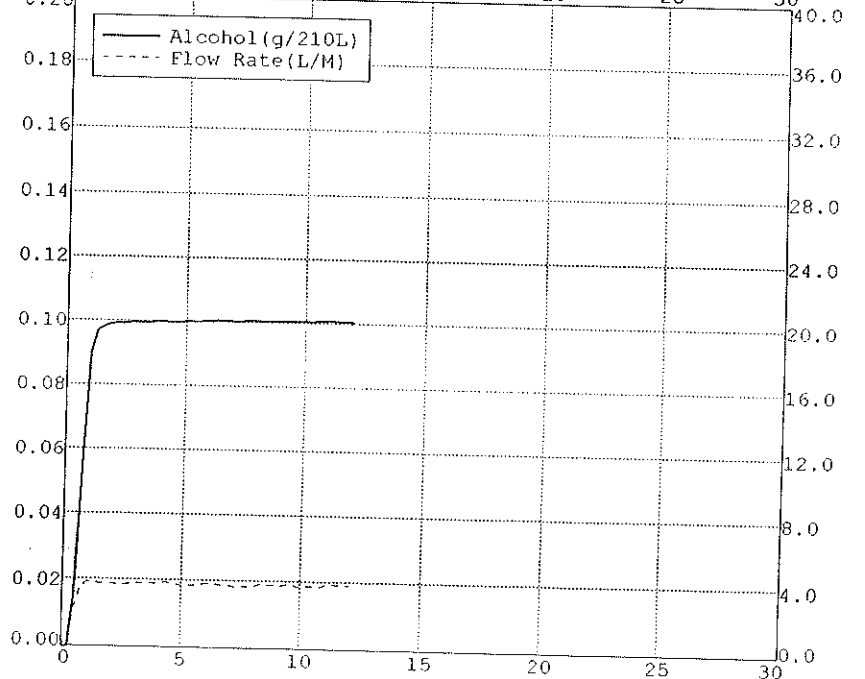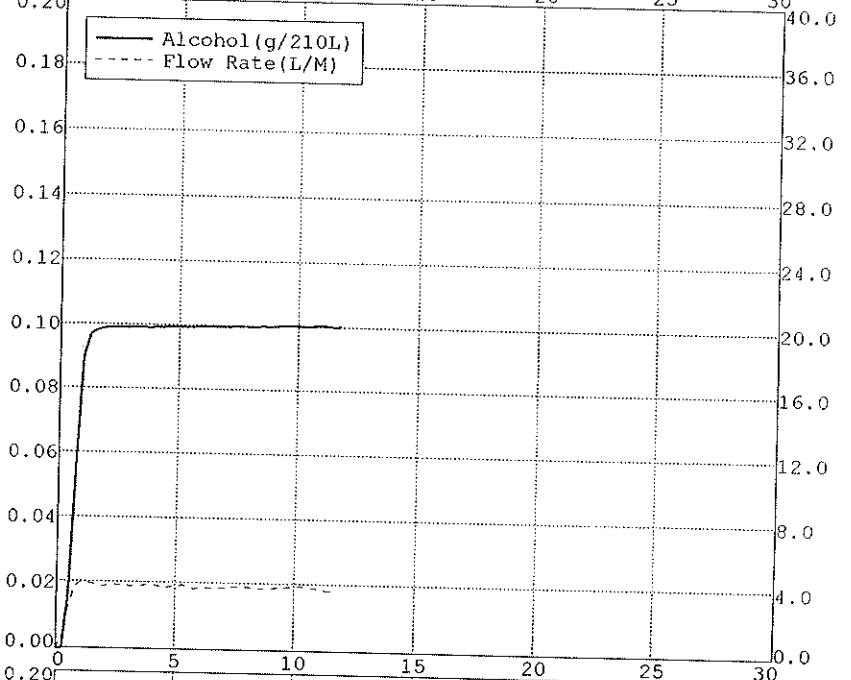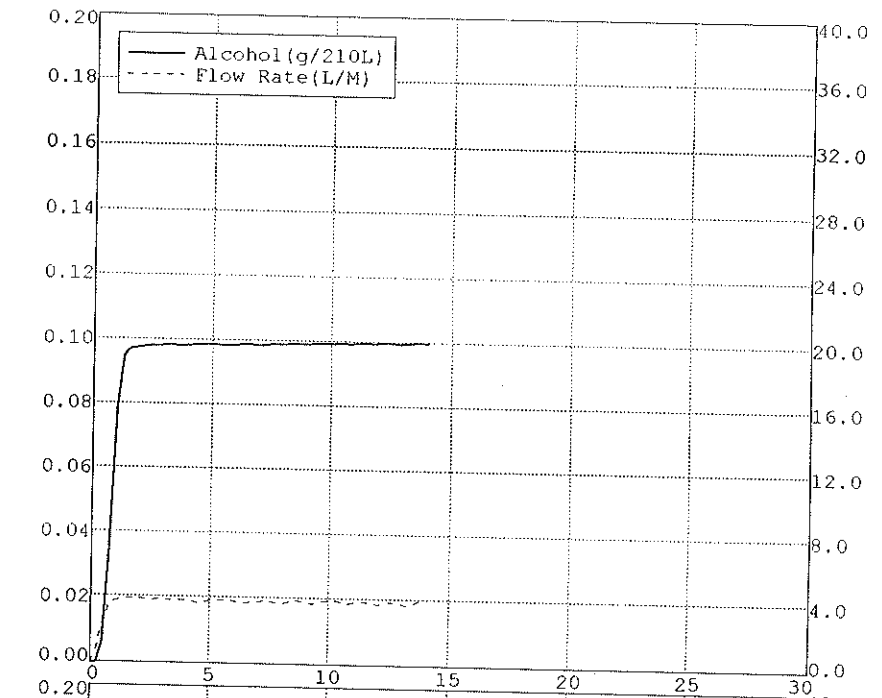

▼ { ◆ → ↕ - ↕ - ↕ B

SOLUTION CHANGE




NEW HARTFORD TOWN
 POLICE DEPT
 DATAMASTER dmt: 127606

Date: 03/31/2020

OPERATOR NAME:
 MICHAEL T KOWALSKI
 Permit #: 31077
 Operator Agency/Dept: NEW HARTFORD TOWN PD
 Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:08
INTERNAL STANDARD	VERIFIED	15:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:09
BLANK TEST	0.00	15:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:10
BLANK TEST	0.00	15:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:11
BLANK TEST	0.00	15:12

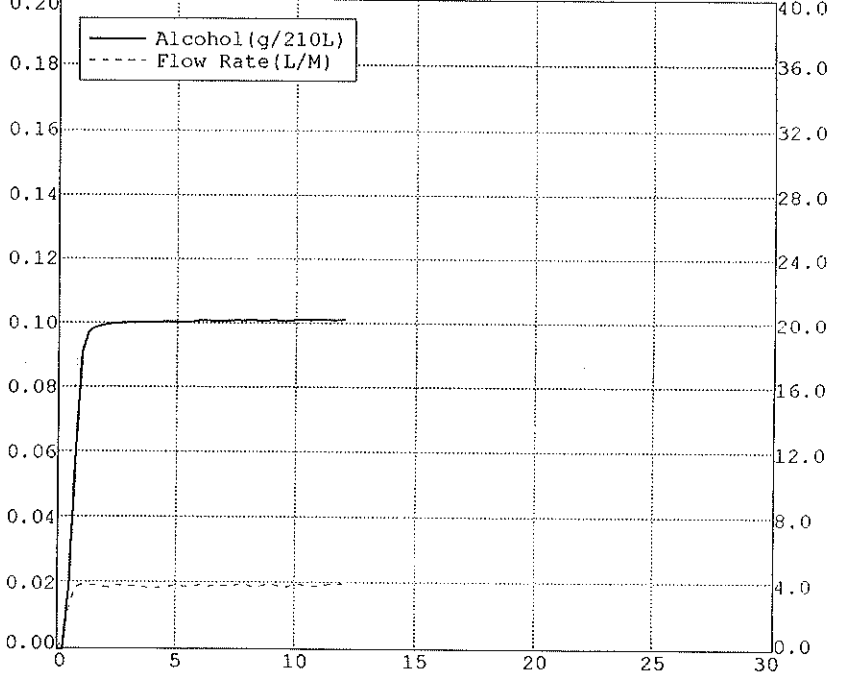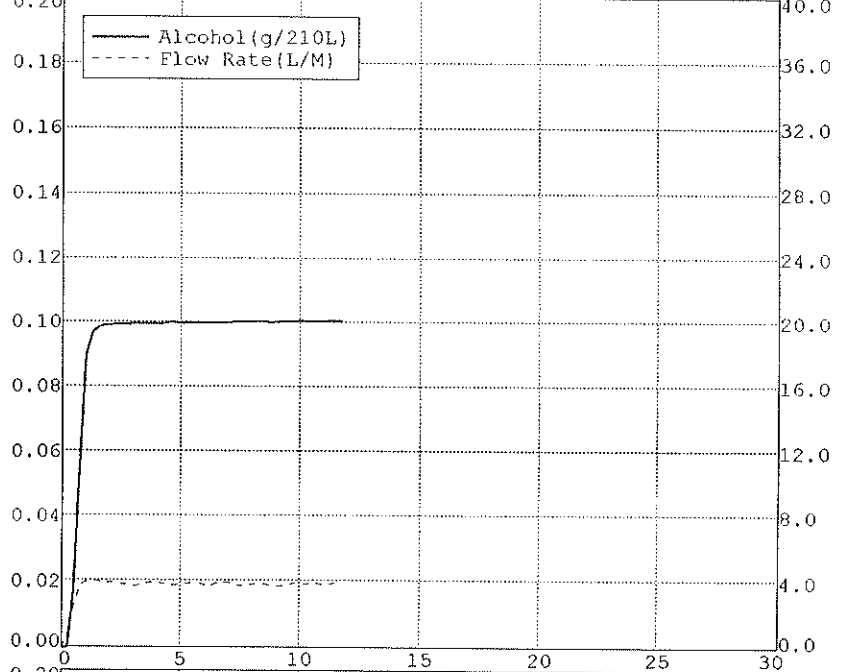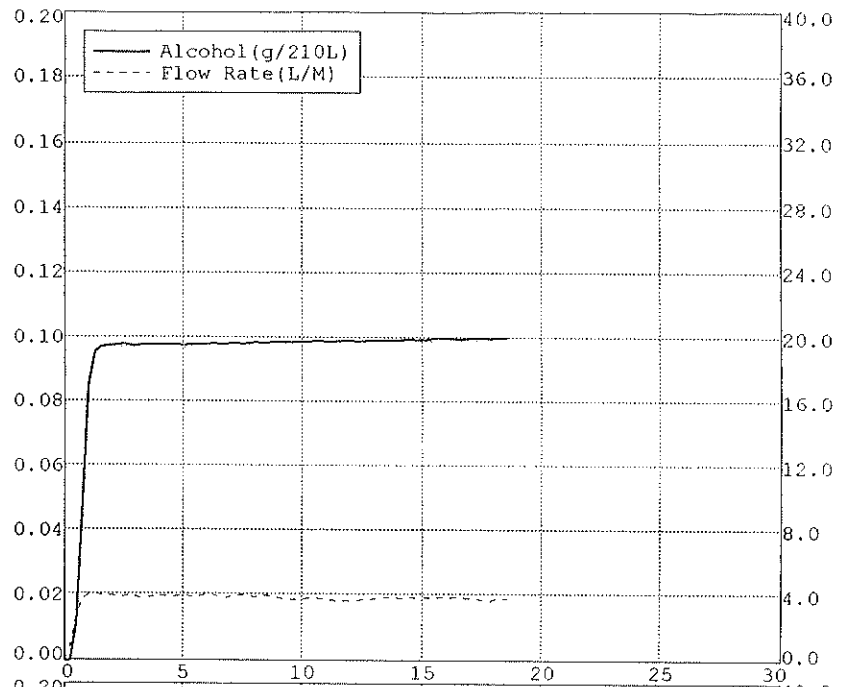

SUPERVISOR TEST

NEW HARTFORD TOWN
POLICE DEPT
DATAMASTER dmt: 127606

Date: 04/07/2020

OPERATOR NAME:
MICHAEL T KOWALSKI
Permit #: 31077
Operator Agency/Dept: NEW HARTFORD TOWN PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:07
INTERNAL STANDARD	VERIFIED	19:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	19:08
BLANK TEST	0.00	19:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	19:09
BLANK TEST	0.00	19:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	19:10
BLANK TEST	0.00	19:11

