

SUPERVISOR TEST

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 141906




Date: 02/19/2020

OPERATOR NAME:
EDWARD F CONSTANTINE
Permit #: 45980
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:44
INTERNAL STANDARD	VERIFIED	18:44
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	18:44
BLANK TEST	0.00	18:45
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	18:46
BLANK TEST	0.00	18:46
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	18:47
BLANK TEST	0.00	18:48

BFO

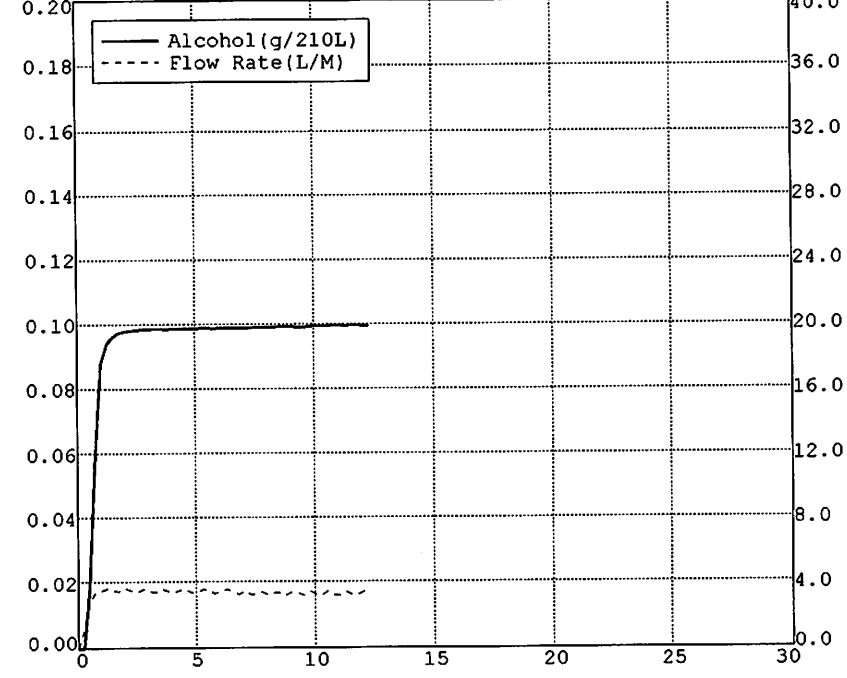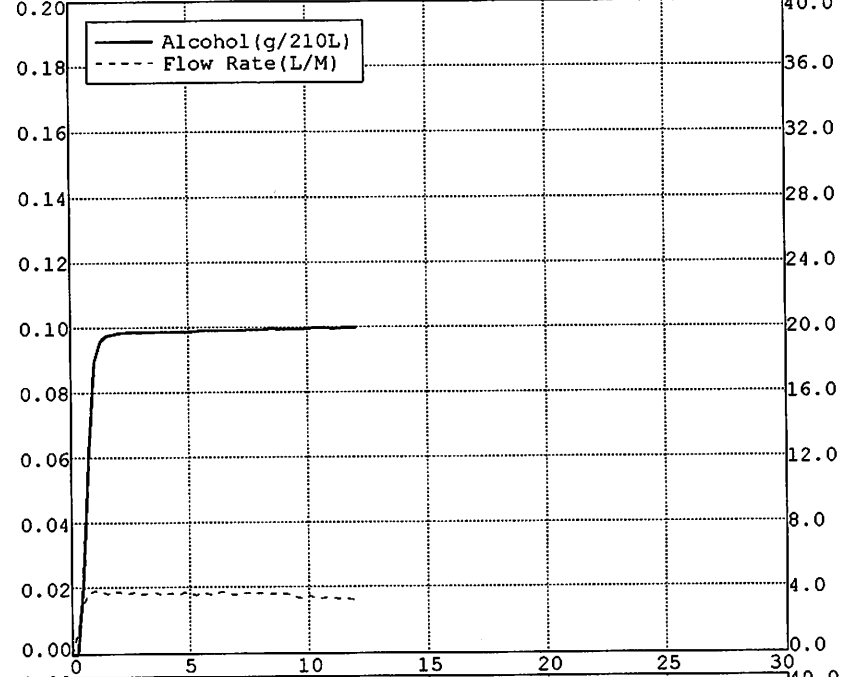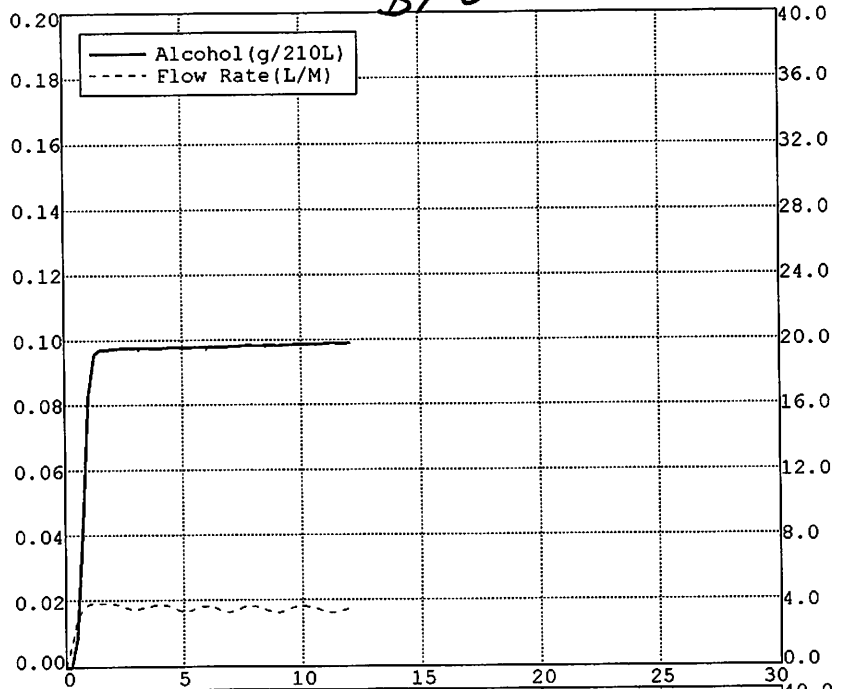

BFO

SUPERVISOR TEST




ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 141906

Date: 02/27/2020

OPERATOR NAME:
LEONARD F DILLENBECK
Permit #: 47621
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:07
INTERNAL STANDARD	VERIFIED	00:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:07
BLANK TEST	0.00	00:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:09
BLANK TEST	0.00	00:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:10
BLANK TEST	0.00	00:11

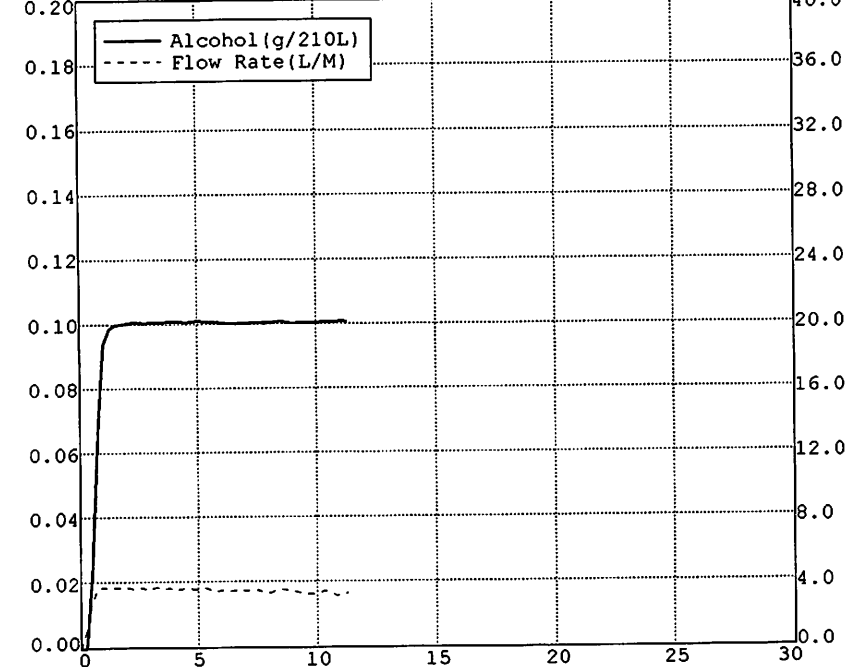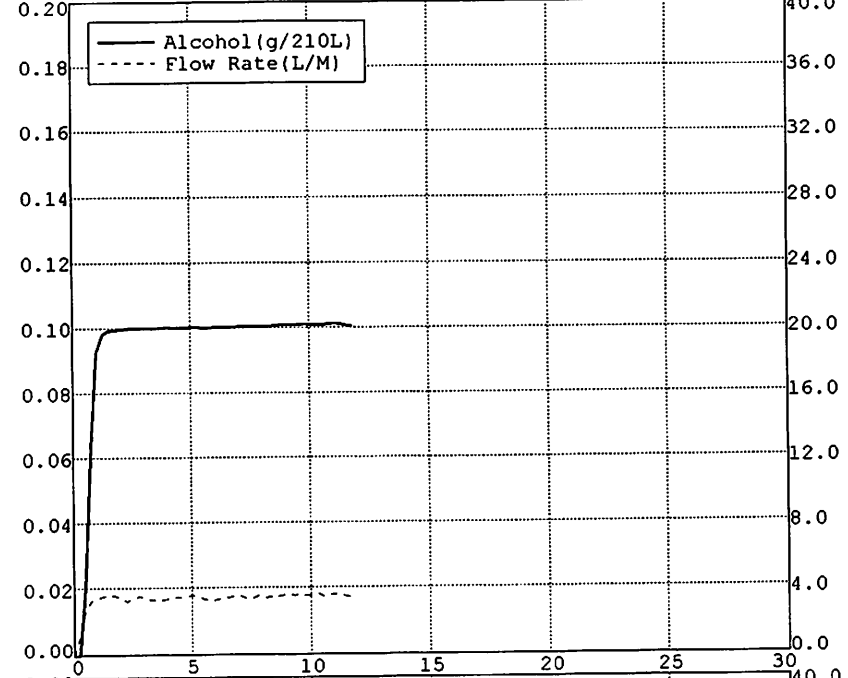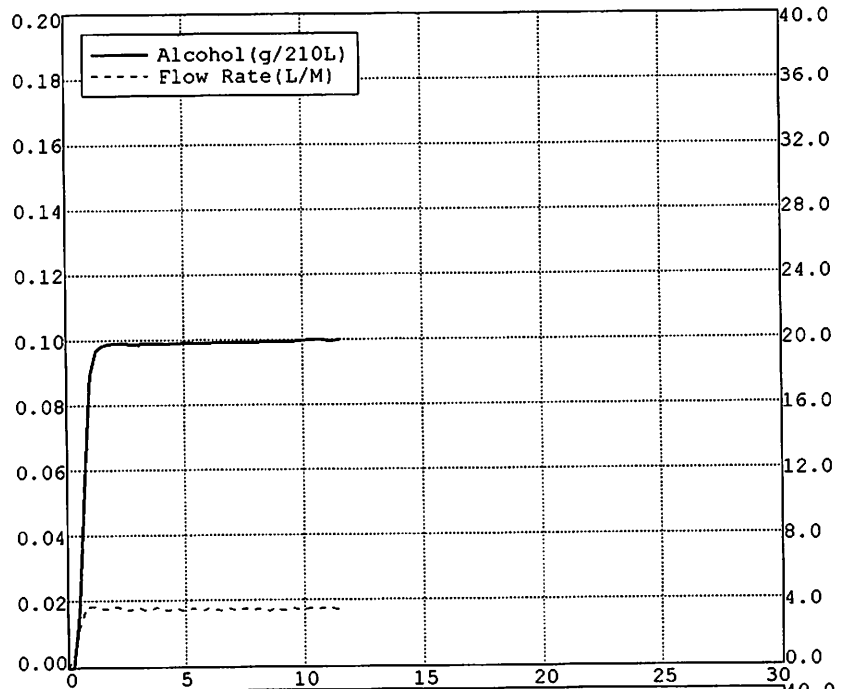

BFO

SUPERVISOR TEST

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 141906

Date: 02/27/2020

OPERATOR NAME:
LEONARD F DILLENBECK
Permit #: 47621
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:02
INTERNAL STANDARD	VERIFIED	00:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:03
BLANK TEST	0.00	00:04

RFI Detected

