

SUPERVISOR TEST

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 141906




BFC

Date: 01/22/2020

OPERATOR NAME:
LAUREN C MARLEAU
Permit #: 45976
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:22
INTERNAL STANDARD	VERIFIED	16:22
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	16:22
BLANK TEST	0.00	16:23
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	16:23
BLANK TEST	0.00	16:24
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	16:25
BLANK TEST	0.00	16:25

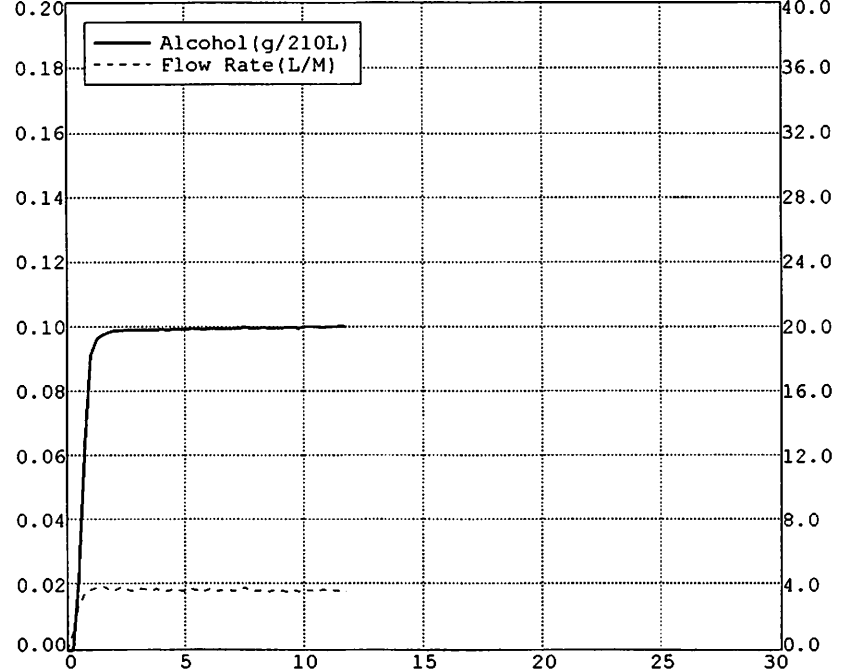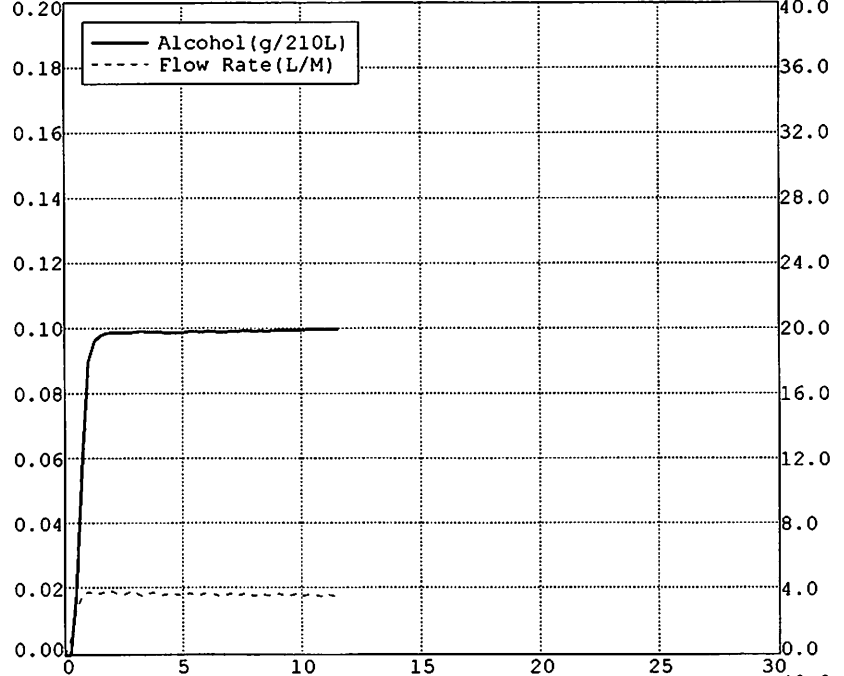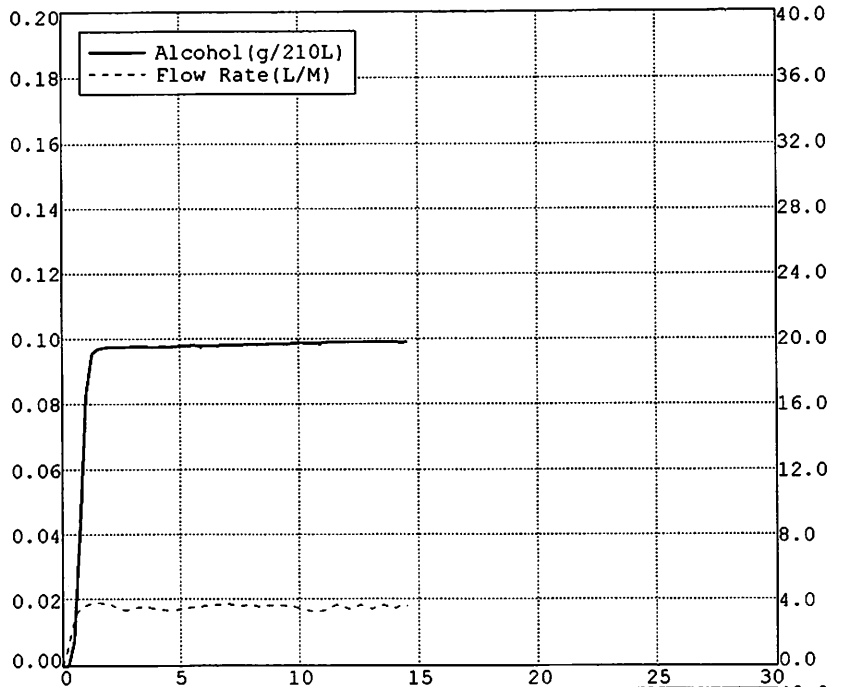

BFO

SUPERVISOR TEST



ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 141906

Date: 01/30/2020

OPERATOR NAME:
LEONARD F DILLENBECK
Permit #: 47621
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:18
INTERNAL STANDARD	VERIFIED	00:18
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	00:18
BLANK TEST	0.00	00:19
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	00:19
BLANK TEST	0.00	00:20
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	00:20
BLANK TEST	0.00	00:21

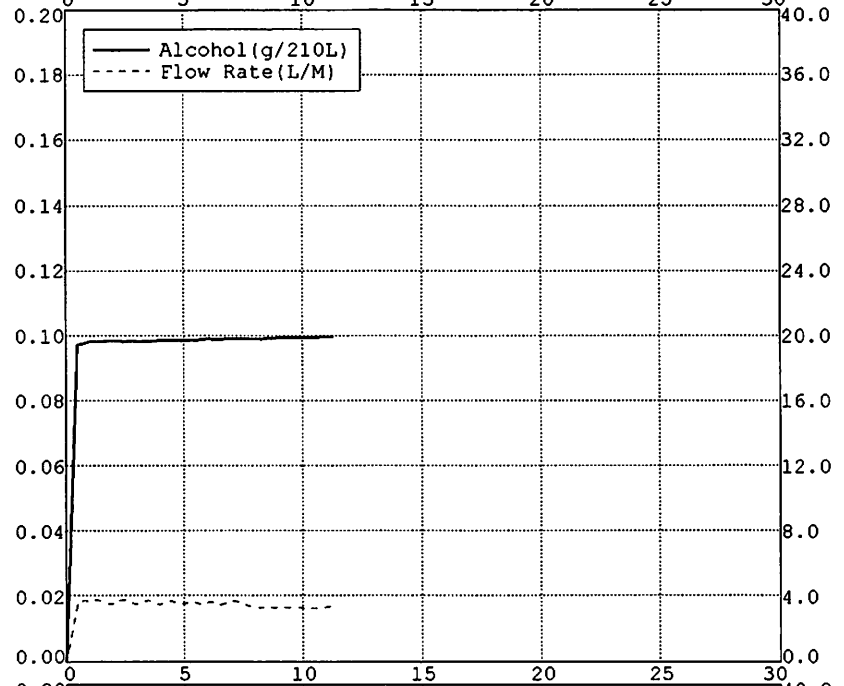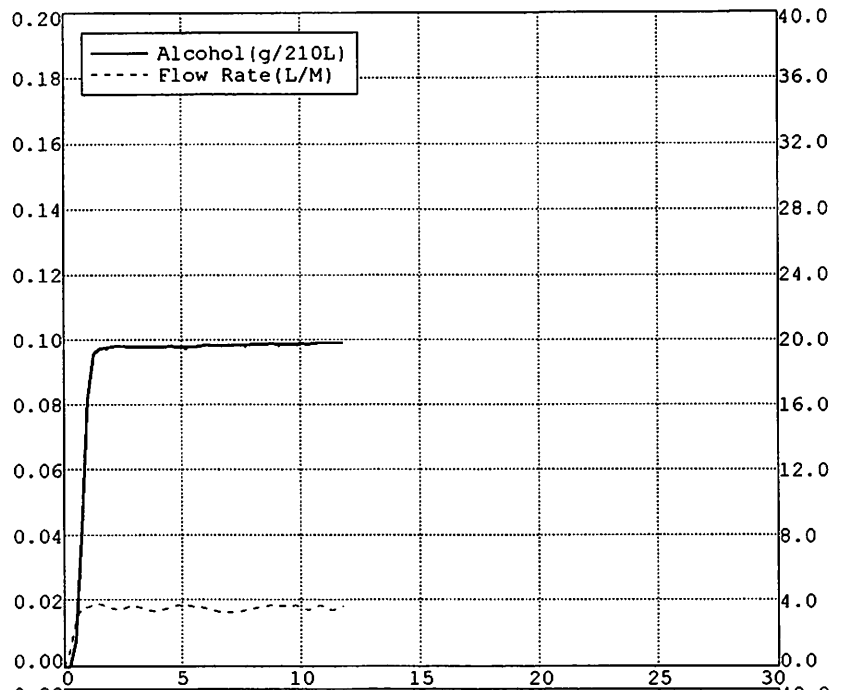

BFO

SOLUTION CHANGE


ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 141906

Date: 02/01/2020

OPERATOR NAME:
EDWARD F CONSTANTINE
Permit #: 45980
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 530

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:03
INTERNAL STANDARD	VERIFIED	19:03
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	19:03
BLANK TEST	0.00	19:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	19:04
BLANK TEST	0.00	19:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	19:06
BLANK TEST	0.00	19:06

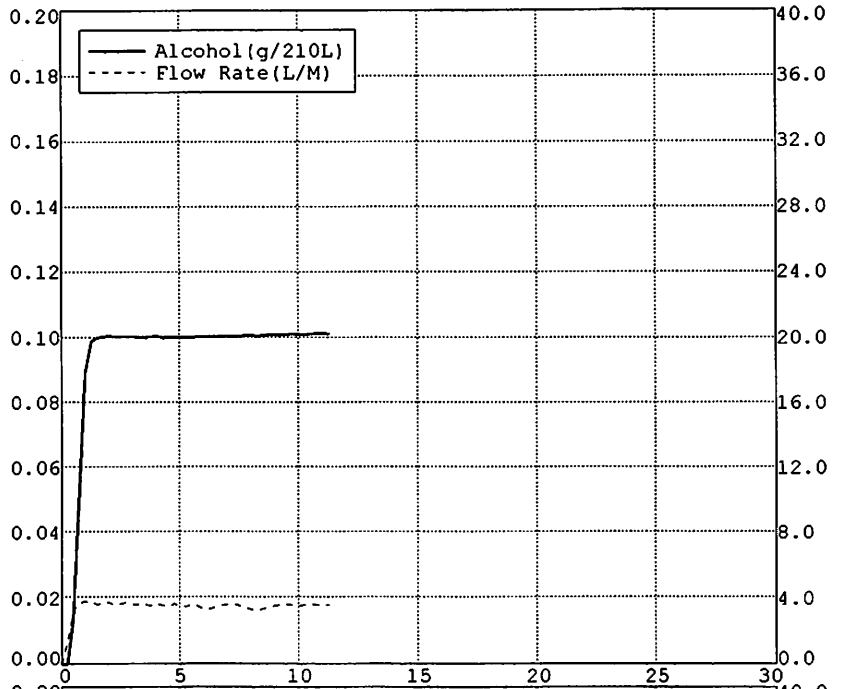

SUPERVISOR TEST

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 141906

Date: 02/05/2020

OPERATOR NAME:
EDWARD F CONSTANTINE
Permit #: 45980
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:09
INTERNAL STANDARD	VERIFIED	22:09
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	22:09
BLANK TEST	0.00	22:10
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	22:10
BLANK TEST	0.00	22:11
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	22:12
BLANK TEST	0.00	22:12

BFO

