

SOLUTION CHANGE




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 05/01/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:17
INTERNAL STANDARD	VERIFIED	23:17
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:17
BLANK TEST	0.00	23:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:18
BLANK TEST	0.00	23:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:20
BLANK TEST	0.00	23:21

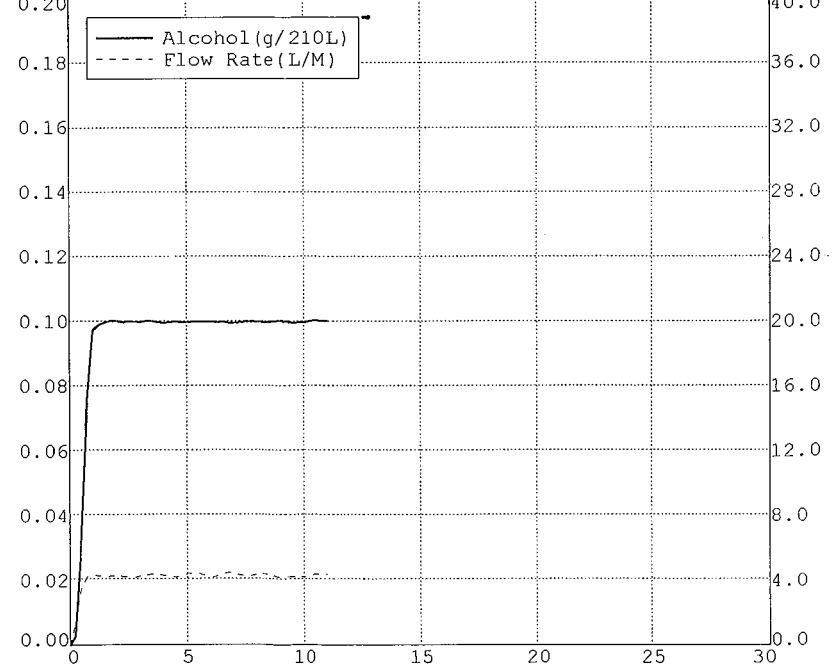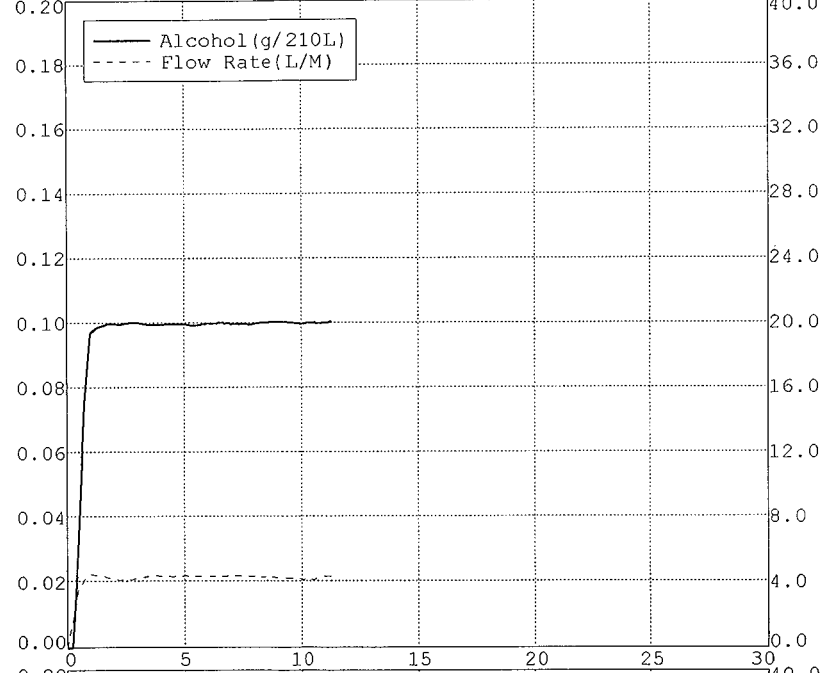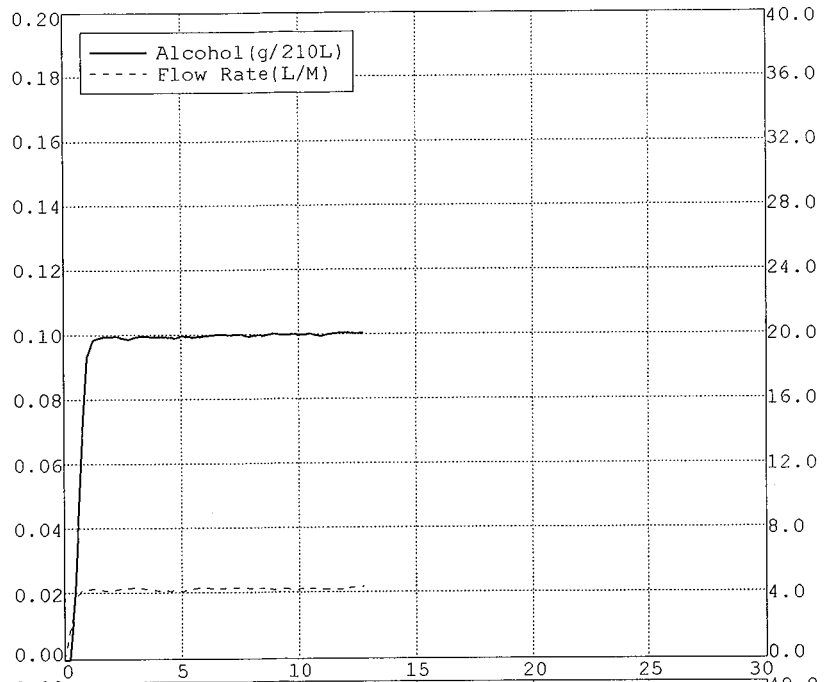

Hollie Kennedy Rome PD 05/01/19
10805

SUPERVISOR TEST




ROME CITY
 POLICE DEPT
 DATAMASTER dmt: 106106

Date: 05/03/2019

OPERATOR NAME:
 HOLLIE B KENNEDY
 Permit #: 39044
 Operator Agency/Dept: ROME CITY PD
 Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:22
INTERNAL STANDARD	VERIFIED	15:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:23
BLANK TEST	0.00	15:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:24
BLANK TEST	0.00	15:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:25
BLANK TEST	0.00	15:26

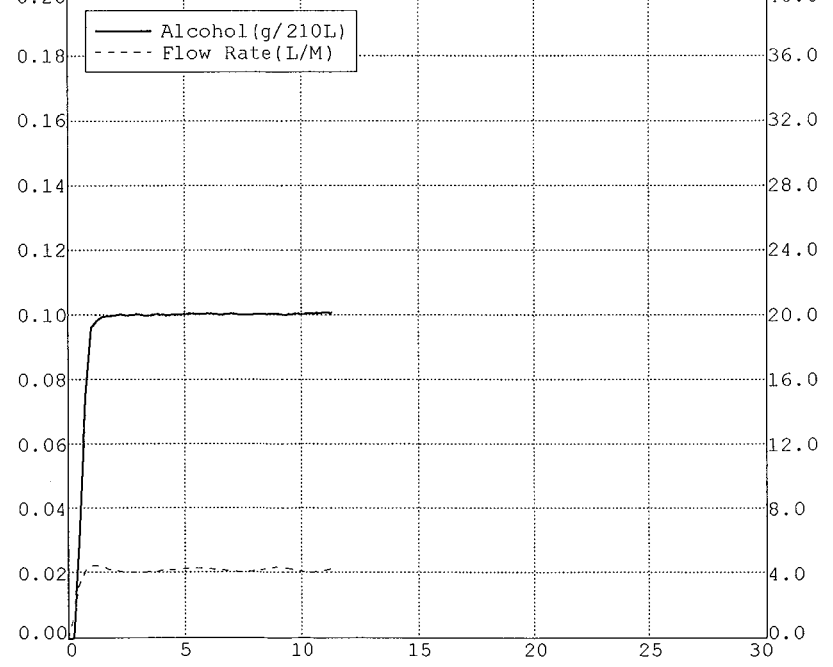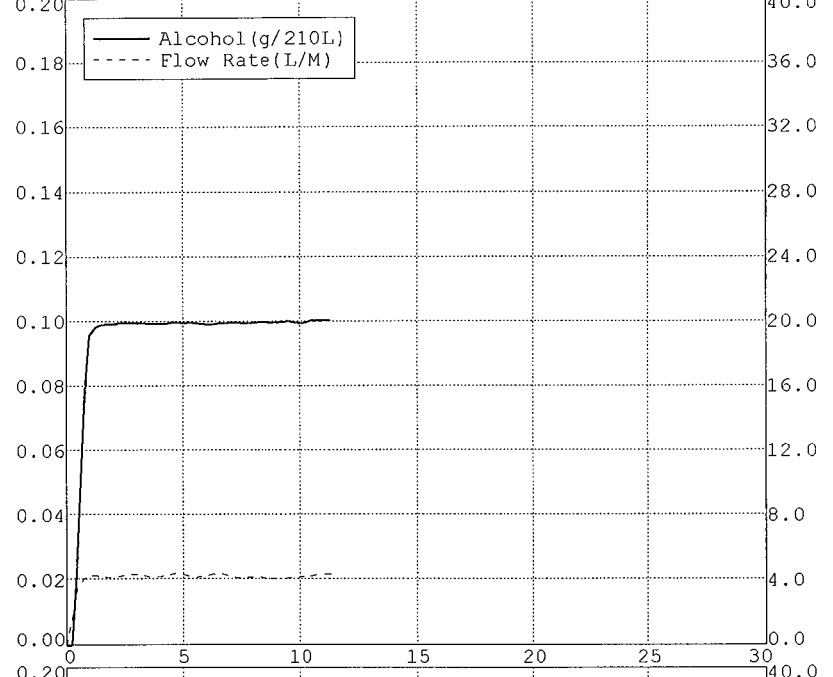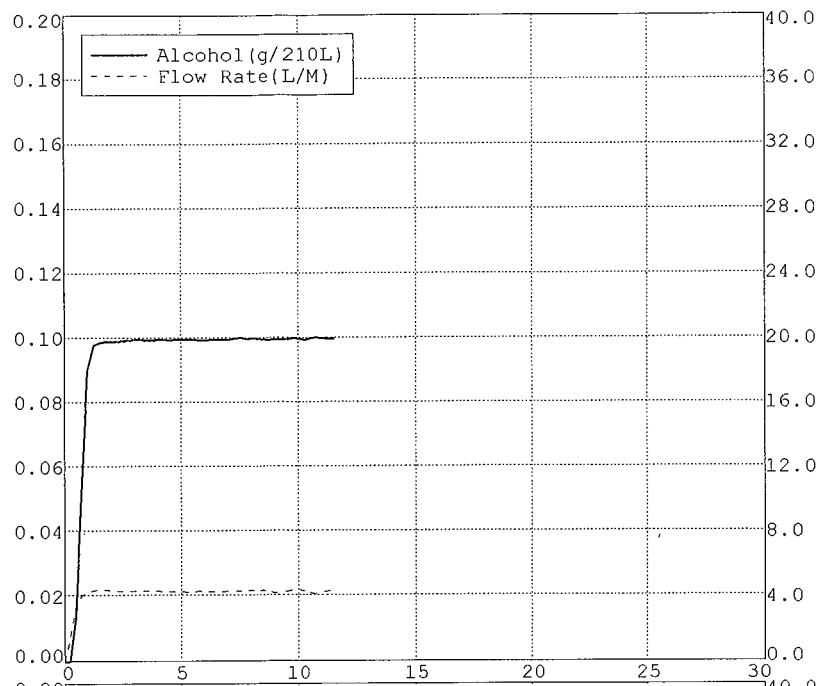

Hollie B Kennedy Rome PD 05/03/19
10000

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 05/10/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:59
INTERNAL STANDARD	VERIFIED	15:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:59
BLANK TEST	0.00	16:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:00
BLANK TEST	0.00	16:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:01
BLANK TEST	0.00	16:02

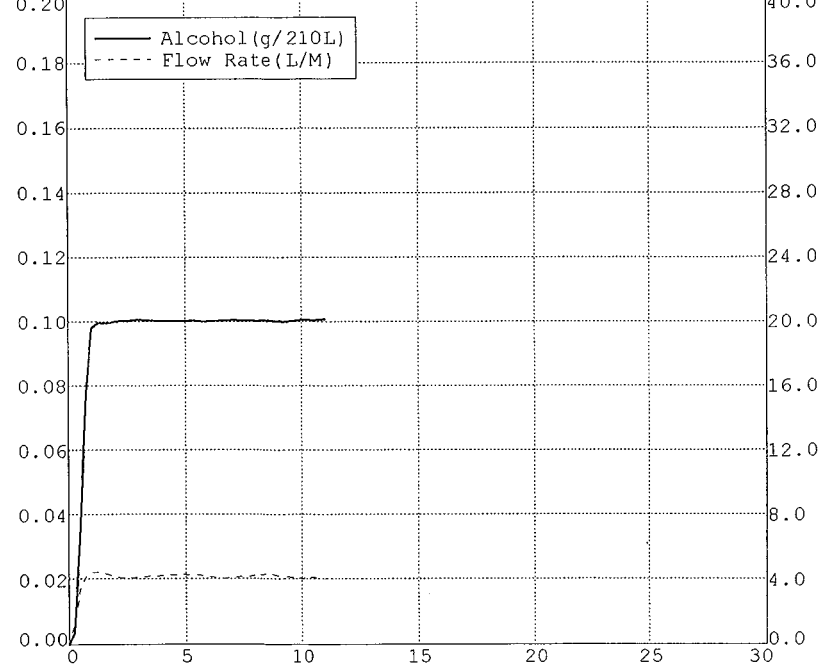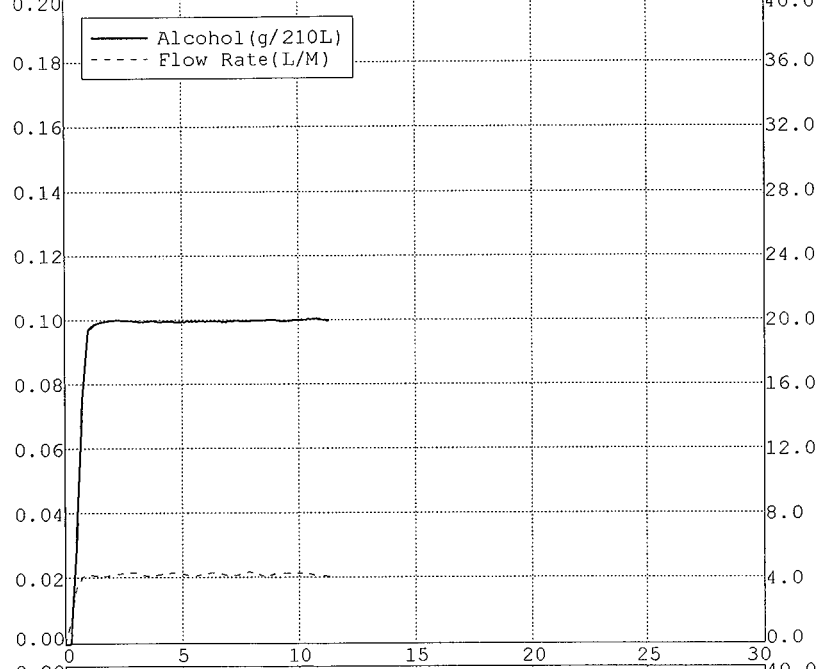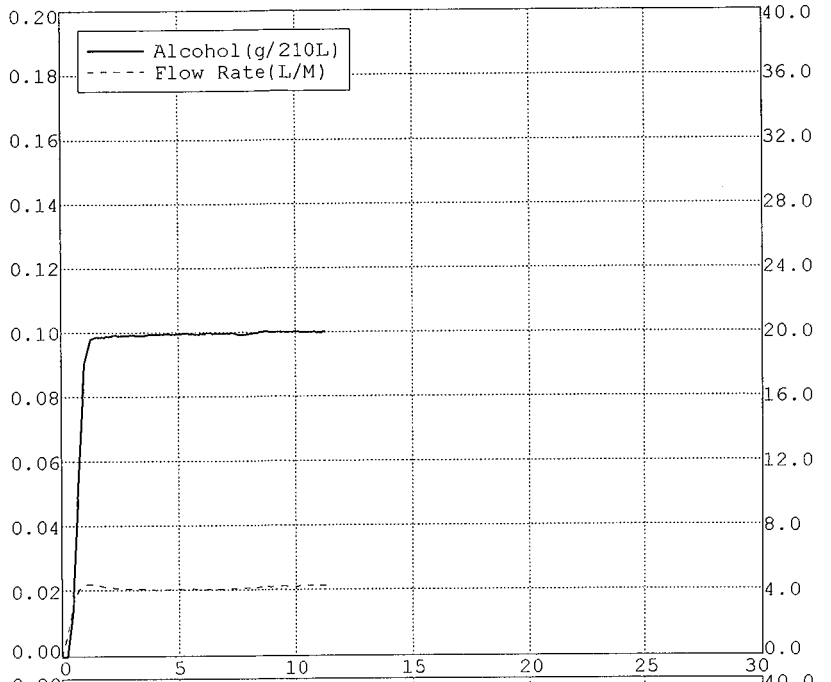

Hollie Kennedy Rome PD 05/10/19
Reference 10805

SUPERVISOR TEST




ROME CITY
 POLICE DEPT
 DATAMASTER dmt: 106106

Date: 05/17/2019

OPERATOR NAME:
 HOLLIE B KENNEDY
 Permit #: 39044
 Operator Agency/Dept: ROME CITY PD
 Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:29
INTERNAL STANDARD	VERIFIED	19:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:29
BLANK TEST	0.00	19:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	19:31
BLANK TEST	0.00	19:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	19:32
BLANK TEST	0.00	19:33

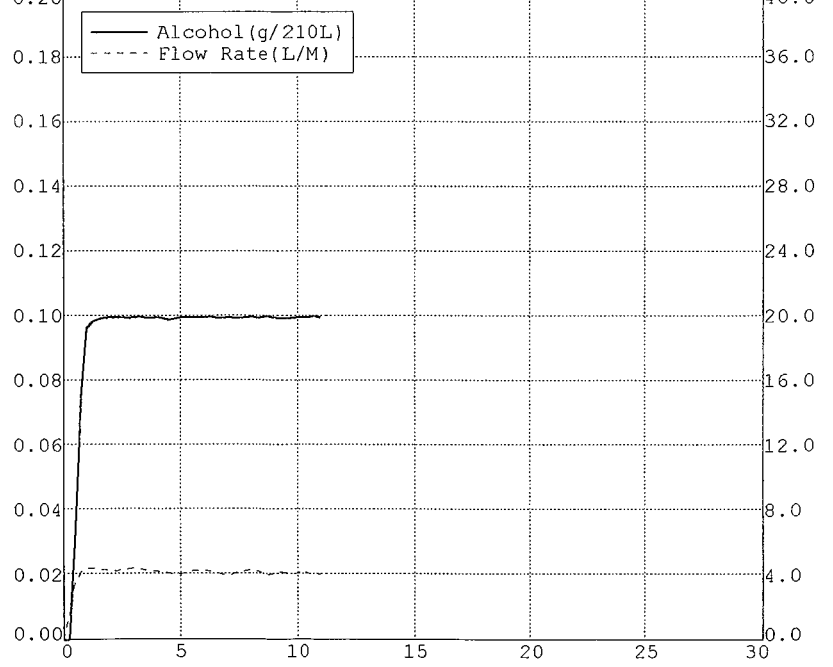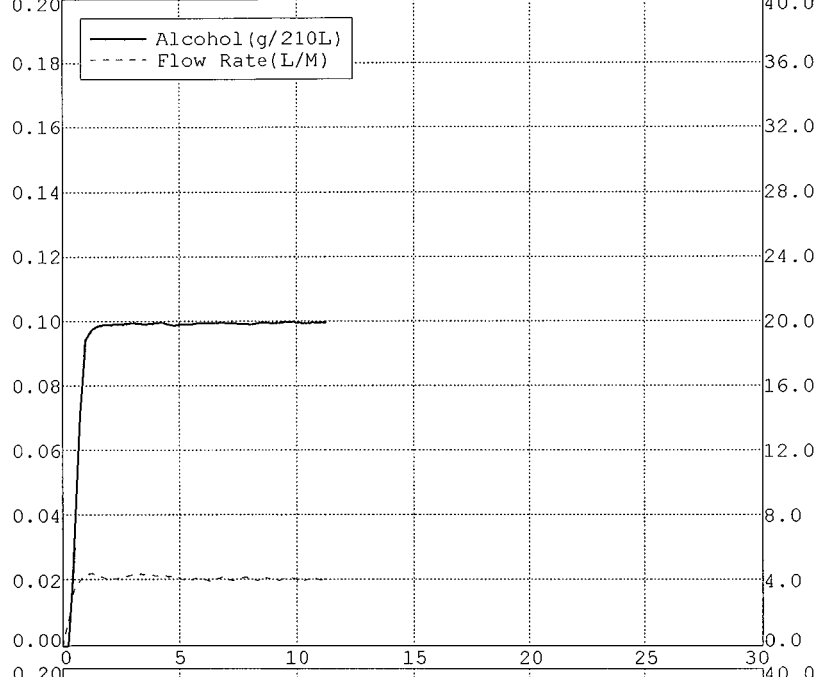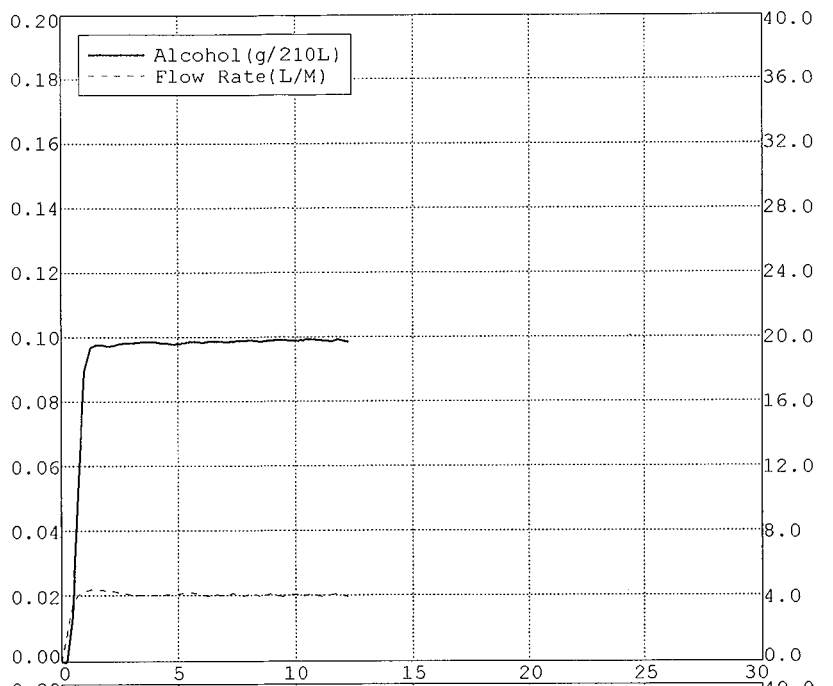

Hollie B Kennedy Rome PD 05/17/19
 10805

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 05/24/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:57
INTERNAL STANDARD	VERIFIED	21:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:57
BLANK TEST	0.00	21:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:58
BLANK TEST	0.00	21:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:59
BLANK TEST	0.00	22:00

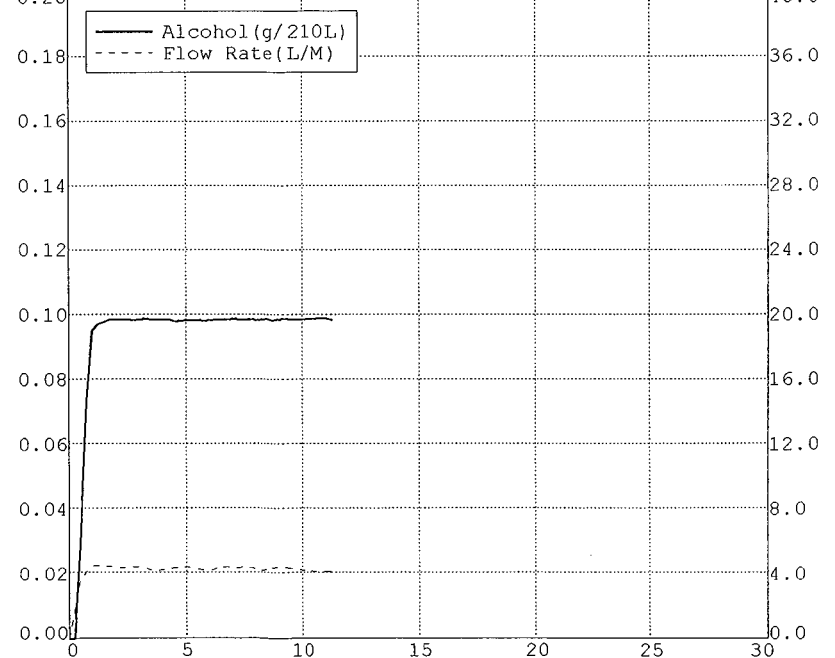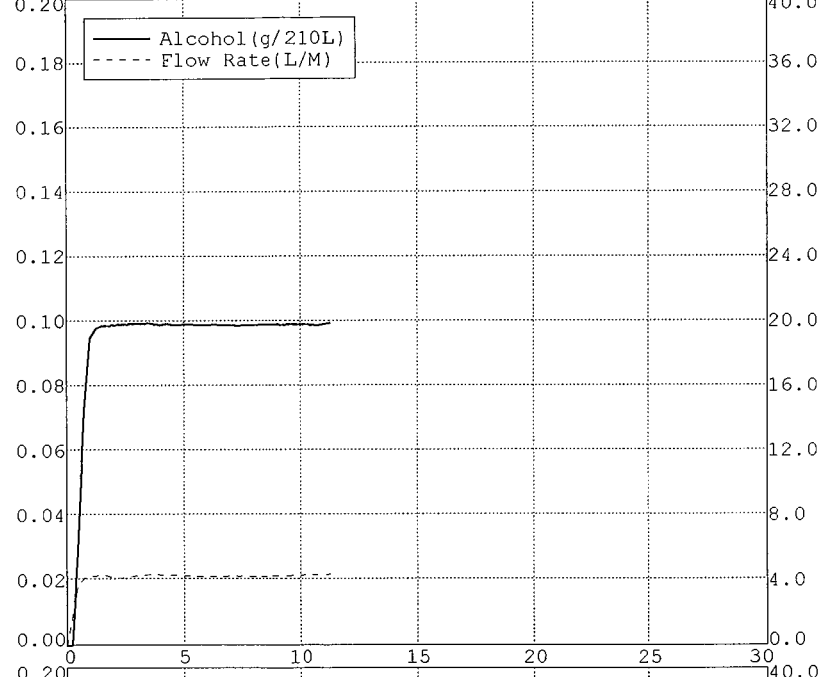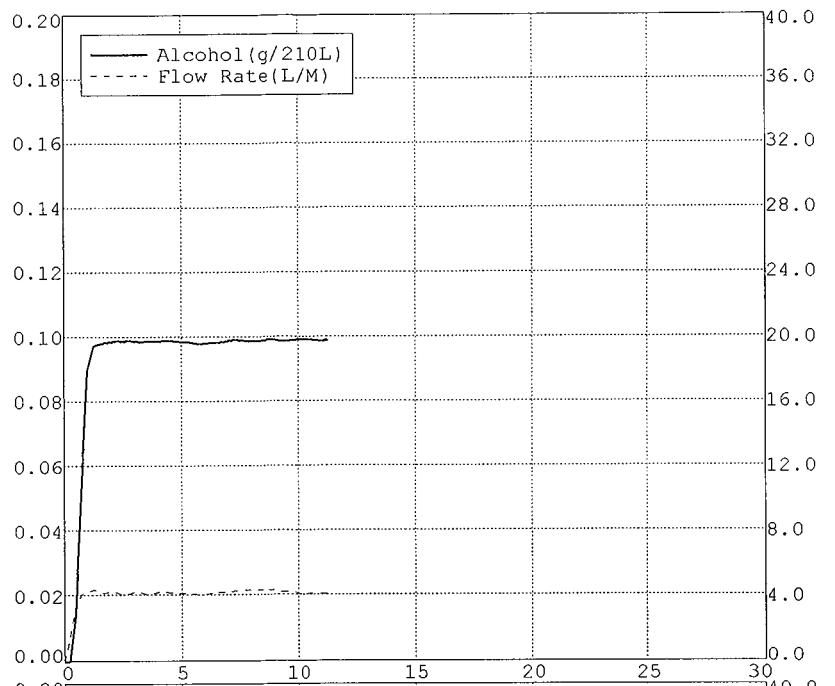

Hollie Kennedy Rome PD 05/24/19
10805

SUPERVISOR TEST




ROME CITY
 POLICE DEPT
 DATAMASTER dmt: 106106

Date: 05/31/2019

OPERATOR NAME:
 HOLLIE B KENNEDY
 Permit #: 39044
 Operator Agency/Dept: ROME CITY PD
 Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:27
INTERNAL STANDARD	VERIFIED	15:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:27
BLANK TEST	0.00	15:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:28
BLANK TEST	0.00	15:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:30
BLANK TEST	0.00	15:30

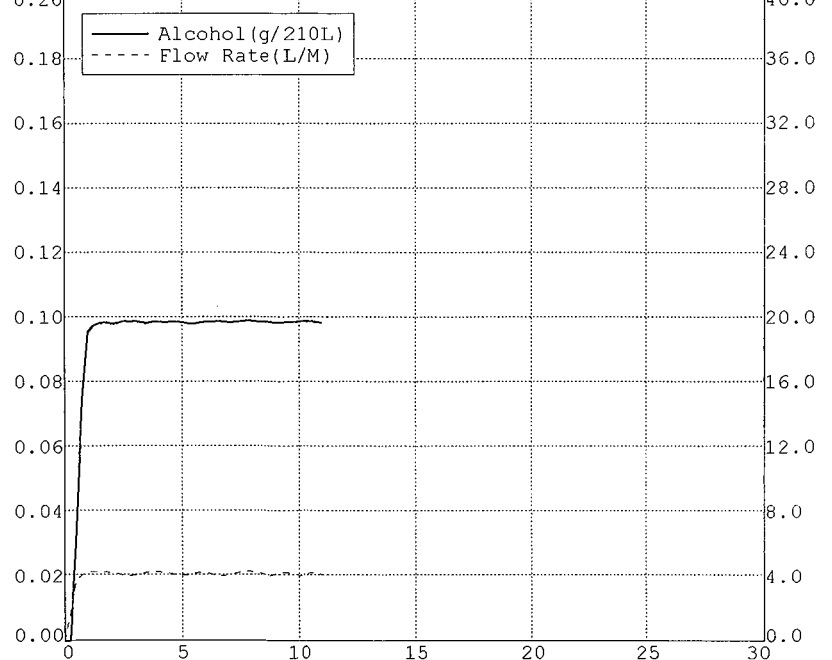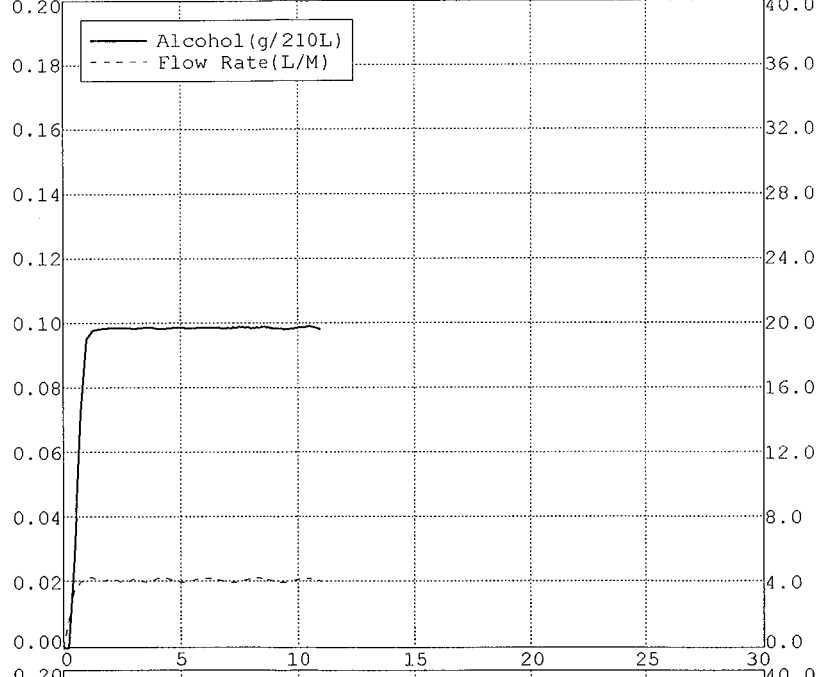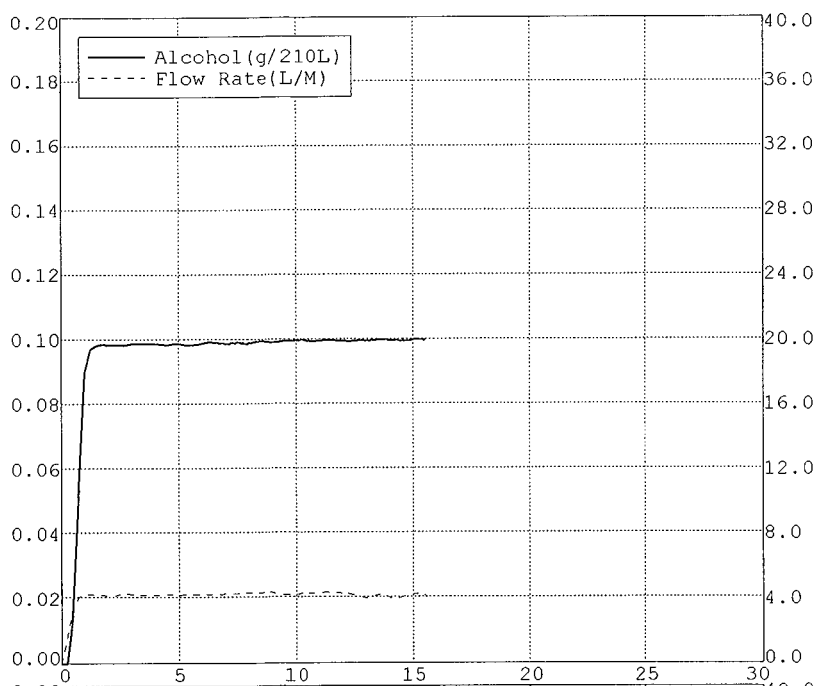

Hollie Kennedy Rome PD 05/31/19
 [Signature]