

SOLUTION CHANGE




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 08/01/2019

OPERATOR NAME:
HOLLIE B SILVERMAN
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:33
INTERNAL STANDARD	VERIFIED	18:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:34
BLANK TEST	0.00	18:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:35
BLANK TEST	0.00	18:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:36
BLANK TEST	0.00	18:37



Hollie B Silverman Rome PD 08/01/19
Hollie Silverman 10805

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 08/02/2019

OPERATOR NAME:
HOLLIE B SILVERMAN
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:32
INTERNAL STANDARD	VERIFIED	15:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:33
BLANK TEST	0.00	15:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:34
BLANK TEST	0.00	15:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:35
BLANK TEST	0.00	15:36

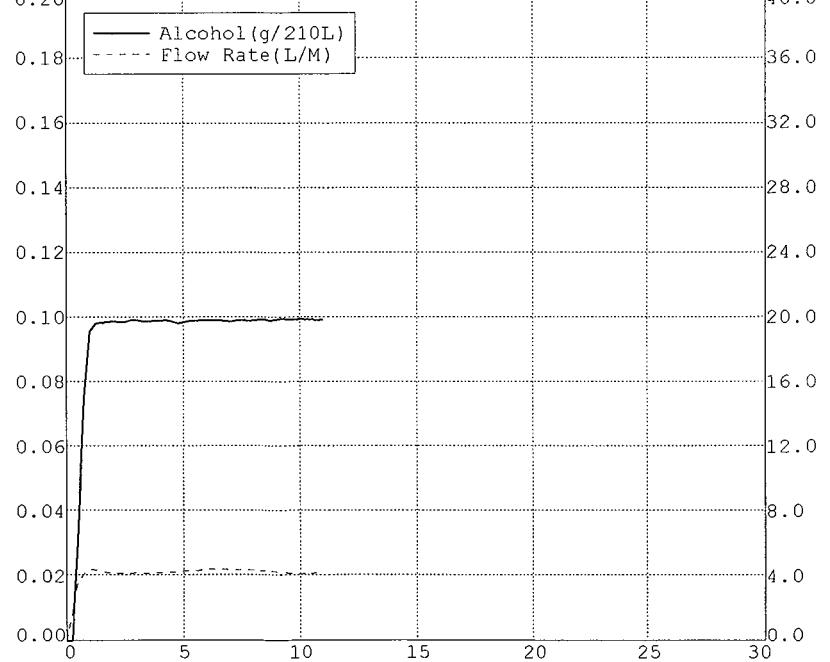

Hollie B Silverman Romeo 08/02/19
~~Rhodie B Silverman~~ 08/02/19

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 08/09/2019

OPERATOR NAME:
HOLLIE B SILVERMAN
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:25
INTERNAL STANDARD	VERIFIED	15:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:25
BLANK TEST	0.00	15:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:27
BLANK TEST	0.00	15:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:28
BLANK TEST	0.00	15:29



Hollie B. Silverman Rome PD 08/09/19
Hollie B. Silverman 10805

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 08/23/2019

OPERATOR NAME:
HOLLIE B SILVERMAN
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:16
INTERNAL STANDARD	VERIFIED	03:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:16
BLANK TEST	0.00	03:17
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:18
BLANK TEST	0.00	03:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:19
BLANK TEST	0.00	03:20



Hollie B. Silverman Rome PD 08/23/19
Hollie Silverman 10605

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 08/30/2019

OPERATOR NAME:
HOLLIE B SILVERMAN
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:30
INTERNAL STANDARD	VERIFIED	21:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:31
BLANK TEST	0.00	21:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:32
BLANK TEST	0.00	21:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:33
BLANK TEST	0.00	21:34



Hollie B. Silverman Rome PD 08/30/19
Hollie Silverman 10805