

SOLUTION CHANGE




ROME CITY  
POLICE DEPT  
DATAMASTER dmt: 106106

Date: 09/01/2019

OPERATOR NAME:  
HOLLIE B SILVERMAN  
Permit #: 39044  
Operator Agency/Dept: ROME CITY PD  
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:47
INTERNAL STANDARD	VERIFIED	14:47
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:47
BLANK TEST	0.00	14:48
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:48
BLANK TEST	0.00	14:49
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:49
BLANK TEST	0.00	14:50

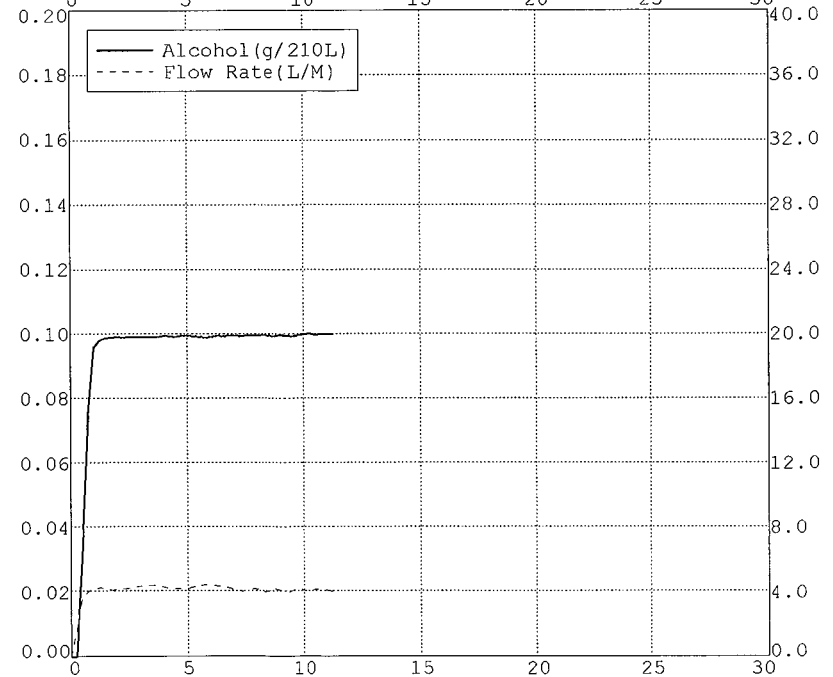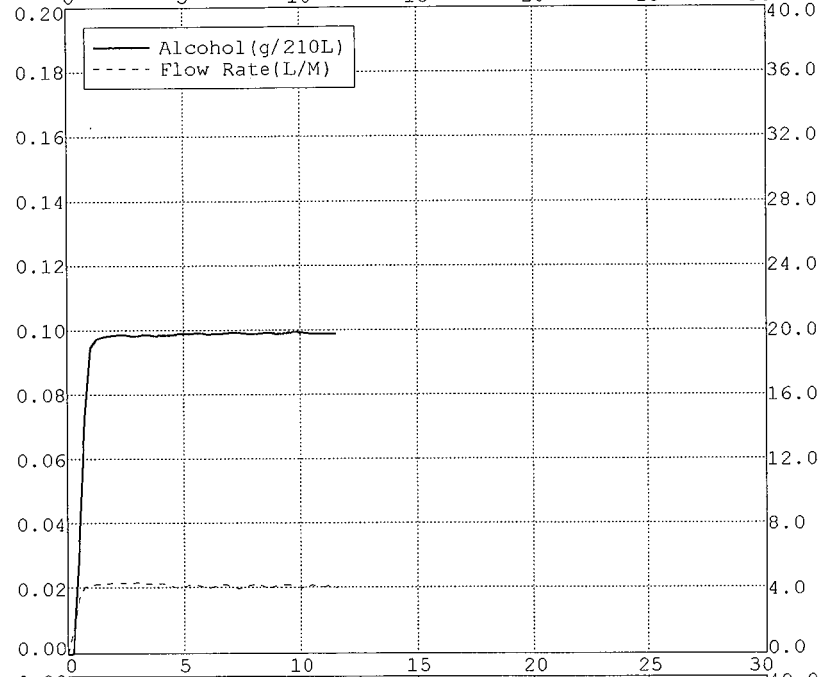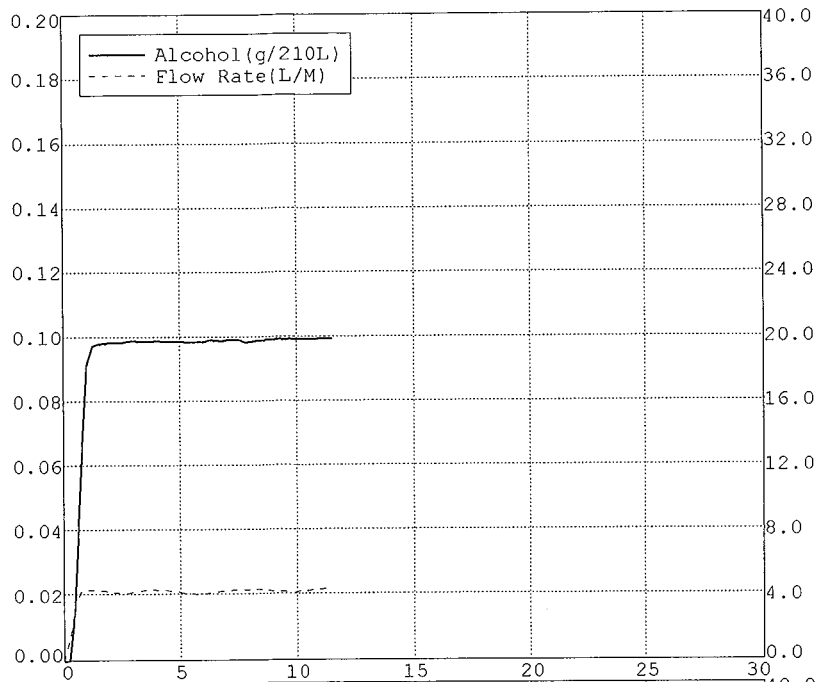

*Hollie B Silverman Rome PD 09/01/19*  
*Hollie Silverman 10855*

SUPERVISOR TEST




ROME CITY  
 POLICE DEPT  
 DATAMASTER dmt: 106106

Date: 09/06/2019

OPERATOR NAME:  
 HOLLIE B SILVERMAN  
 Permit #: 39044  
 Operator Agency/Dept: ROME CITY PD  
 Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:42
INTERNAL STANDARD	VERIFIED	21:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:42
BLANK TEST	0.00	21:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:43
BLANK TEST	0.00	21:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:45
BLANK TEST	0.00	21:45

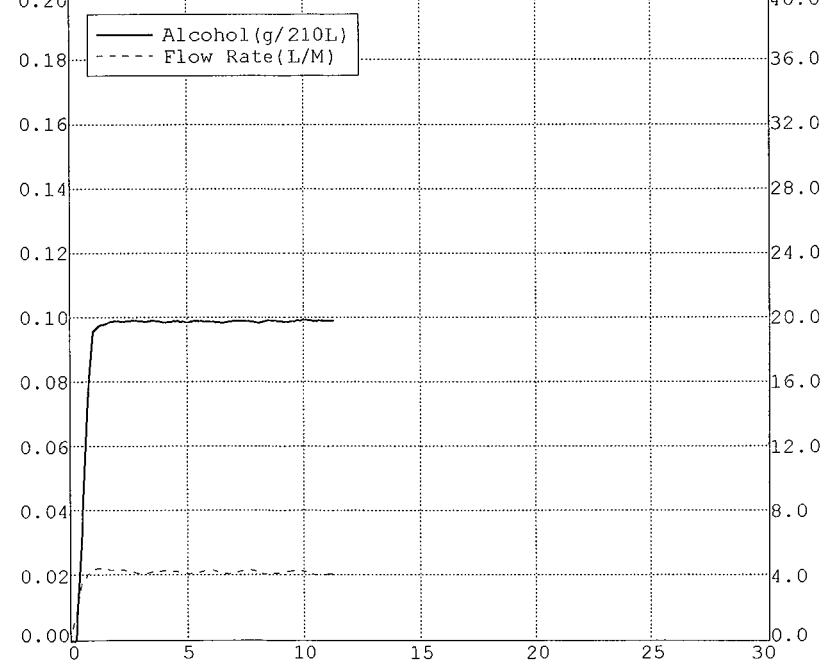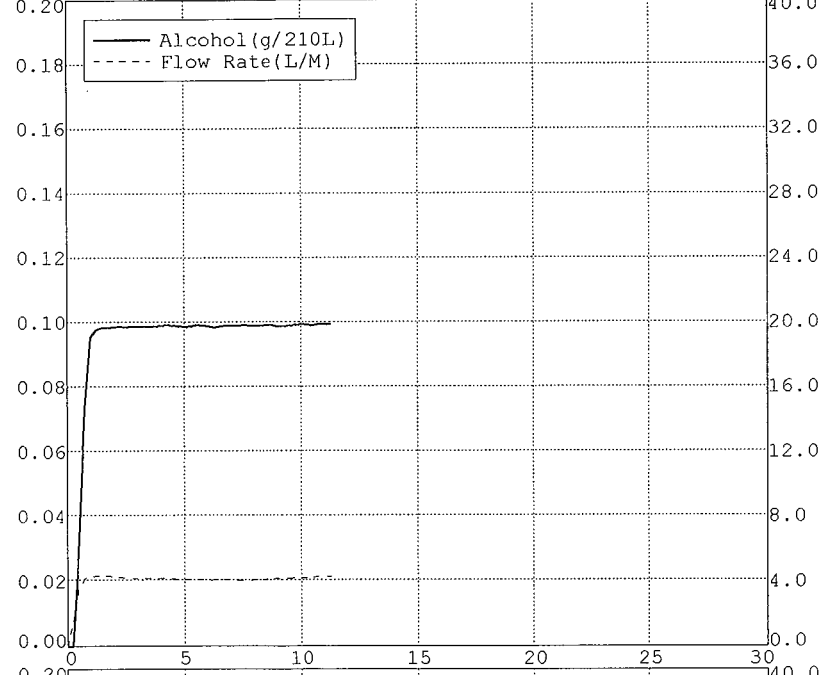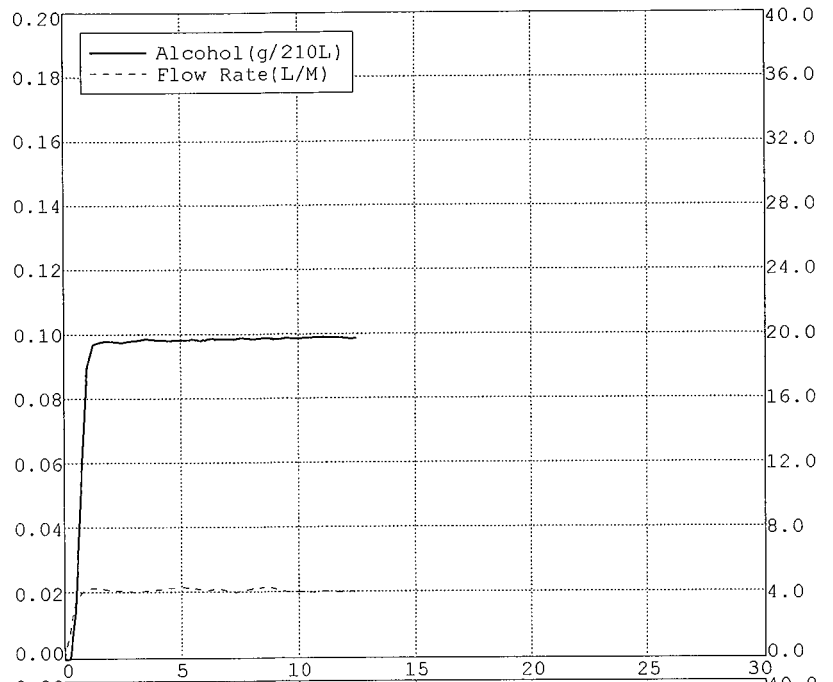

Hollie B. Silverman Rome PD 09/06/19  
 Hollie B. Silverman 106106

SUPERVISOR TEST




ROME CITY  
POLICE DEPT  
DATAMASTER dmt: 106106

Date: 09/13/2019

OPERATOR NAME:  
HOLLIE B SILVERMAN  
Permit #: 39044  
Operator Agency/Dept: ROME CITY PD  
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:20
INTERNAL STANDARD	VERIFIED	15:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:20
BLANK TEST	0.00	15:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:21
BLANK TEST	0.00	15:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:23
BLANK TEST	0.00	15:23

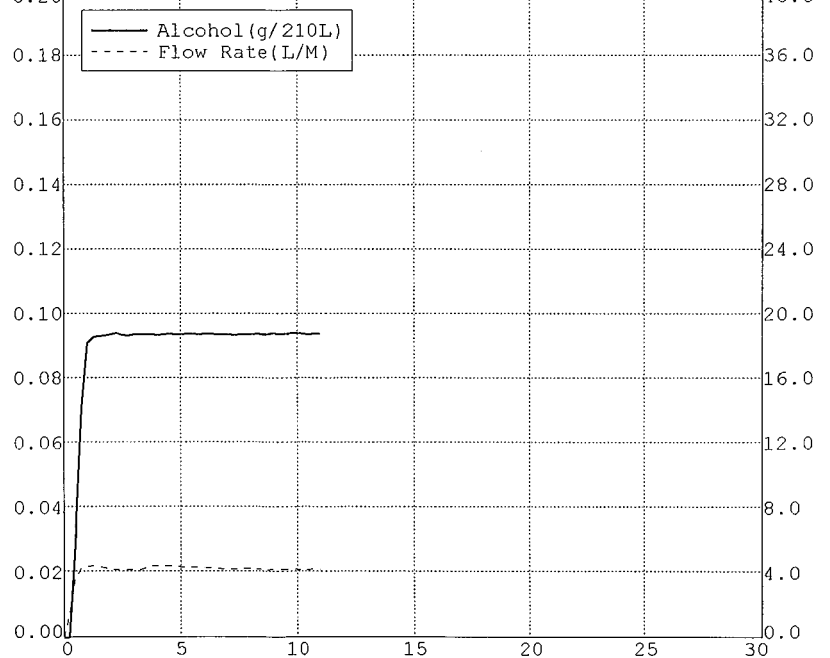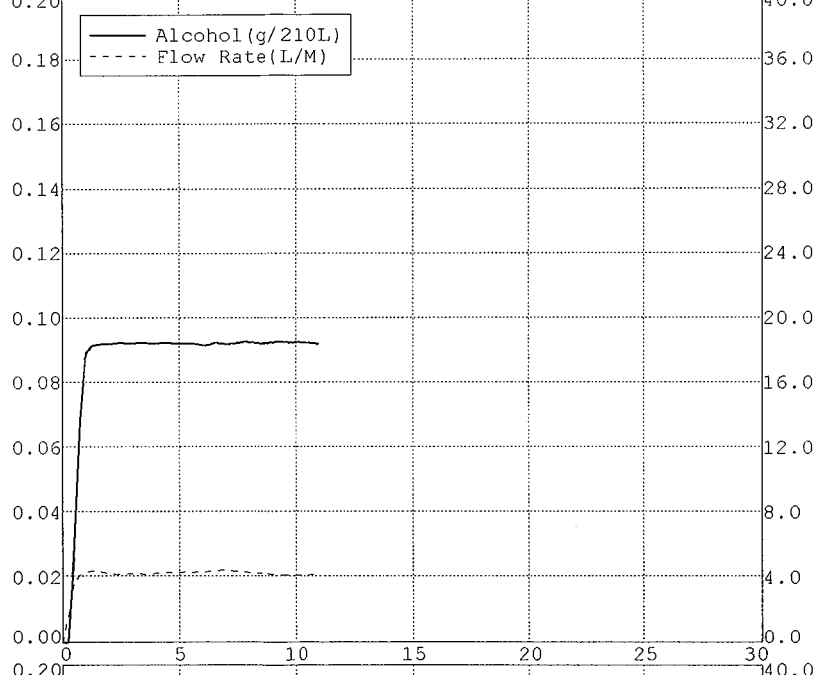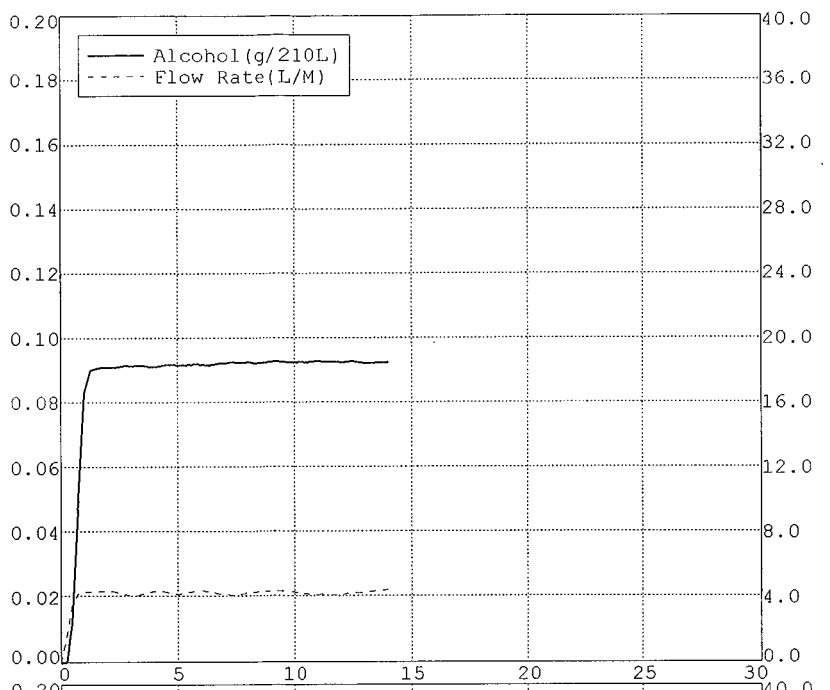

*Hollie B. Silverman Rome PD 09/13/19*  
*Hollie Silverman 10805*

SUPERVISOR TEST




ROME CITY  
POLICE DEPT  
DATAMASTER dmt: 106106

Date: 09/20/2019

OPERATOR NAME:  
HOLLIE B SILVERMAN  
Permit #: 39044  
Operator Agency/Dept: ROME CITY PD  
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:07
INTERNAL STANDARD	VERIFIED	16:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:08
BLANK TEST	0.00	16:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:09
BLANK TEST	0.00	16:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:10
BLANK TEST	0.00	16:11

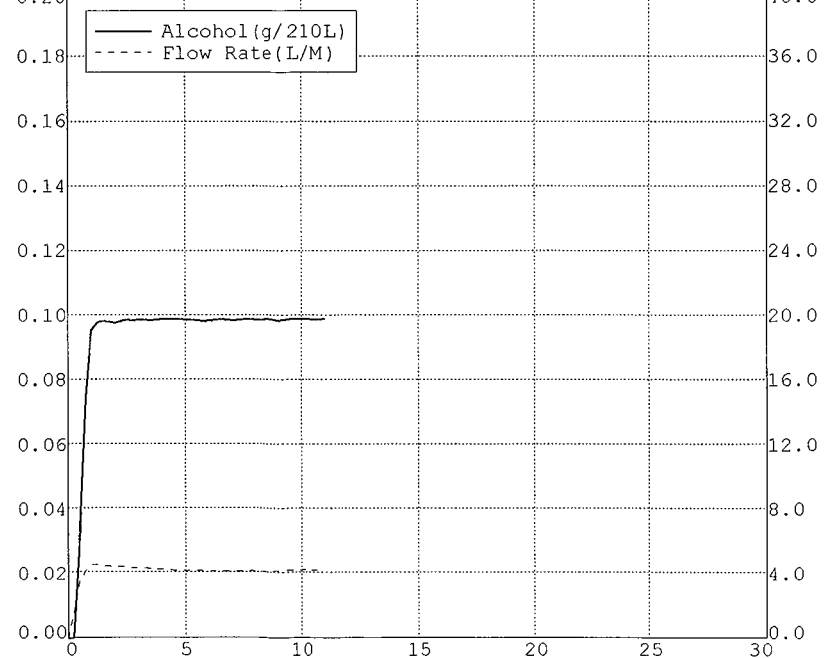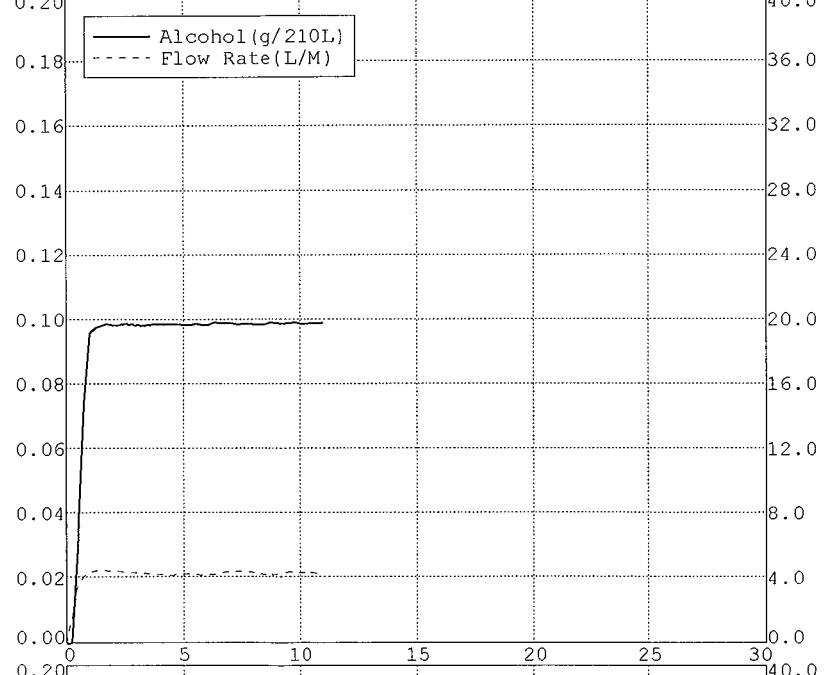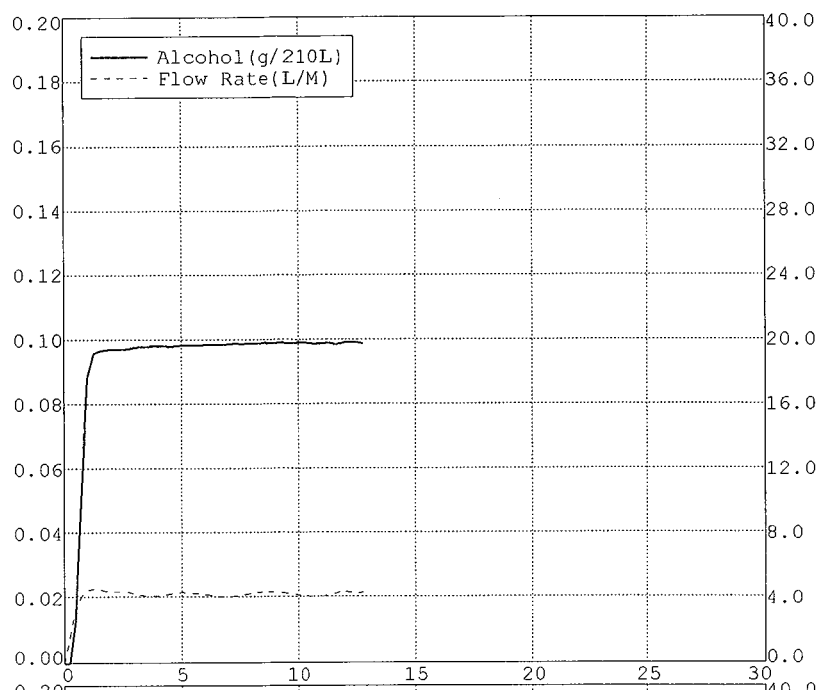

Hollie B. Silverman Rome PD 09/20/19  
Hollie B. Silverman 10905

SUPERVISOR TEST



ROME CITY  
POLICE DEPT  
DATAMASTER dmt: 106106

ate: 09/27/2019

OPERATOR NAME:  
HOLLIE B SILVERMAN  
Permit #: 39044  
Operator Agency/Dept: ROME CITY PD  
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:33
INTERNAL STANDARD	VERIFIED	23:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:34
BLANK TEST	0.00	23:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:35
BLANK TEST	0.00	23:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:36
BLANK TEST	0.00	23:37

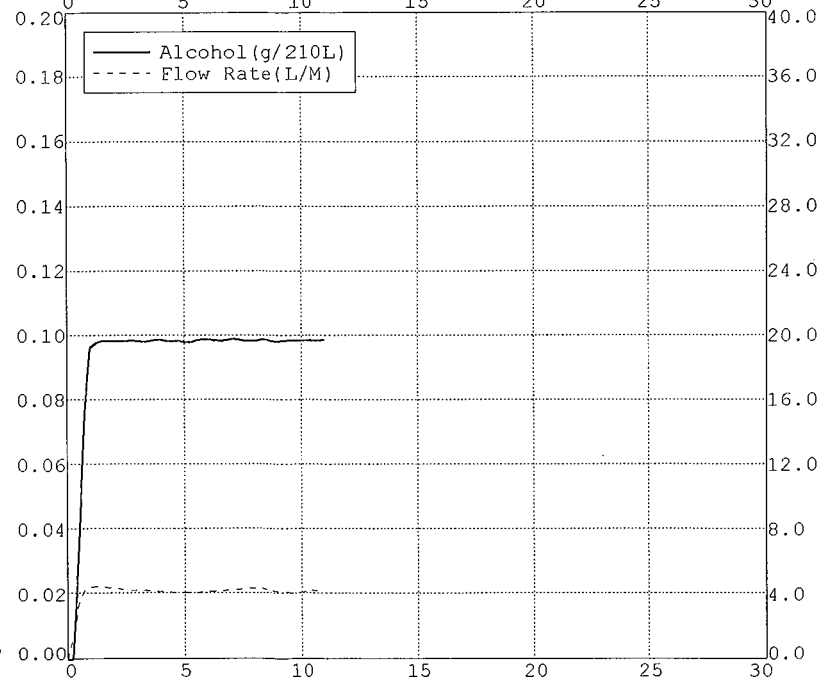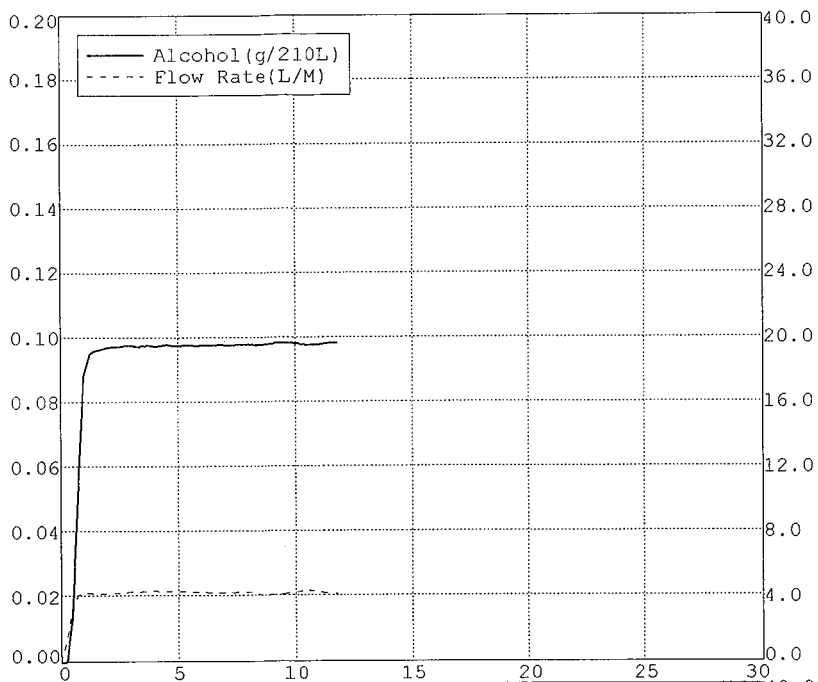

*Hollie B. Silverman Rome PD 09/27/19*  
*Hollie B. Silverman 10905*