

SOLUTION CHANGE




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 02/02/2020

OPERATOR NAME:
HOLLIE B SILVERMAN
Permit #: 19350
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:14
INTERNAL STANDARD	VERIFIED	16:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:14
BLANK TEST	0.00	16:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:15
BLANK TEST	0.00	16:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:17
BLANK TEST	0.00	16:17

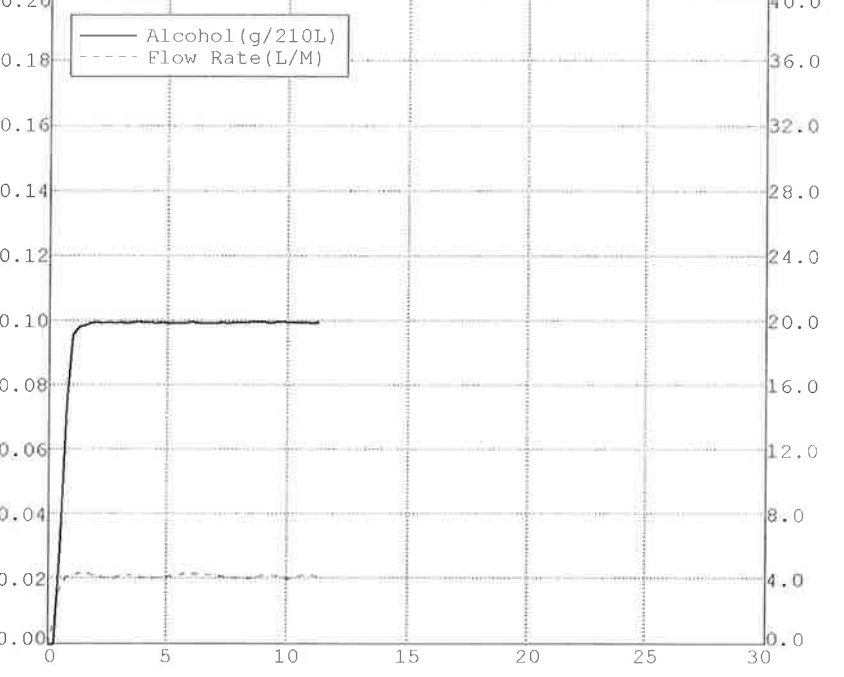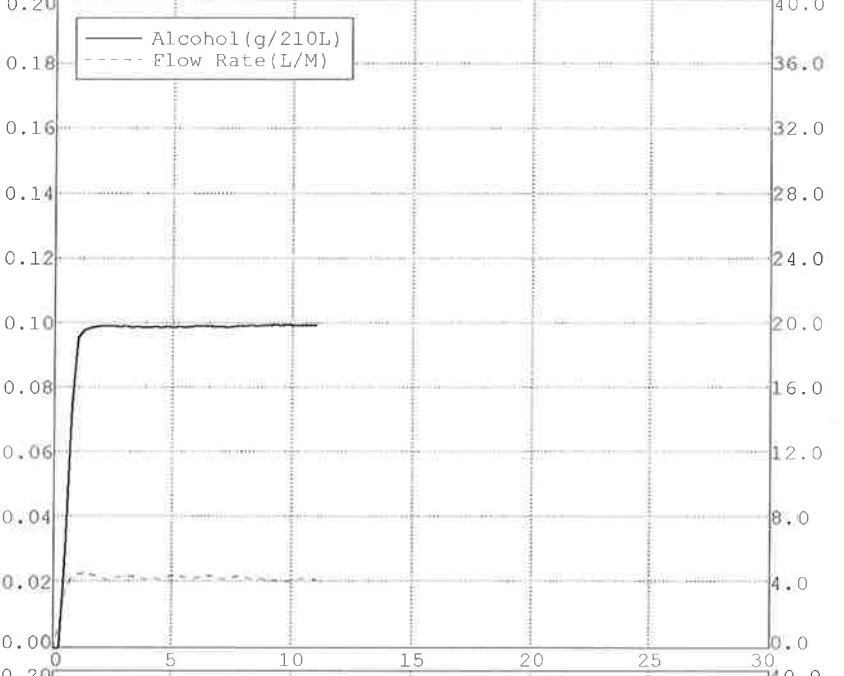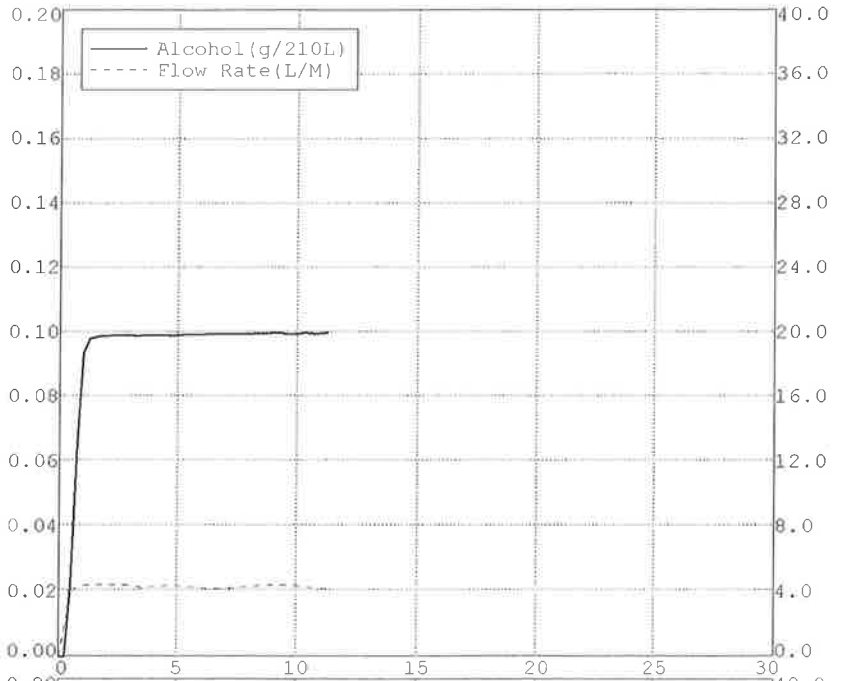

Hollie B. Silverman Rome PD 02/02/2020
Hollie B. Silverman 10905