

SUPERVISOR TEST



ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 02/14/2020

OPERATOR NAME:
HOLLIE B SILVERMAN
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19350

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 17:45 |
| INTERNAL STANDARD | VERIFIED | 17:45 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 17:45 |
| BLANK TEST | 0.00 | 17:46 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 17:46 |
| BLANK TEST | 0.00 | 17:47 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 17:47 |
| BLANK TEST | 0.00 | 17:48 |

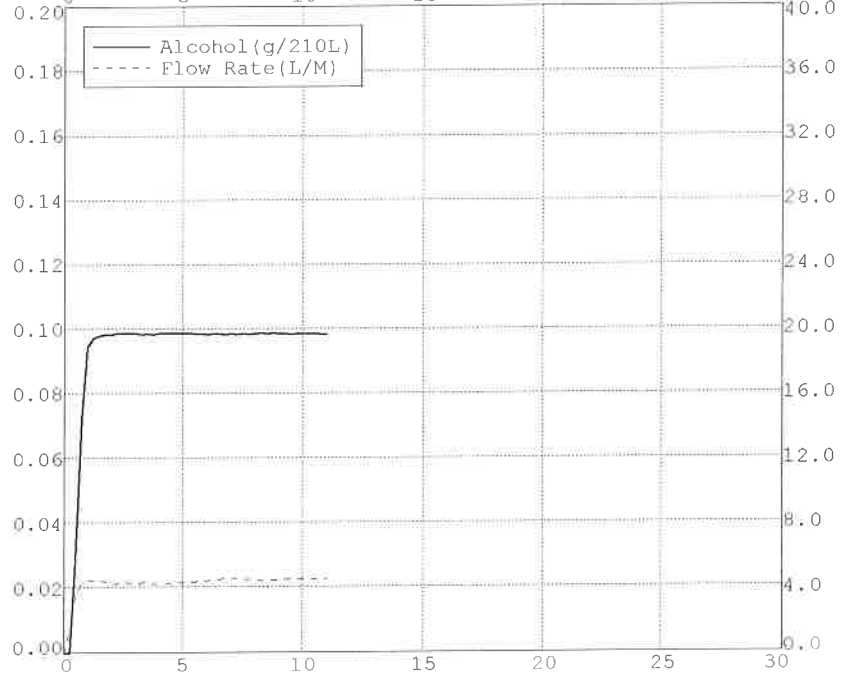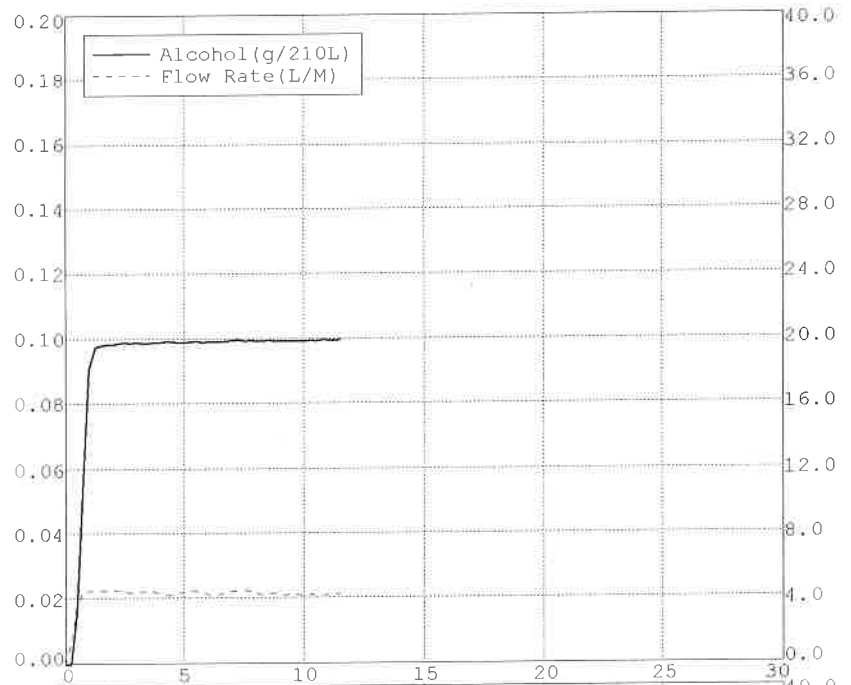

Hollie B. Silverman Rome PD 02/14/2020
Hollie B. Silverman Rome PD