

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 03/27/2020

OPERATOR NAME:
HOLLIE B SILVERRMAN
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:24
INTERNAL STANDARD	VERIFIED	15:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:25
BLANK TEST	0.00	15:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:26
BLANK TEST	0.00	15:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:27
BLANK TEST	0.00	15:28

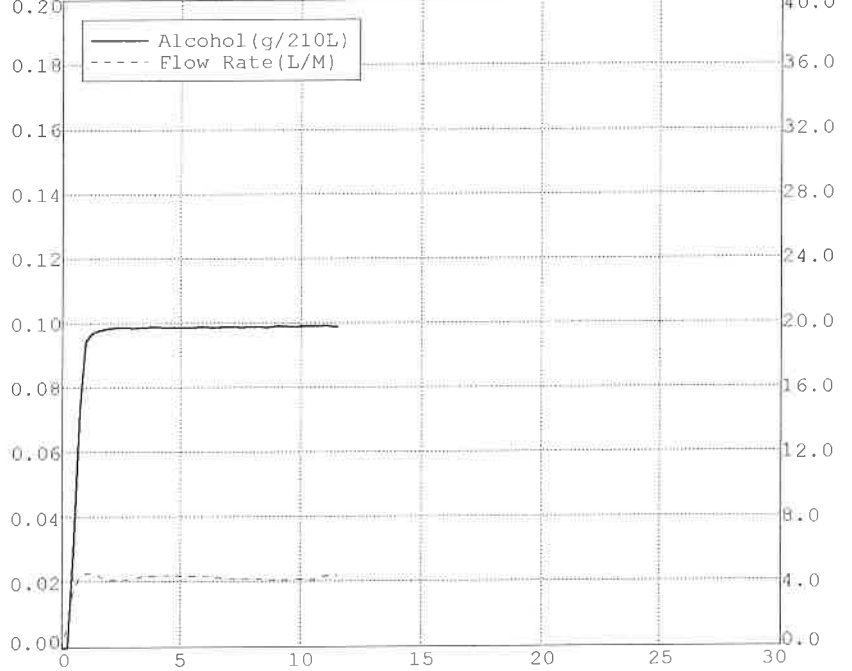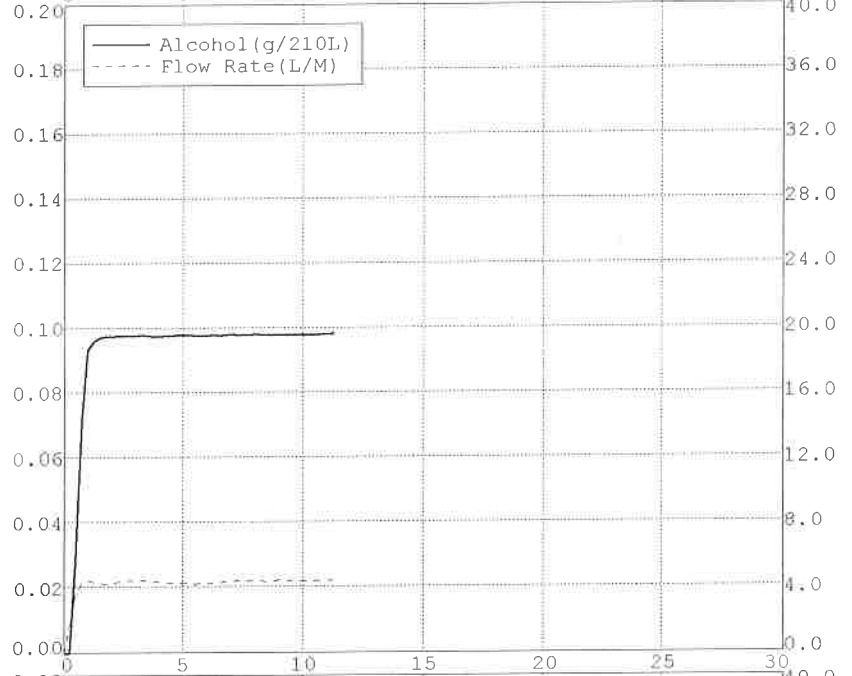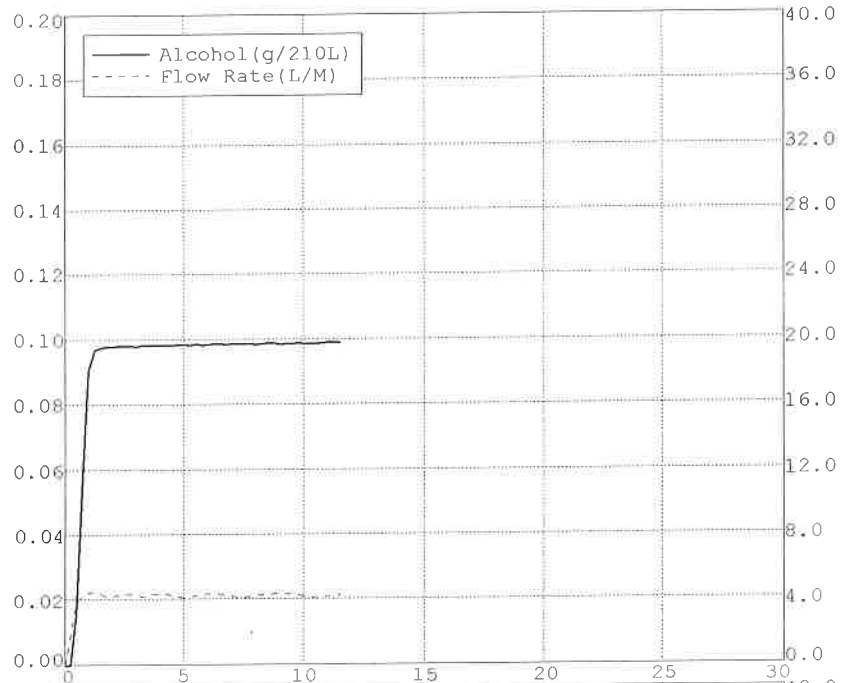

Hollie B. Silverman ROME PD 03/27/2020
Hollie B. Silverman 10005