

SUPERVISOR TEST




ROME CITY  
 POLICE DEPT  
 DATAMASTER dmt: 106106

Date: 07/10/2020

OPERATOR NAME:  
 HOLLIE B SILVERMAN  
 Permit #: 39044  
 Operator Agency/Dept: ROME CITY PD  
 Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:07
INTERNAL STANDARD	VERIFIED	14:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:08
BLANK TEST	0.00	14:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:09
BLANK TEST	0.00	14:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:10
BLANK TEST	0.00	14:11

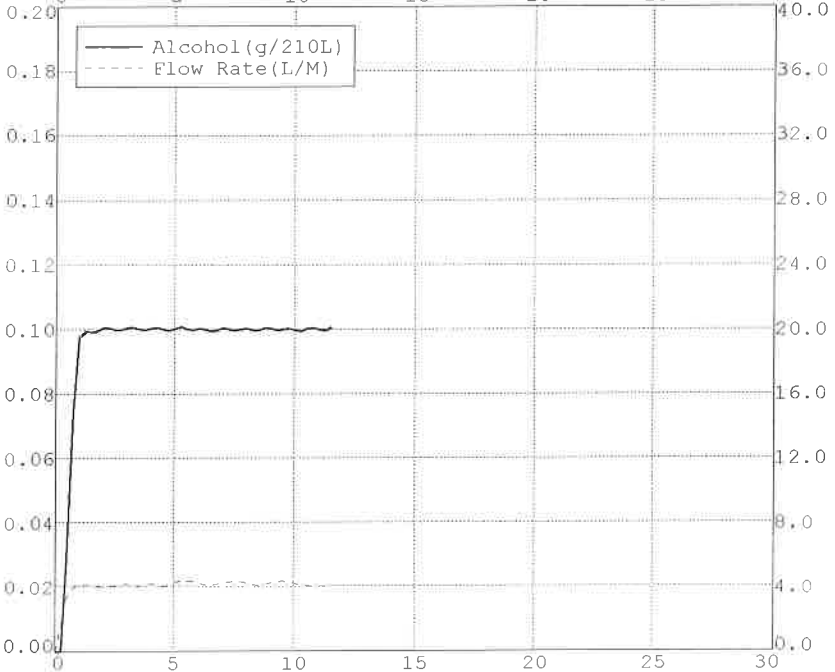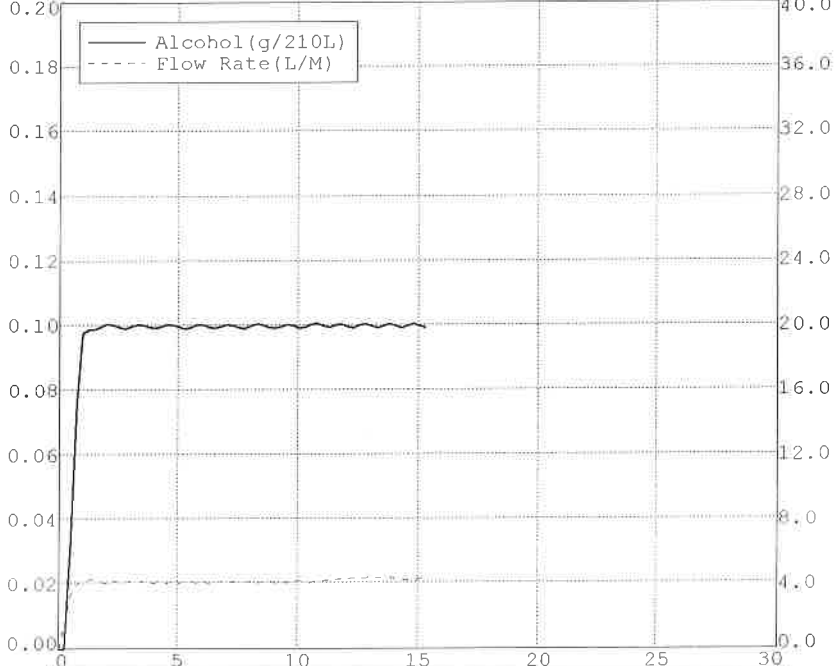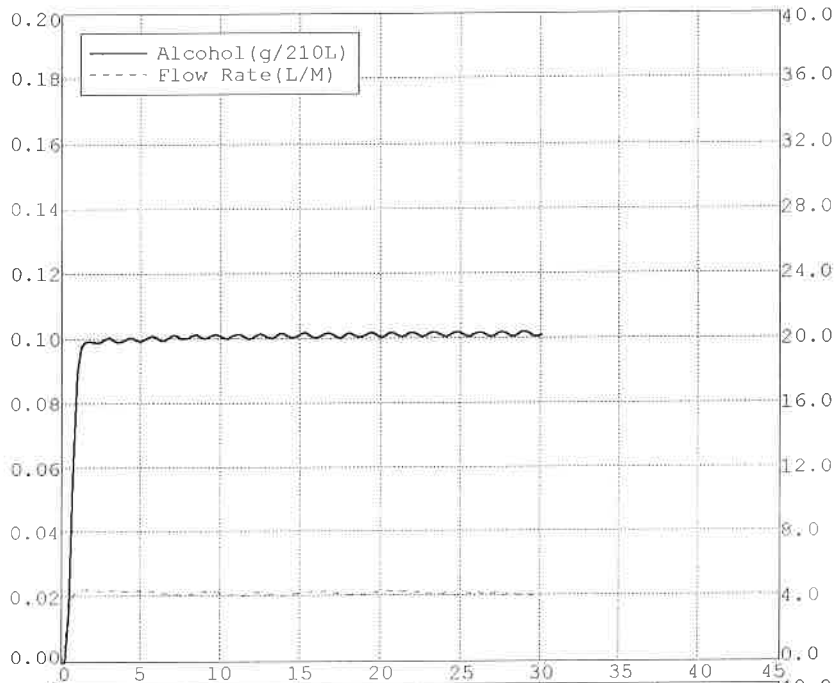

*Hollie B. Silverman* Rome PD 07/10/2020

*Hollie B. Silverman* 10115