

SOLUTION CHANGE

UTICA CITY  
POLICE DEPT  
DATAMASTER dmt: 100282




Date: 05/01/2020

OPERATOR NAME:  
MICHAEL J CLIVE  
Permit #: 36682  
Operator Agency/Dept: UTICA CITY PD  
Reference Standard #: 20040

*RM's*  
*20-11/189*

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:29
INTERNAL STANDARD	VERIFIED	12:29
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	12:29
BLANK TEST	0.00	12:30
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	12:30
BLANK TEST	0.00	12:31
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	12:31
BLANK TEST	0.00	12:32

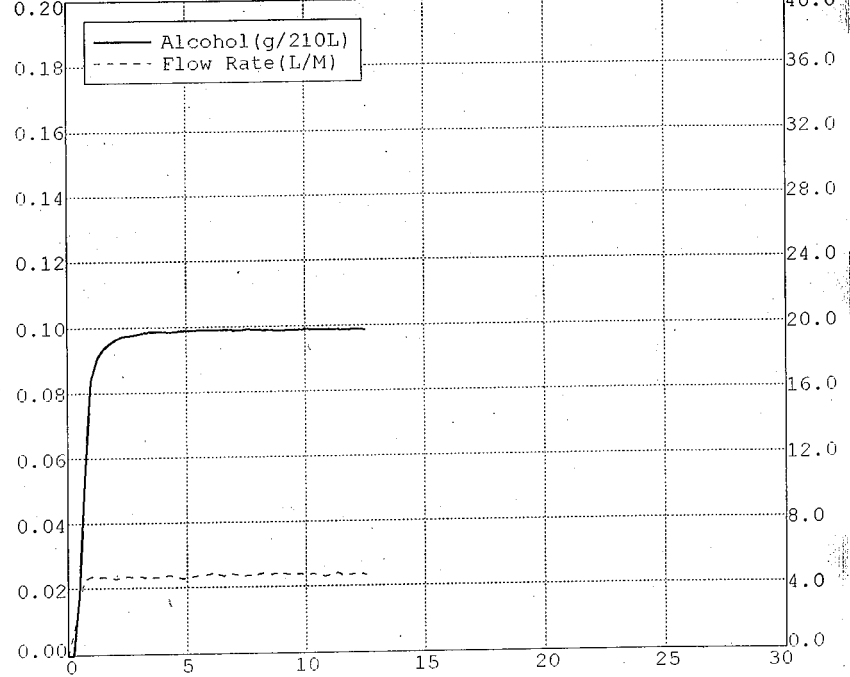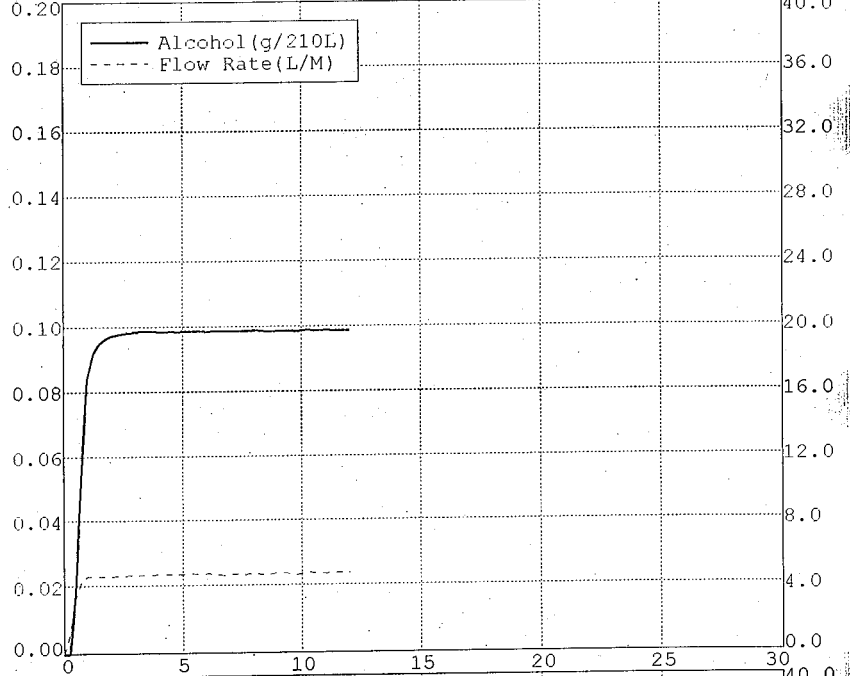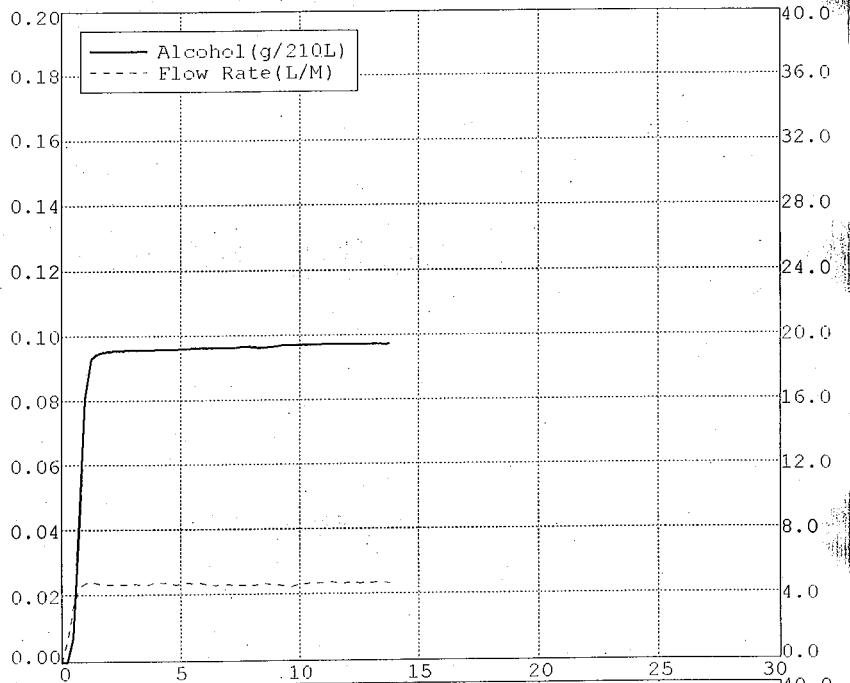

SOLUTION CHANGE

UTICA CITY  
 POLICE DEPT  
 DATAMASTER dmt: 107308

*RMS*  
*20-14/189*

Date: 05/01/2020

OPERATOR NAME:  
 MICHAEL J CLIVE  
 Permit #: 36682  
 Operator Agency/Dept: UTICA CITY PD  
 Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:11
INTERNAL STANDARD	VERIFIED	13:11
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	13:11
BLANK TEST	0.00	13:12
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	13:12
BLANK TEST	0.00	13:13
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	13:13
BLANK TEST	0.00	13:14

