

SUPERVISOR TEST

UTICA CITY
 POLICE DEPT
 DATAMASTER dmt: 107308




Date: 04/28/2020

RW
20-13798

OPERATOR NAME:
 MICHAEL J CLIVE
 Permit #: 36682
 Operator Agency/Dept: UTICA CITY PD
 Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:57
INTERNAL STANDARD	VERIFIED	11:57
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:57
BLANK TEST	0.00	11:58
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:58
BLANK TEST	0.00	11:59
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:00
BLANK TEST	0.00	12:00

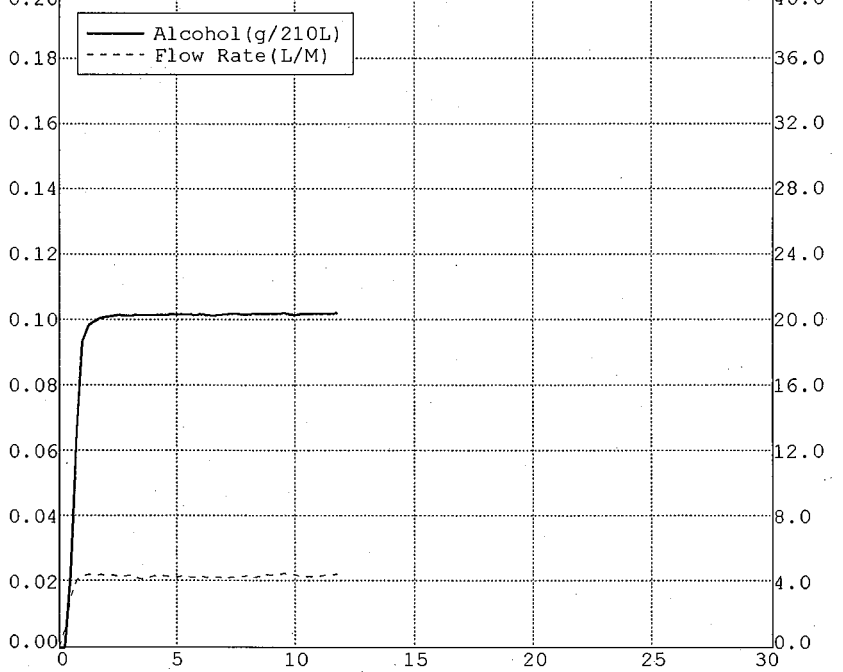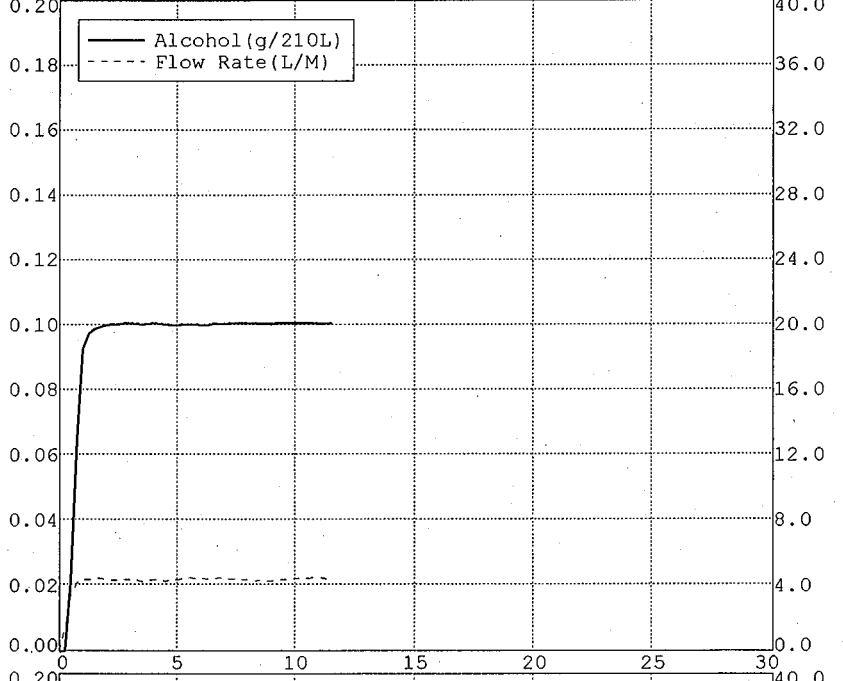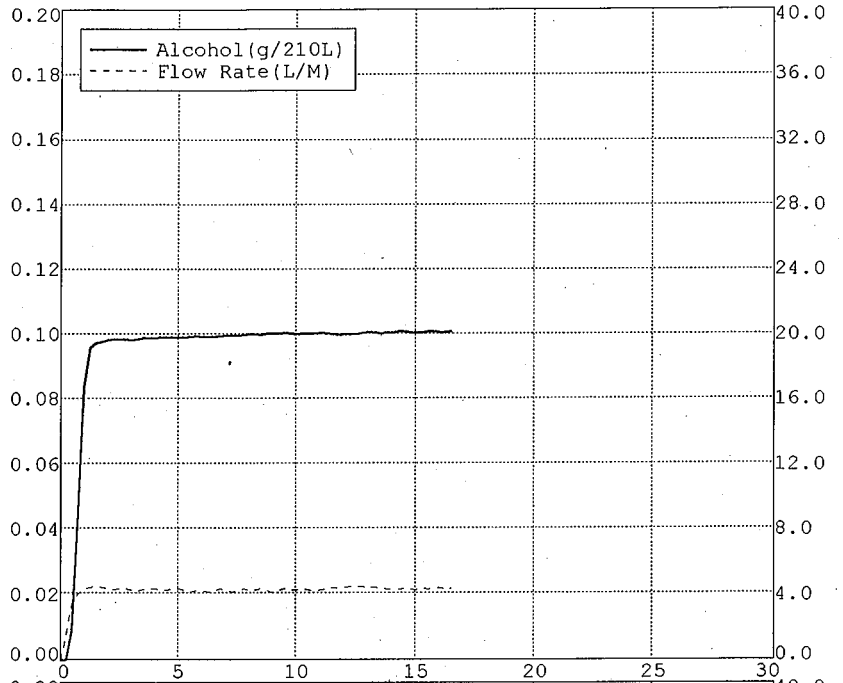

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282

Date: 04/28/2020

RM>
20-15798

OPERATOR NAME:
MICHEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:51
INTERNAL STANDARD	VERIFIED	11:51
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	11:51
BLANK TEST	0.00	11:52
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	11:52
BLANK TEST	0.00	11:53
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	11:53
BLANK TEST	0.00	11:54

