

BREATH INSTRUMENT  
CALIBRATION TEST RECORD

Dept. NEW HARTFORD POLICE DEPARTMENT

Inst. No. 127606

DATE	SOLUTION LOT NO.	TEST RESULTS			TEMP.	OPERATOR	SIMULATOR EQUILIBRA
		1	2	3			
3/1/20	19380					new solution	MPY199
3/1/20	19380	.10	.10	.10	34.0	Kawaler	" "
3/6/20	19380	.10	.10	.10	34.0	"	" "
3/13/20	19380	.10	.10	.10	34.0	"	" "
3/20/20	19380	.10	.10	.10	34.0	"	" "
3/27/20	19380	.10	.10	.10	34.0	"	" "
3/31/20	20040					new solution	" "
3/31/20	20040	.10	.10	.10	34.0	Kawaler	" "
4/7/20	20040	.10	.10	.10	34.0	"	" "
4/15/20	20040	.10	.10	.10	34.0	"	" "
4/22/20	20040	.10	.10	.10	34.0	"	" "
4/29/20	20040	.09	.10	.10	34.0	"	" "
5/3/20	20040					new solution	" "
5/3/20	20040	.10	.10	.10	34.0	Kawaler	" "
5/7/20	20040	.10	.10	.10	34.0	"	" "

**SUPERVISOR TEST**




NEW HARTFORD TOWN  
POLICE DEPT  
DATAMASTER dmt: 127606

Date: 04/15/2020

OPERATOR NAME:  
MICHAEL T KOWALSKI  
Permit #: 31077  
Operator Agency/Dept: NEW HARTFORD TOWN PD  
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:29
INTERNAL STANDARD	VERIFIED	07:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:30
BLANK TEST	0.00	07:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:31
BLANK TEST	0.00	07:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:32
BLANK TEST	0.00	07:33

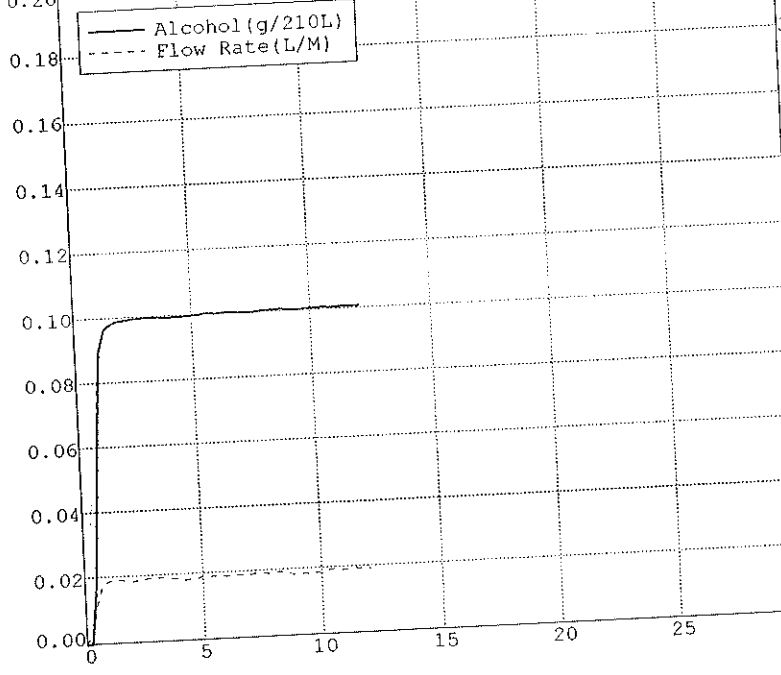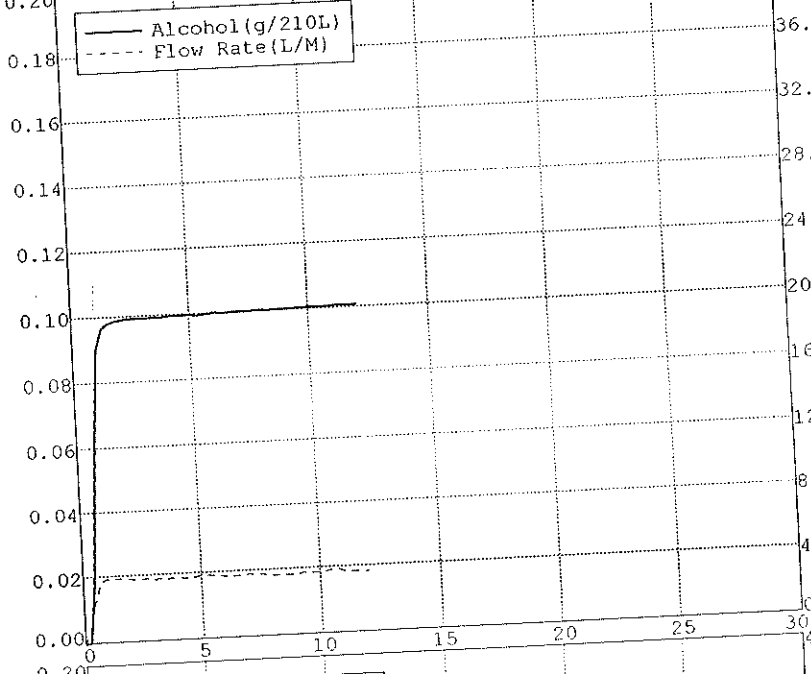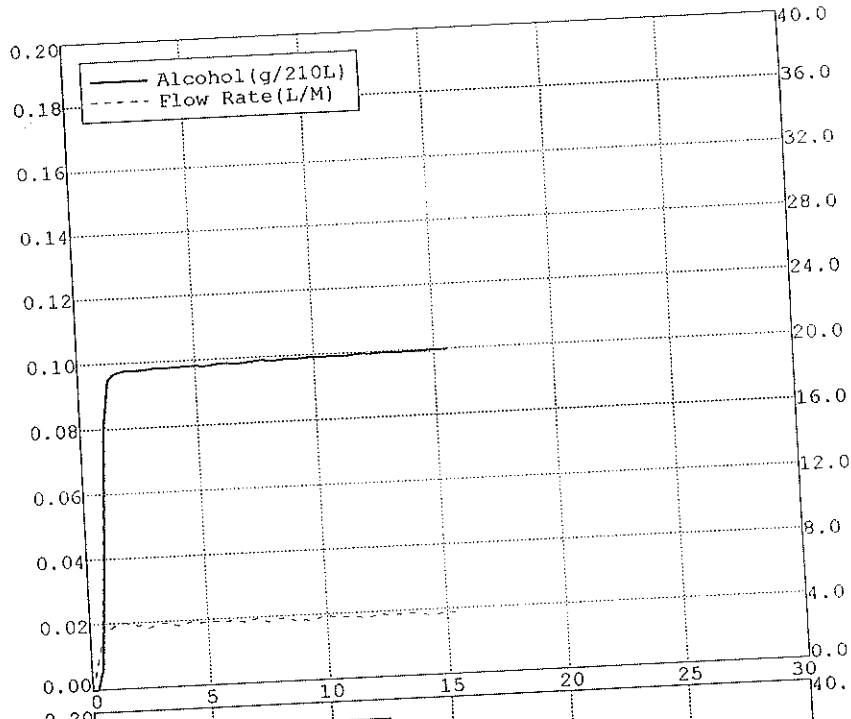

SUPERVISOR TEST




NEW HARTFORD TOWN  
POLICE DEPT  
DATAMASTER dmt: 127606

Date: 04/22/2020

OPERATOR NAME:  
MICHAEL T KOWALSKI  
Permit #: 31077  
Operator Agency/Dept: NEW HARTFORD TOWN PD  
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:32
INTERNAL STANDARD	VERIFIED	07:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:33
BLANK TEST	0.00	07:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:34
BLANK TEST	0.00	07:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:35
BLANK TEST	0.00	07:36

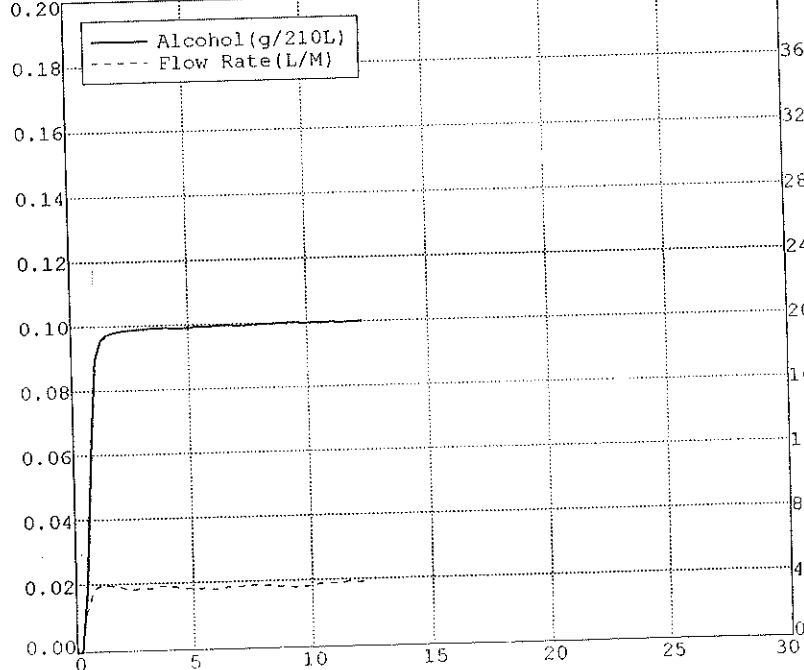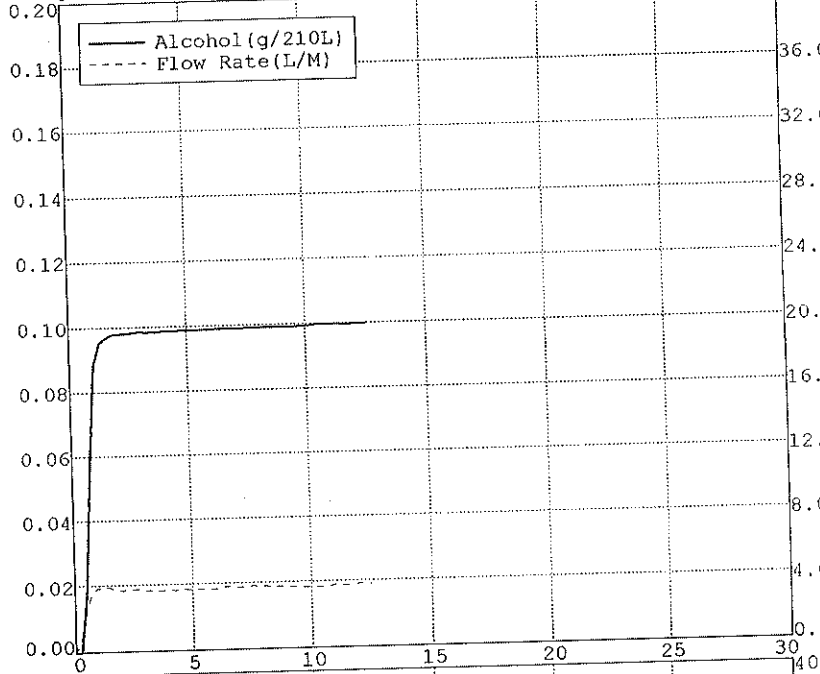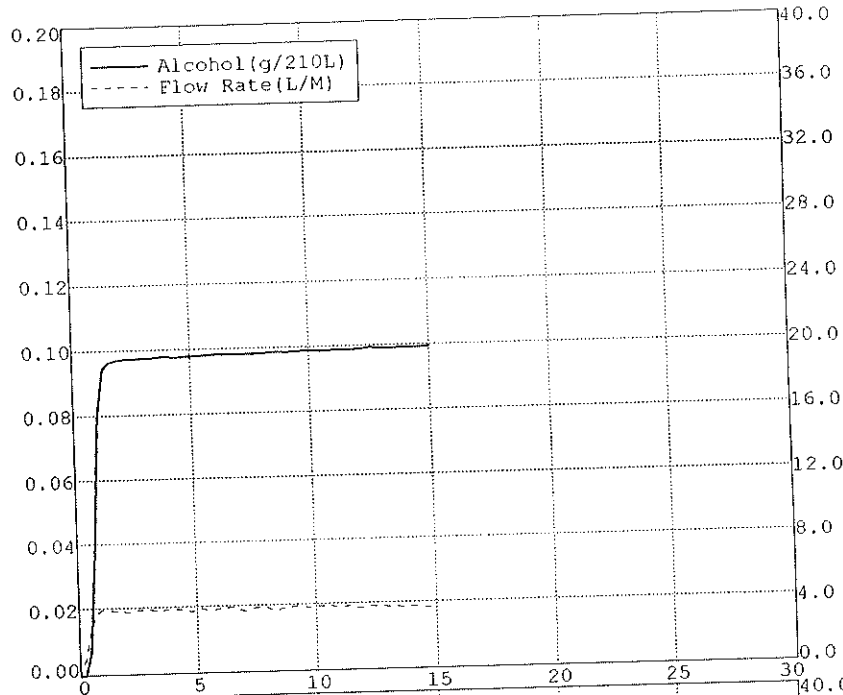

SUPERVISOR TEST




NEW HARTFORD TOWN  
POLICE DEPT  
DATAMASTER dmt: 127606

Date: 04/29/2020

OPERATOR NAME:  
MICHAEL T KOWALSKI  
Permit #: 31077  
Operator Agency/Dept: NEW HARTFORD TOWN PD  
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:33
INTERNAL STANDARD	VERIFIED	08:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	08:34
BLANK TEST	0.00	08:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:35
BLANK TEST	0.00	08:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:36
BLANK TEST	0.00	08:37

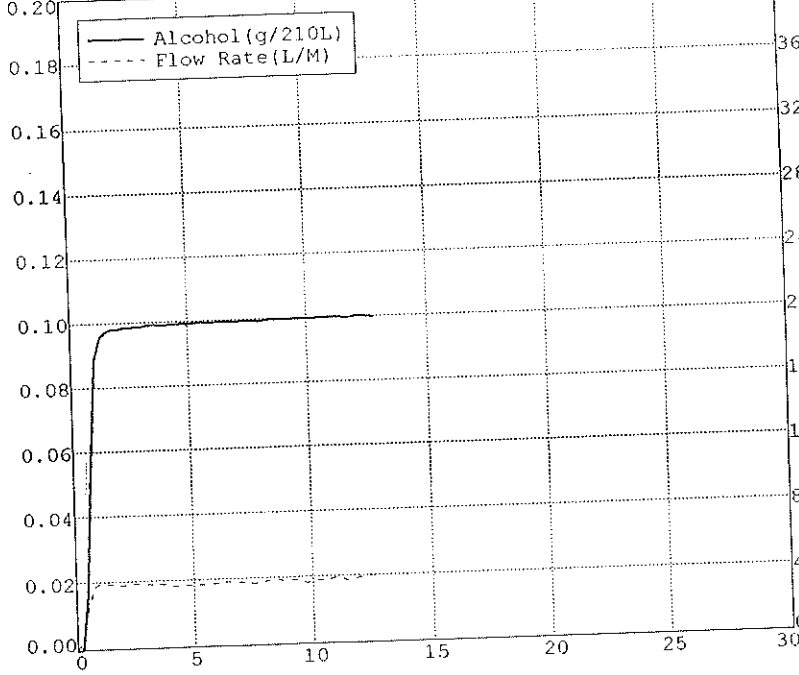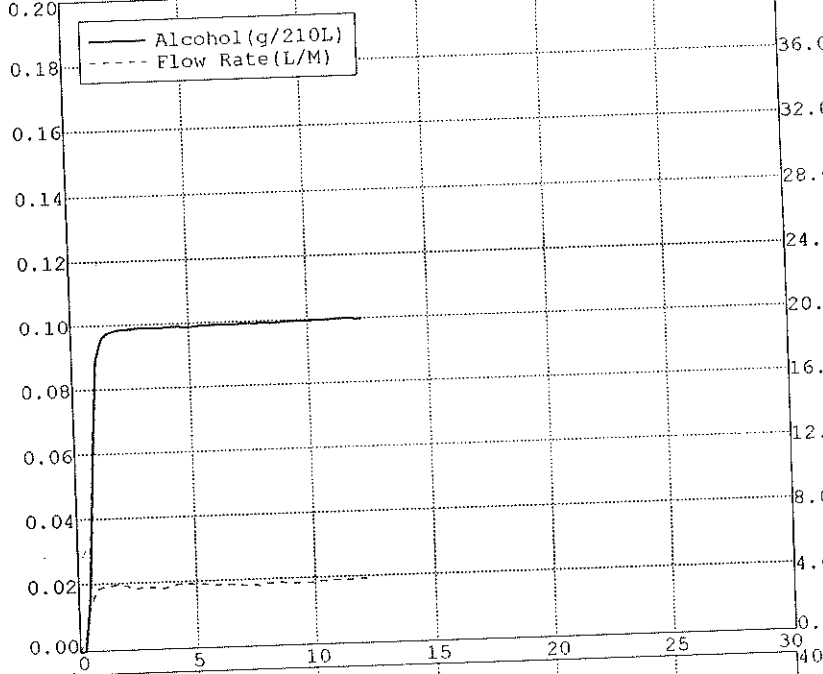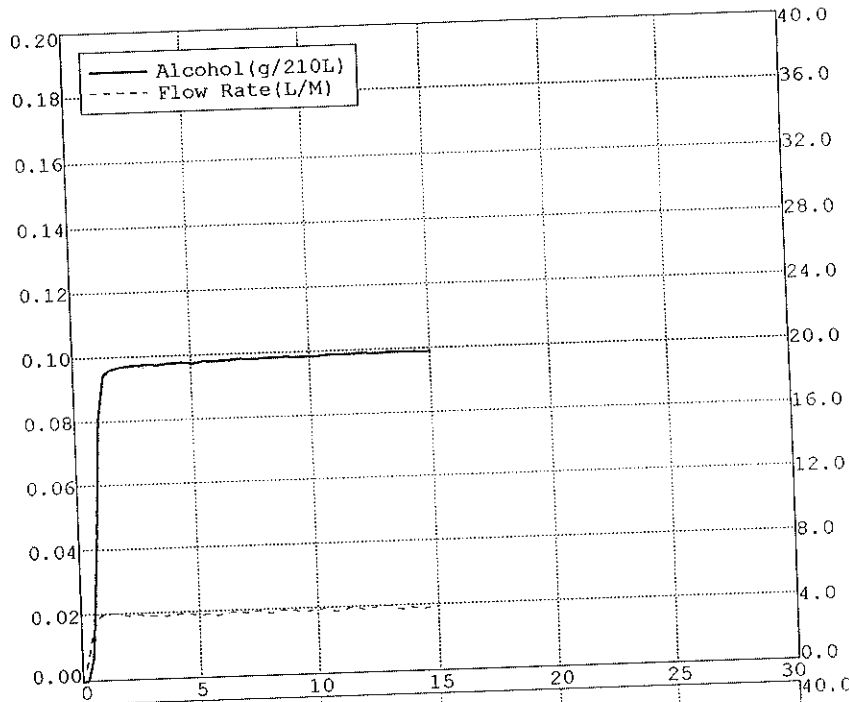

SUPERVISOR TEST *SC*




NEW HARTFORD TOWN  
POLICE DEPT  
DATAMASTER dmt: 127606

Date: 05/03/2020

OPERATOR NAME:  
MICHAEL T KOWALSKI  
Permit #: 31077  
Operator Agency/Dept: NEW HARTFORD TOWN PD  
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:48
INTERNAL STANDARD	VERIFIED	16:48
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:49
BLANK TEST	0.00	16:49
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:50
BLANK TEST	0.00	16:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:51
BLANK TEST	0.00	16:52

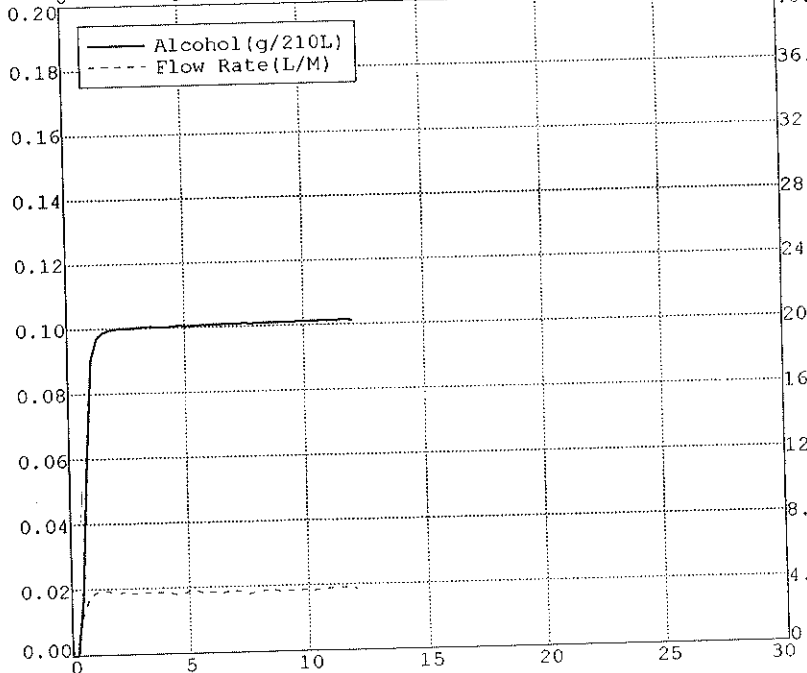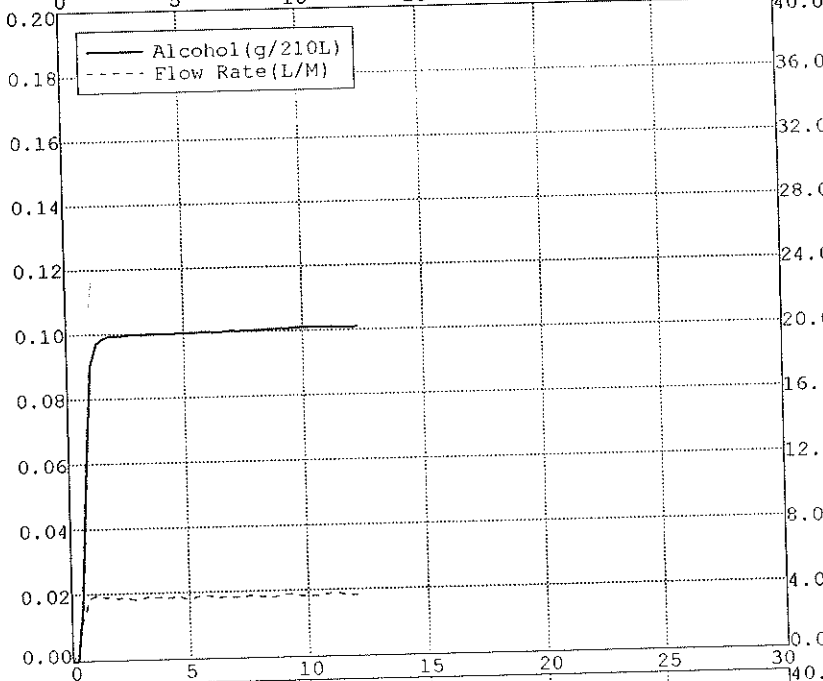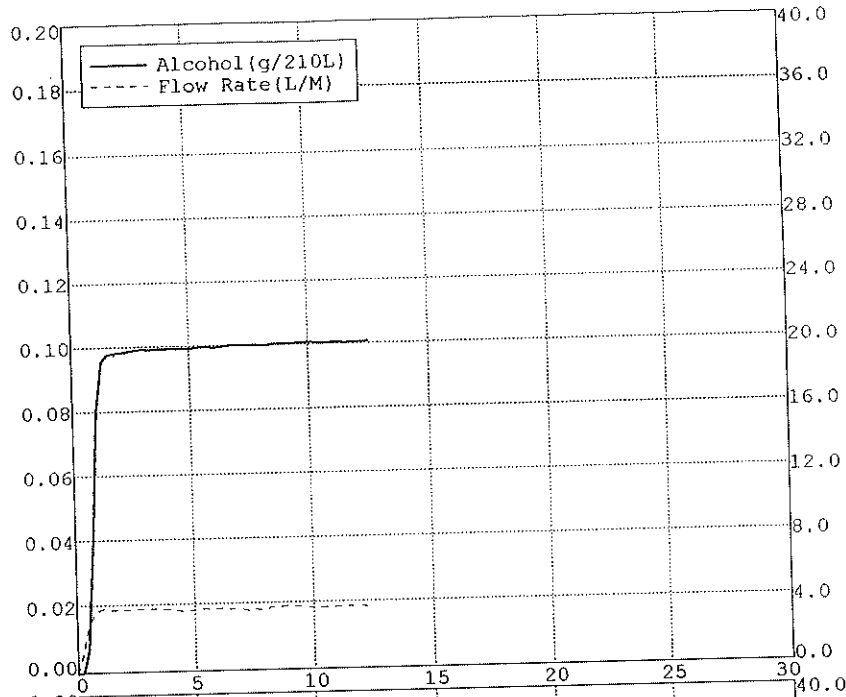

SUPERVISOR TEST

NEW HARTFORD TOWN  
POLICE DEPT  
DATAMASTER dmt: 127606

Date: 05/07/2020

OPERATOR NAME:  
MICHAEL T KOWALSKI  
Permit #: 31077  
Operator Agency/Dept: NEW HARTFORD TOWN PD  
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:22
INTERNAL STANDARD	VERIFIED	12:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:22
BLANK TEST	0.00	12:23
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:24
BLANK TEST	0.00	12:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:25
BLANK TEST	0.00	12:26

