



STATE OF NEW YORK  
DIVISION OF CRIMINAL JUSTICE SERVICES

Alfred E. Smith State Office Bldg.  
80 South Swan Street  
Albany, New York 12210  
<http://criminaljustice.ny.gov>

**CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS  
MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, Mark E. Fettinger, Supervisor of Public Safety Programs, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NAT'L PATENT ANALYTICAL SYS, DATAMASTER DMT breath test instrument, serial number 100197, performed on April 14, 2015 by Office of Public Safety employee Paul Hasbrouck, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/ maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

Digitally signed under  
ESRA by Mark E. Fettinger  
on 4/16/2015 11:44 AM

---

**Mark E. Fettinger**  
Supervisor of Public Safety Programs  
Office of Public Safety

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Oneida County Sheriff's Office

Manufacturer: NAT'L PATENT ANALYTICAL SYS

Model: DATAMASTER DMT

Date: April 14, 2015

Serial Number: 100197

Reference Solution Lot Number: 14160

Reference Solution Standard: 0.10 % at 34.0 degrees centigrade

| Test No | Test Result | Simulator Temperature    |
|---------|-------------|--------------------------|
| 1       | 0.102 %     | 33.99 degrees centigrade |
| 2       | 0.101 %     | 34.02 degrees centigrade |
| 3       | 0.101 %     | 34.00 degrees centigrade |
| 4       | 0.101 %     | 34.01 degrees centigrade |

Reference Solution Lot Number: 14120

Reference Solution Standard: 0.08 % at 34.0 degrees centigrade

| Test No | Test Result | Simulator Temperature    |
|---------|-------------|--------------------------|
| 1       | 0.082 %     | 34.02 degrees centigrade |
| 2       | 0.081 %     | 34.00 degrees centigrade |
| 3       | 0.081 %     | 34.01 degrees centigrade |
| 4       | 0.081 %     | 34.00 degrees centigrade |

Reference Solution Lot Number: 15030

Reference Solution Standard: 0.180 % at 34.0 degrees centigrade

| Test No | Test Result | Simulator Temperature    |
|---------|-------------|--------------------------|
| 1       | 0.181 %     | 34.01 degrees centigrade |
| 2       | 0.180 %     | 34.00 degrees centigrade |
| 3       | 0.180 %     | 34.01 degrees centigrade |
| 4       | 0.181 %     | 34.00 degrees centigrade |

I hereby certify that I have performed any necessary maintenance procedures and calibrated NAT'L PATENT ANALYTICAL SYS breath test instrument model DATAMASTER DMT, serial number 100197, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.

Performed by:



Digitally signed under  
ESRA by Paul Hasbrouck  
on 4/14/2015 2:16 PM

Reviewed by:



Digitally signed under  
ESRA by Lisa A. Lee  
on 4/16/2015 10:43 AM

**Paul Hasbrouck**  
Highway Safety Equipment Technician  
Breath Analysis Operator Permit # 30738

**Lisa A. Lee**  
Highway Safety Equipment Technical  
Supervisor  
Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

**Name of Submitting Agency: Oneida County Sheriff's Office**  
**Manufacturer: NAT'L PATENT ANALYTICAL SYS**  
**Model: DATAMASTER DMT**  
**Serial Number: 100197**  
**Date: April 14, 2015**

**1. General Appearance and condition of this device -----: OK, LAB MAINT.**


**2. Check controls and indicators -----: OK**

**3. Check breath flow system -----: OK**

**4. Check printer operation -----: OK**

**5. System cycles through all modes -----: OK**

**6. Record any repairs made to this instrument and list services provided: RUN CALIBRATION, RUN DIAGNOSTIC, TECHNICIAN, SUPERVISOR, SUBJECT, AND COMMUNICATION TEST, VERIFIED CALIBRATION, OK**

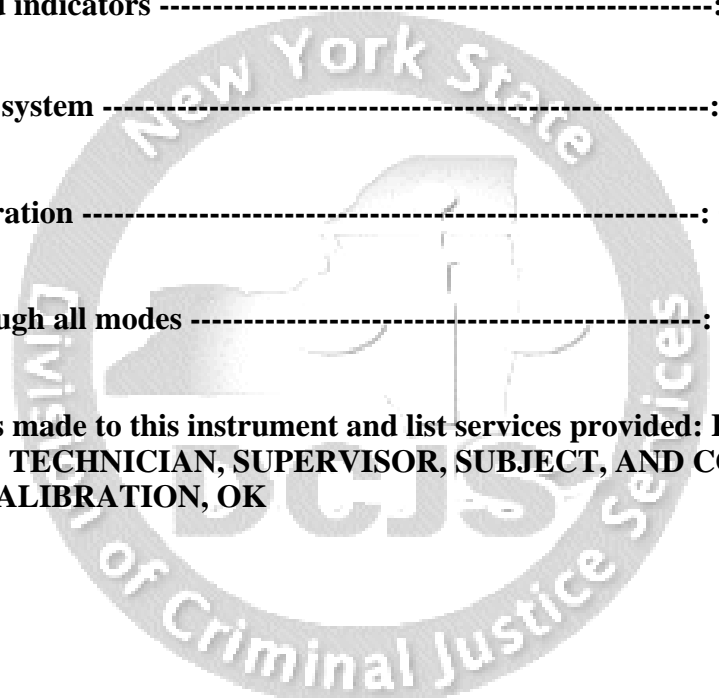

Performed by:

Digitally signed under  
ESRA by Paul Hasbrouck  
on 4/14/2015 2:16 PM

---

**Paul Hasbrouck**  
**Highway Safety Equipment Technician**  
**Breath Analysis Operator Permit # 30738**

Reviewed by:

Digitally signed under  
ESRA by Lisa A. Lee  
on 4/16/2015 10:43 AM

---

**Lisa A. Lee**  
**Highway Safety Equipment Technical**  
**Supervisor**  
**Breath Analysis Technical Supervisor**