

SOLUTION CHANGE

WFO



ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 100197

Date: 07/04/2019

OPERATOR NAME:
EMRAH LATIC
Permit #: 46908
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:29
INTERNAL STANDARD	VERIFIED	01:30
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	01:30
BLANK TEST	0.00	01:31
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	01:31
BLANK TEST	0.00	01:32
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	01:32
BLANK TEST	0.00	01:33

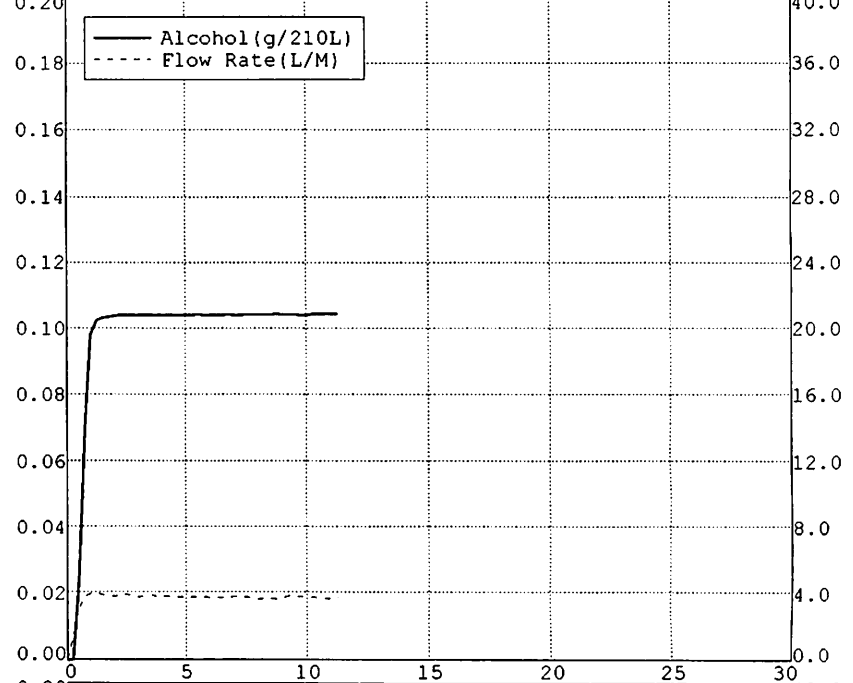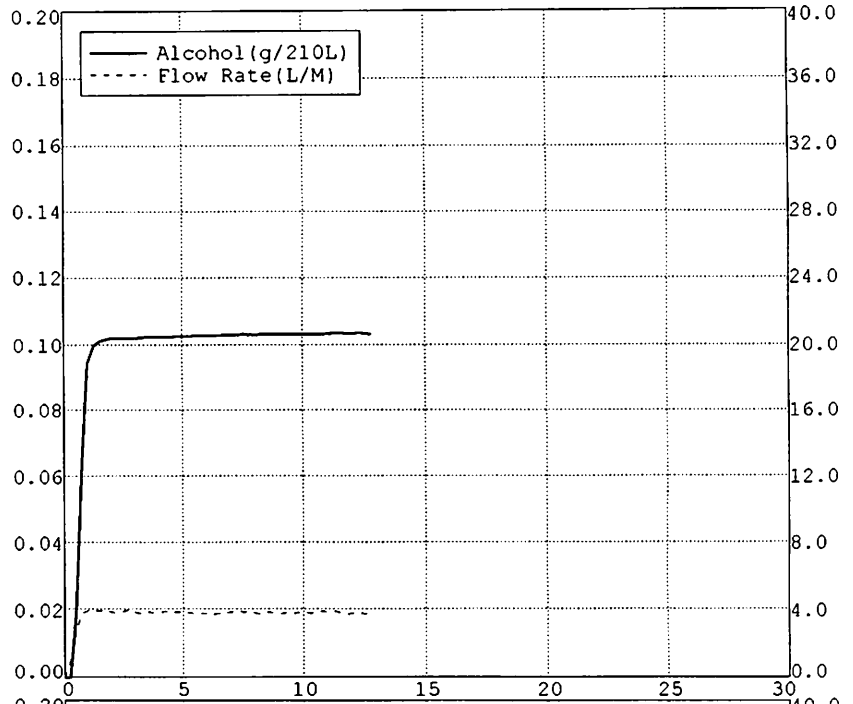

SUPERVISOR TEST

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 100197




Date: 07/10/2019

OPERATOR NAME:
MICHAEL P GIBBONS
Permit #: 45972
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:57
INTERNAL STANDARD	VERIFIED	18:57
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	18:58
BLANK TEST	0.00	18:59
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	18:59
BLANK TEST	0.00	19:00
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	19:00
BLANK TEST	0.00	19:01

*WFO Datamaster
Weekly Test*

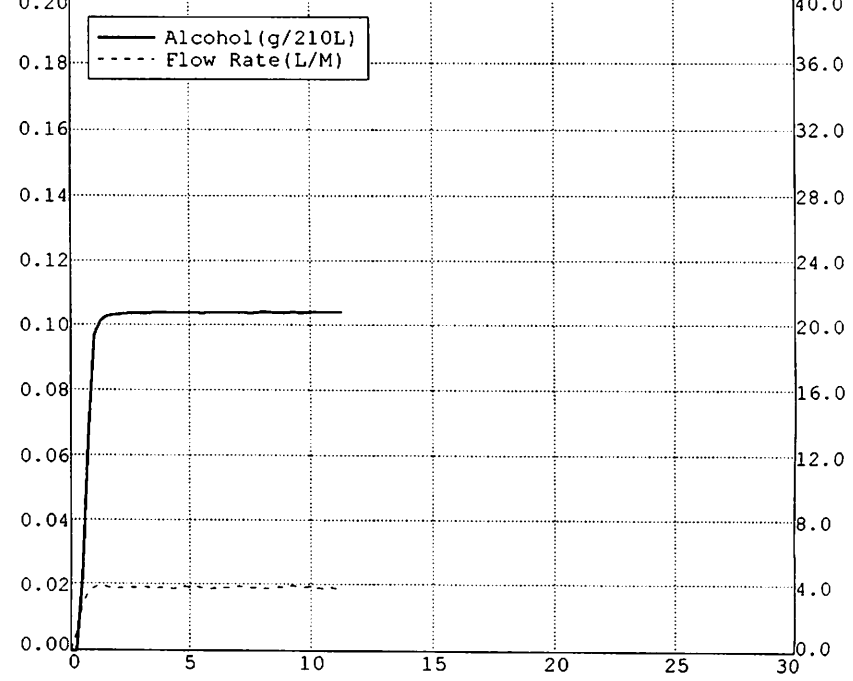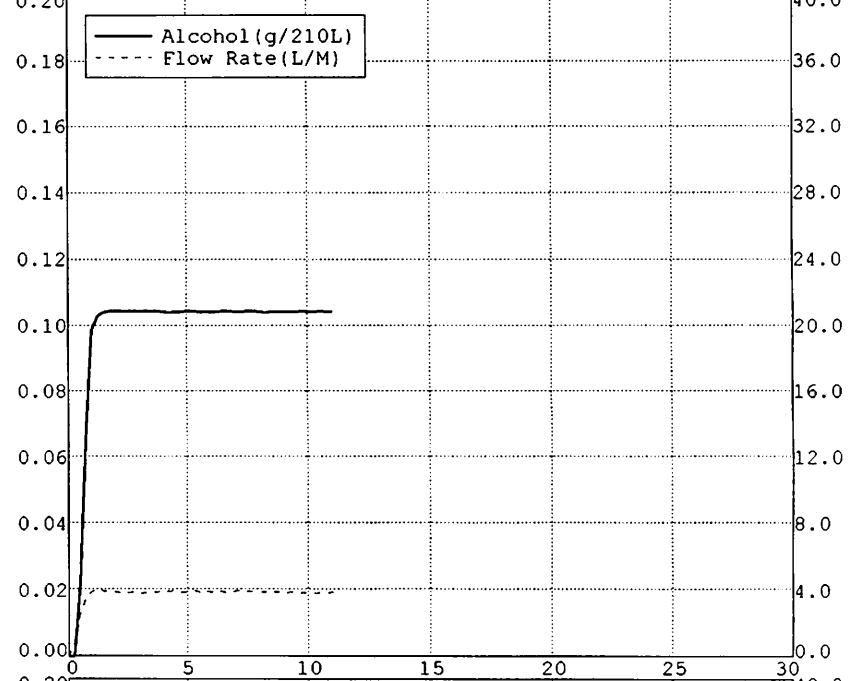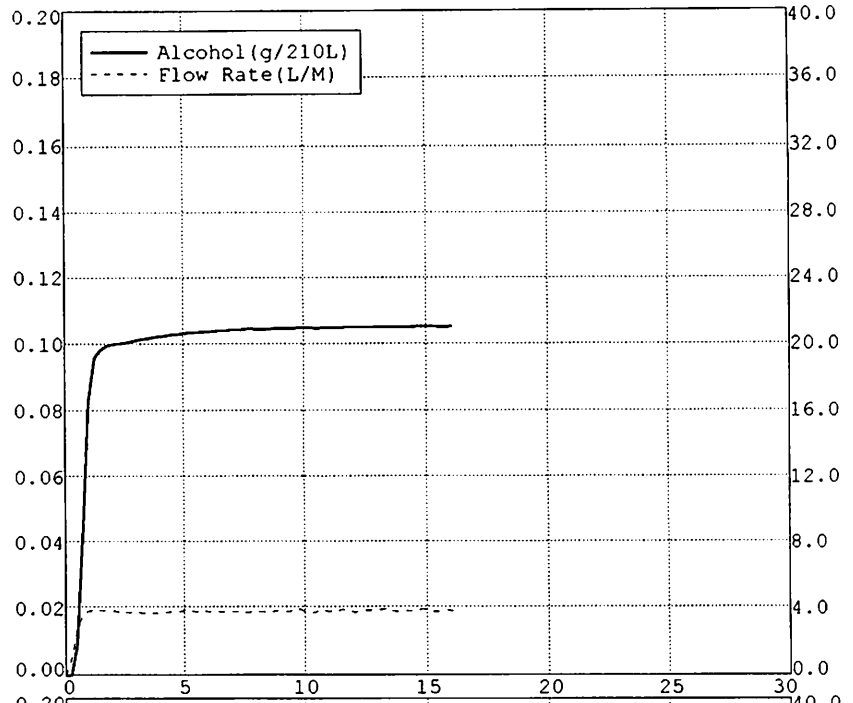

SUPERVISOR TEST

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 100197




Date: 07/18/2019

OPERATOR NAME:
MICHAEL P GIBBONS
Permit #: 45972
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:24
INTERNAL STANDARD	VERIFIED	06:24
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.10	06:24
BLANK TEST	0.00	06:25
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.10	06:25
BLANK TEST	0.00	06:26
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	06:27
BLANK TEST	0.00	06:28

WFO week
Datamaster

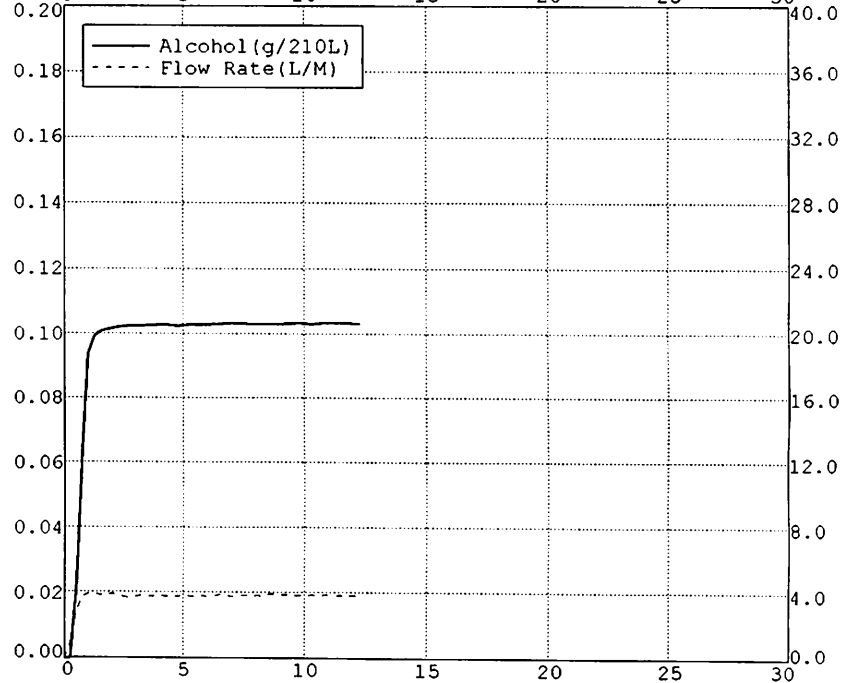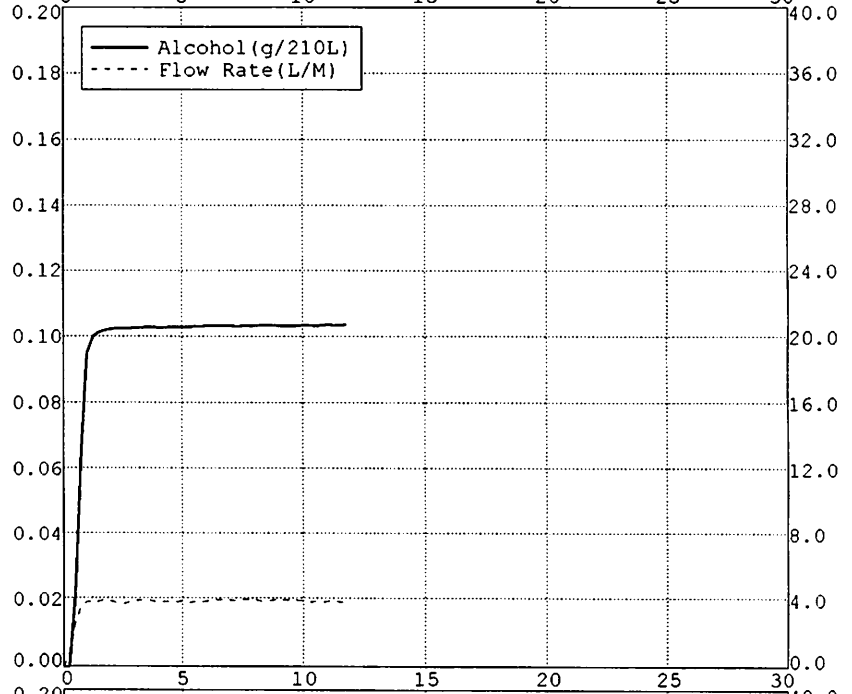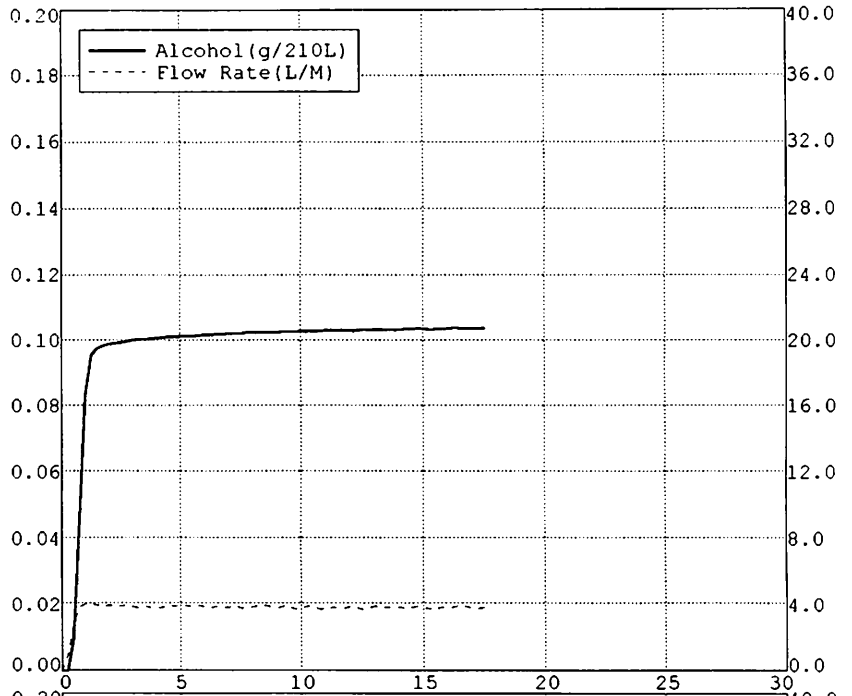

SUPERVISOR TEST

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 100197




Date: 07/24/2019

OPERATOR NAME:
MICHAEL P GIBBONS
Permit #: 45972
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:54
INTERNAL STANDARD	VERIFIED	20:54
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	20:54
BLANK TEST	0.00	20:55
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	20:55
BLANK TEST	0.00	20:56
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	20:57
BLANK TEST	0.00	20:57

WFO Datamaster
Weekly Test

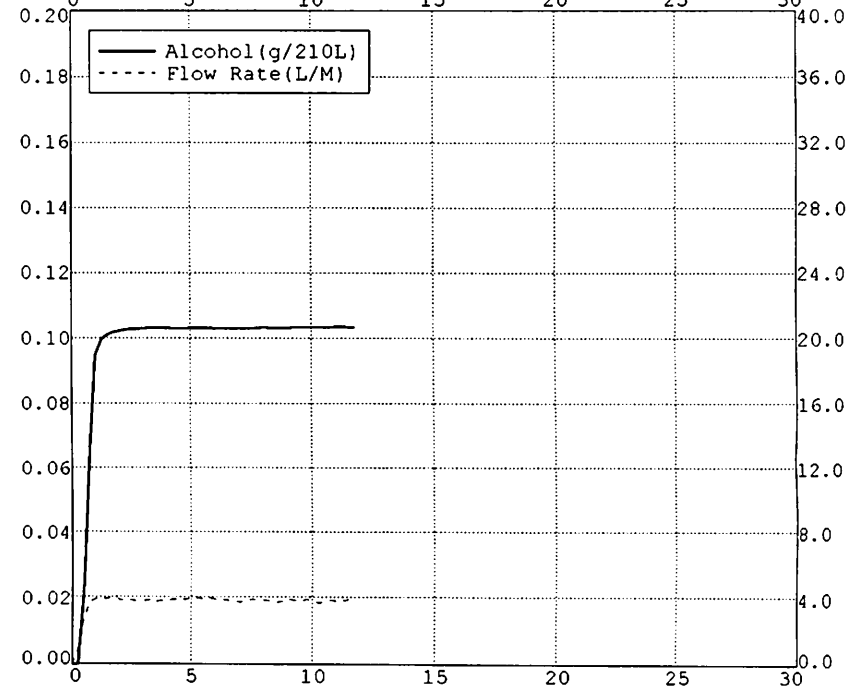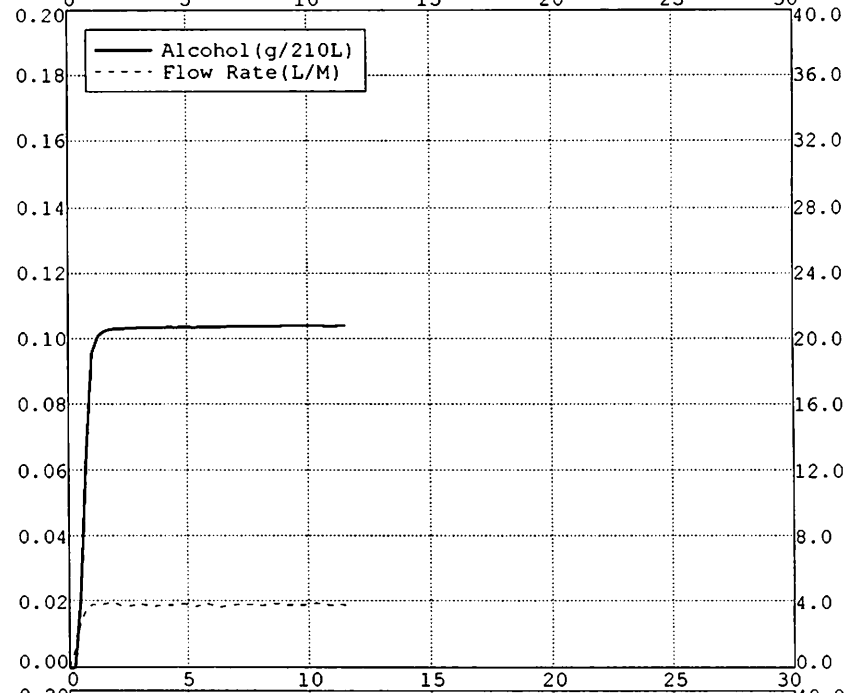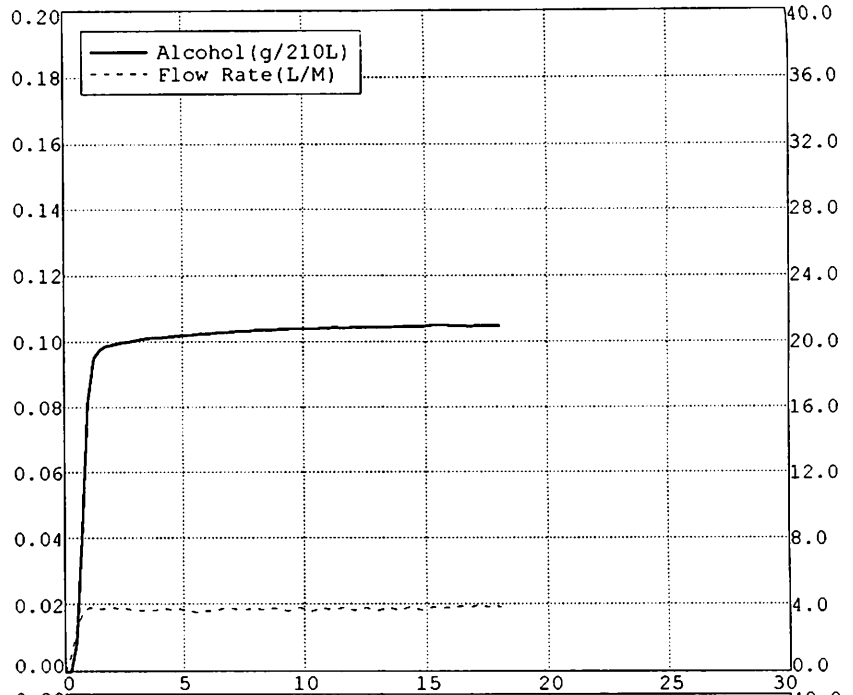

SOLUTION CHANGE



ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 100197

Date: 08/01/2019

OPERATOR NAME:
BRANDON J RUTLEDGE
Permit #: 43762
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:09
INTERNAL STANDARD	VERIFIED	22:10
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	22:10
BLANK TEST	0.00	22:11
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	22:11
BLANK TEST	0.00	22:12
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	22:12
BLANK TEST	0.00	22:13

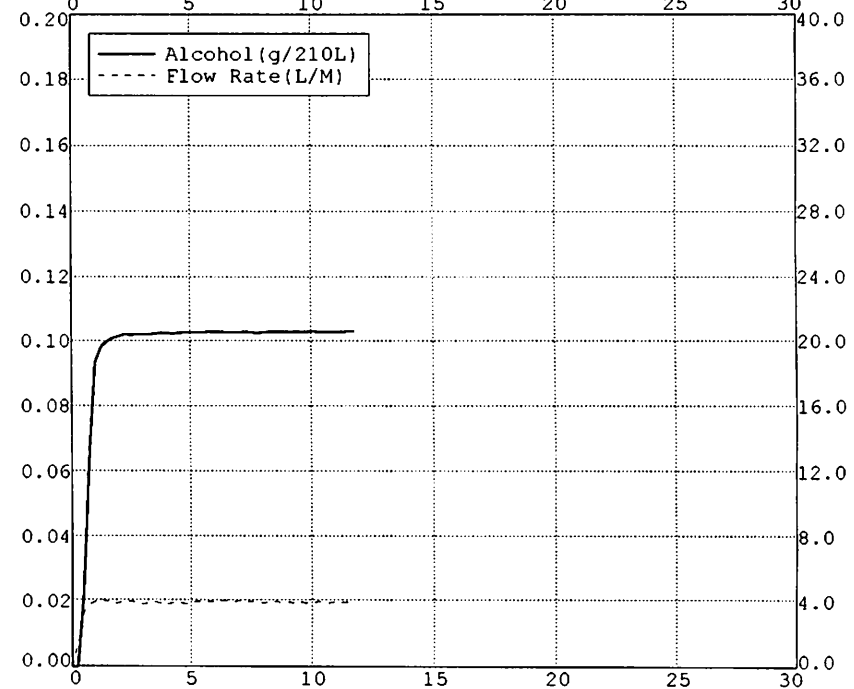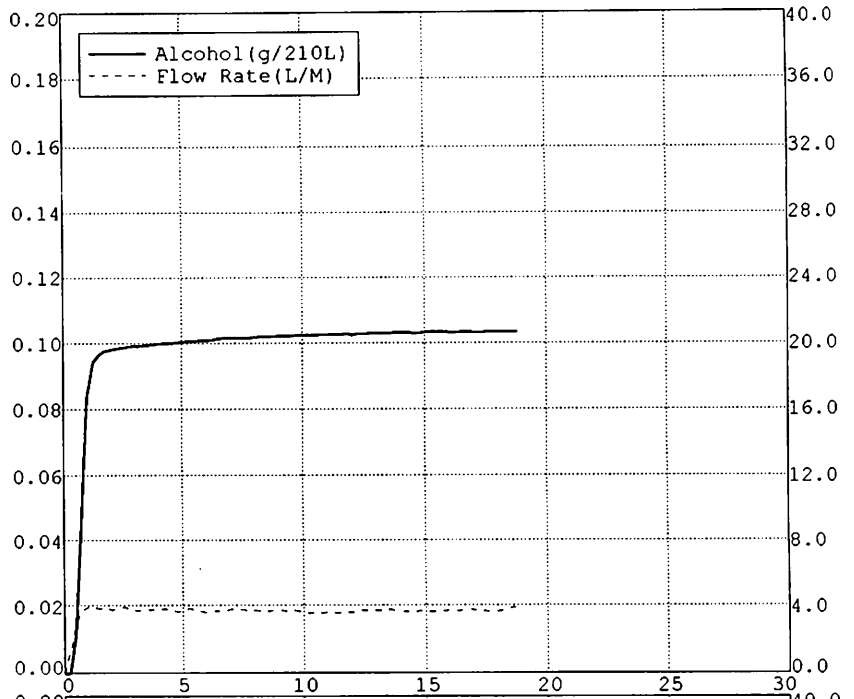

SUPERVISOR TEST

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 100197




Date: 08/07/2019

OPERATOR NAME:
MICHAEL P GIBBONS
Permit #: 45972
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:24
INTERNAL STANDARD	VERIFIED	18:24
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	18:24
BLANK TEST	0.00	18:25
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.10	18:25
BLANK TEST	0.00	18:26
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.10	18:27
BLANK TEST	0.00	18:27

WFO Weekly Test

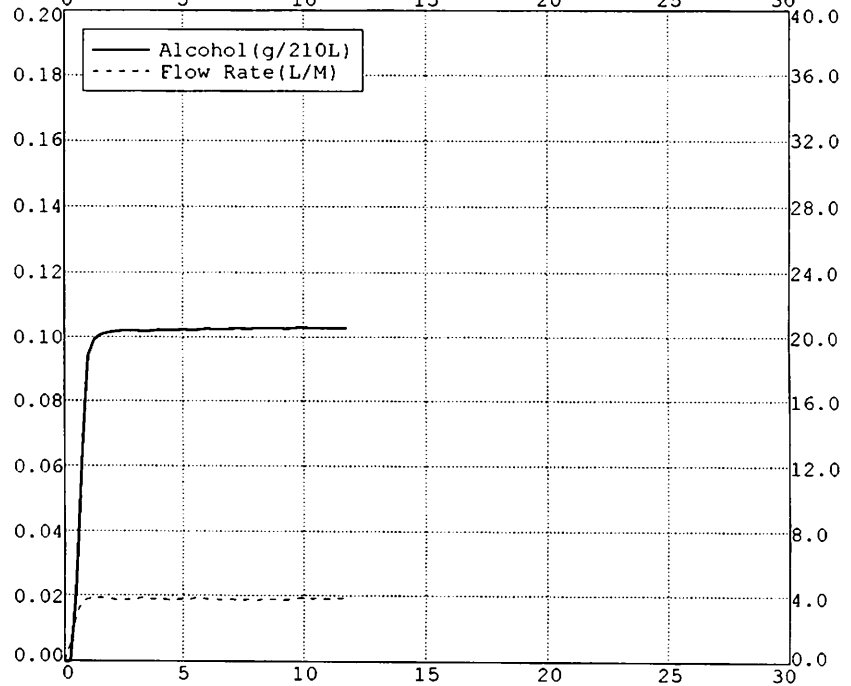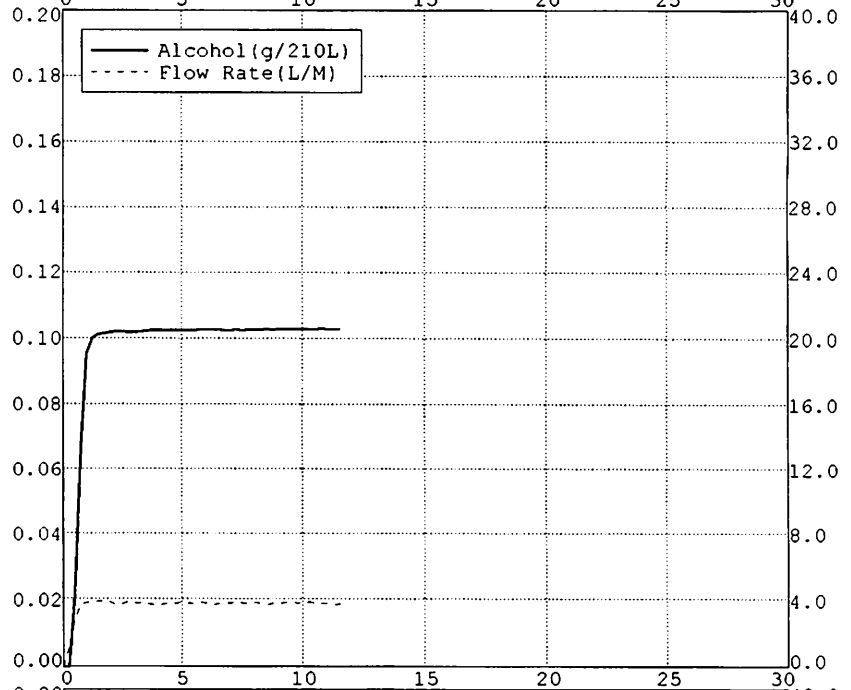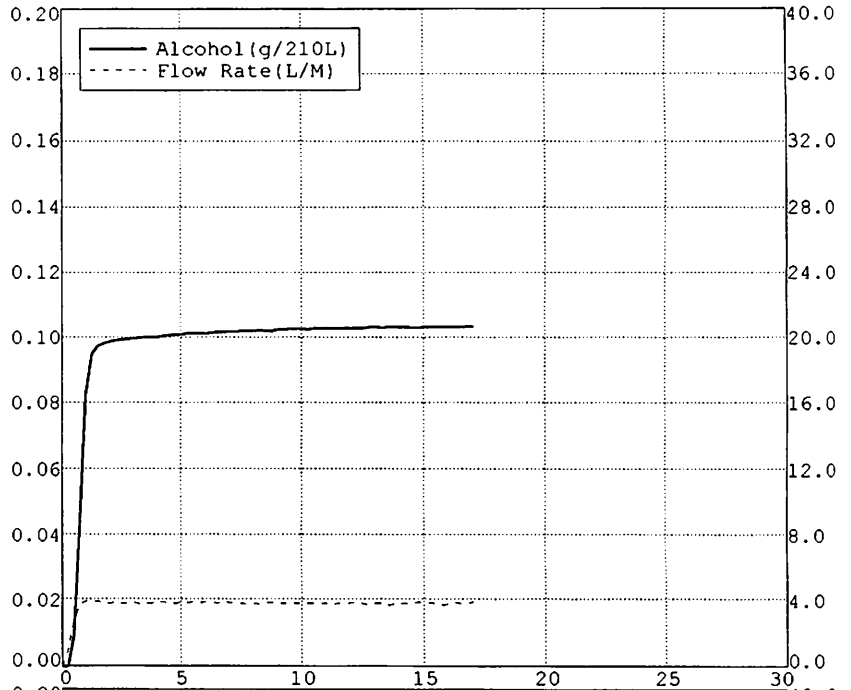

SUPERVISOR TEST




ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 100197

Date: 08/14/2019

OPERATOR NAME:
BRANDON J RUTLEDGE
Permit #: 43762
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:51
INTERNAL STANDARD	VERIFIED	23:51
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	23:52
BLANK TEST	0.00	23:52
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	23:53
BLANK TEST	0.00	23:54
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	23:54
BLANK TEST	0.00	23:55

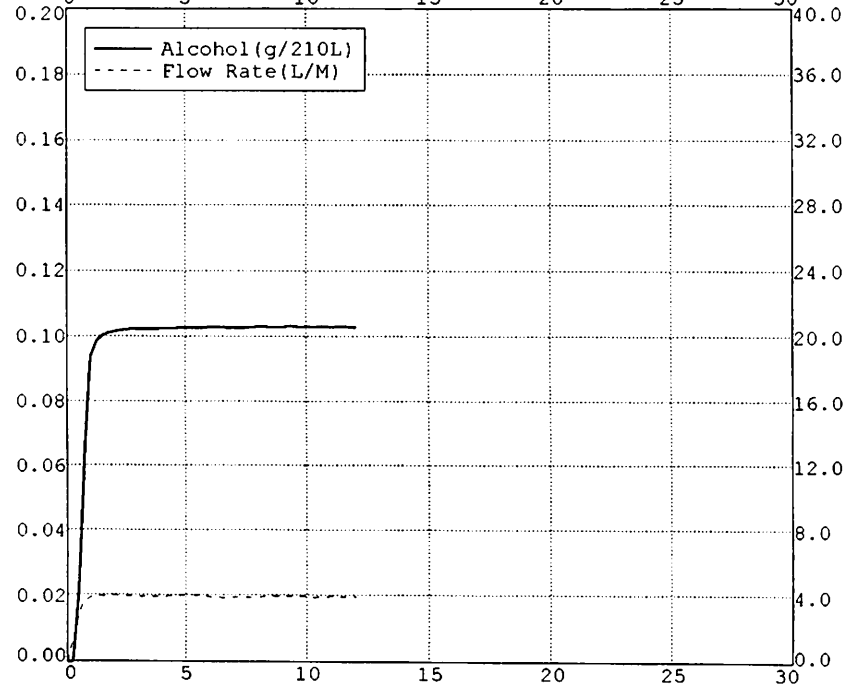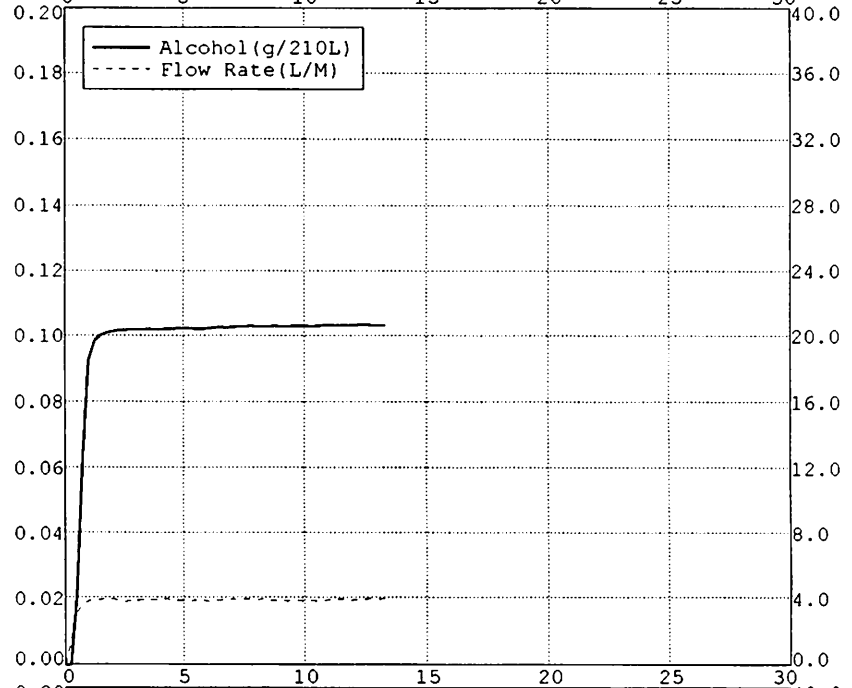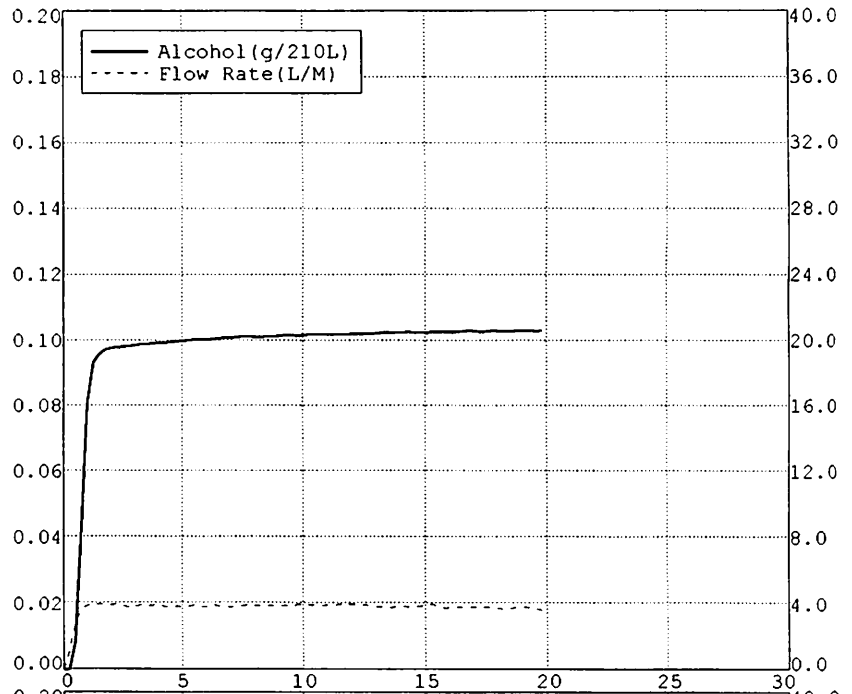

SUBJECT TEST

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 100197

Date: 08/14/2019

OPERATOR NAME:
BRANDON J RUTLEDGE
OPERATOR PERMIT NUMBER: 43762
OPERATOR AGENCY/DEPT:
ONEIDA CO. S.O.
REFERENCE STANDARD NUMBER:
19130

---BREATH ANALYSIS---

User Abort

ACCIDENTLY HIT SUBJECT TEST
INSTEAD OF SUPERVISOR TEST
-RUTLEDGE BY #74

I, _____, am employed by the _____, a government agency, and, having been delegated by my employer to do so, certify that the above record of blood alcohol content analysis was made in the regular and ordinary course of business of this agency; that it is the regular and ordinary course of business of this agency to perform analysis of blood alcohol content and to make records of such analysis at the time they are performed; that the entries appearing on the above record were made at or soon after the time of the acts, transactions, occurrences, or events stated thereon; that this record, if a copy, is a complete and exact duplicate of the original thereof; and that it is part of my employment responsibilities to maintain custody or control of this record.

Date	Signature	Title
Operator Name, Rank and Department:		Permit Number:

SUPERVISOR TEST

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 100197



Date: 08/22/2019

OPERATOR NAME:
MICHAEL P GIBBONS
Permit #: 45972
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:58
INTERNAL STANDARD	VERIFIED	04:58
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	04:59
BLANK TEST	0.00	05:00
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	05:00
BLANK TEST	0.00	05:01
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	05:01
BLANK TEST	0.00	05:02

WFO Weekly Test

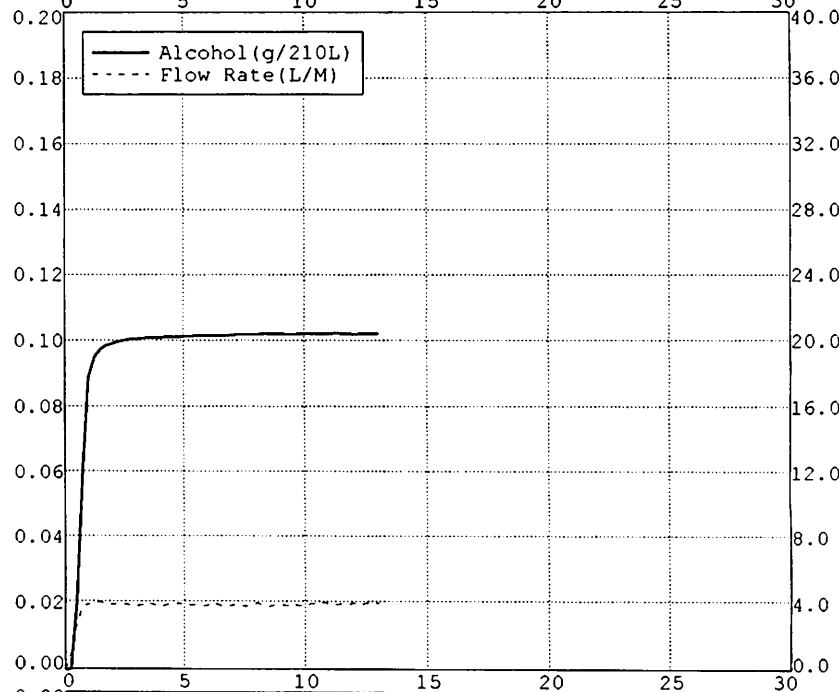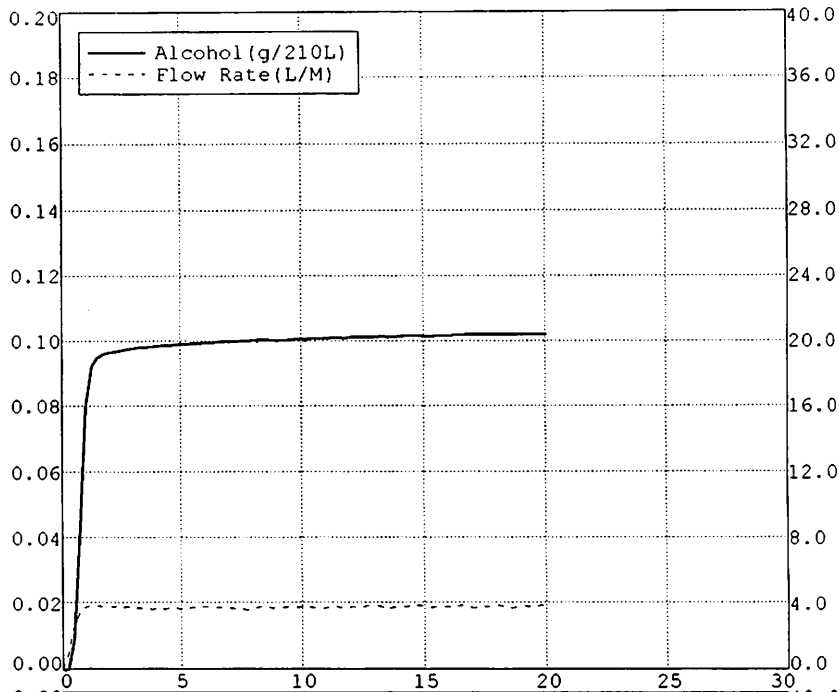

SUPERVISOR TEST

WFO



ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 100197

Date: 08/28/2019

OPERATOR NAME:
JOHN R BOWERS
Permit #: 46887
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:47
INTERNAL STANDARD	VERIFIED	21:47
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	21:48
BLANK TEST	0.00	21:48
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	21:49
BLANK TEST	0.00	21:50
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	21:50
BLANK TEST	0.00	21:51

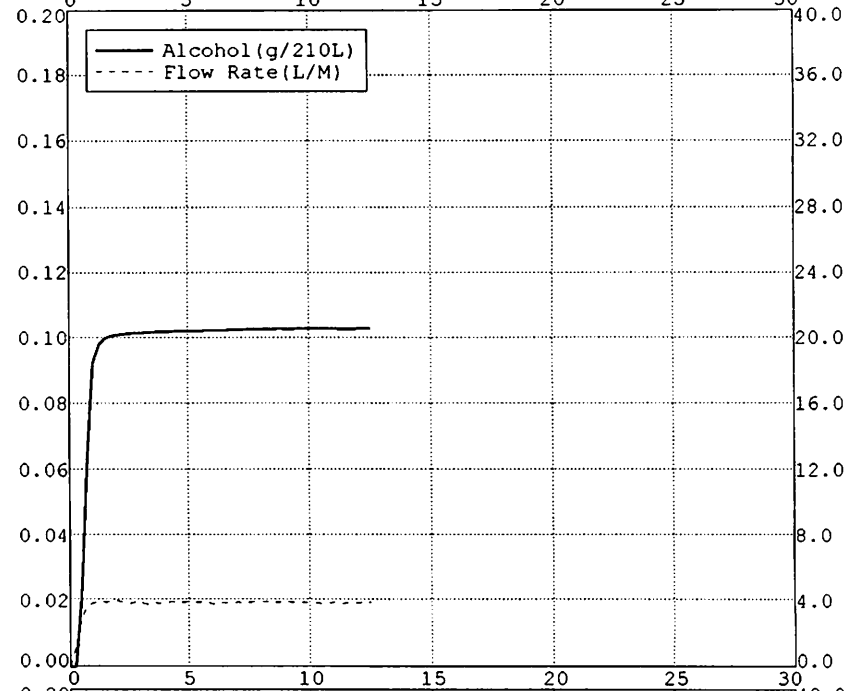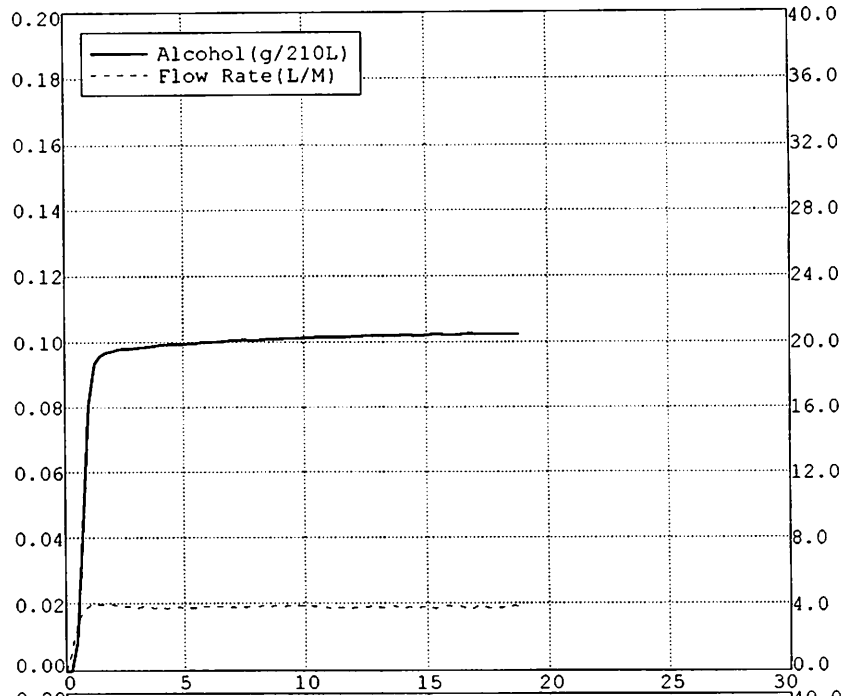

SUPERVISOR TEST



ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 100197

Date: 09/01/2019

OPERATOR NAME:
MICHAEL P GIBBONS
Permit #: 45972
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:17
INTERNAL STANDARD	VERIFIED	19:18
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	19:18
BLANK TEST	0.00	19:19
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.10	19:19
BLANK TEST	0.00	19:20
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	19:20
BLANK TEST	0.00	19:21

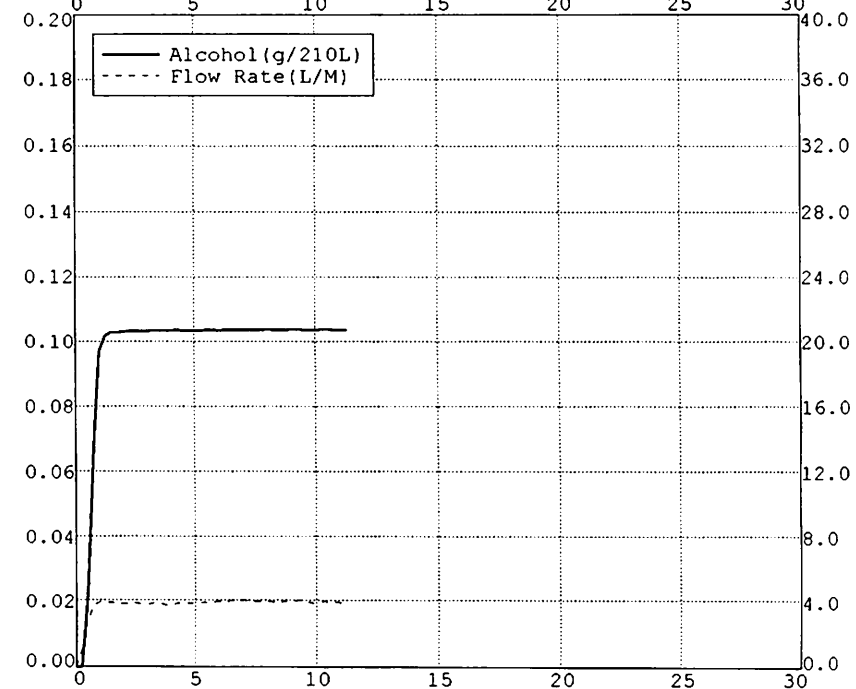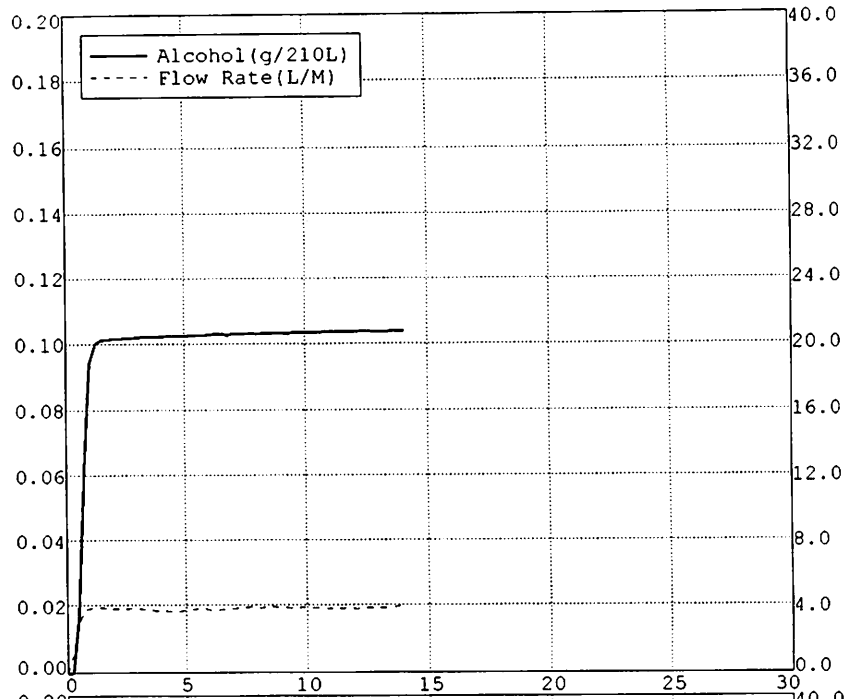

SUPERVISOR TEST

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 100197



Date: 09/04/2019

OPERATOR NAME:
MICHAEL P GIBBONS
Permit #: 45972
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:22
INTERNAL STANDARD	VERIFIED	22:22
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	22:22
BLANK TEST	0.00	22:23
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	22:24
BLANK TEST	0.00	22:25
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	22:25
BLANK TEST	0.00	22:26

*WFO Datamaster
weekly*

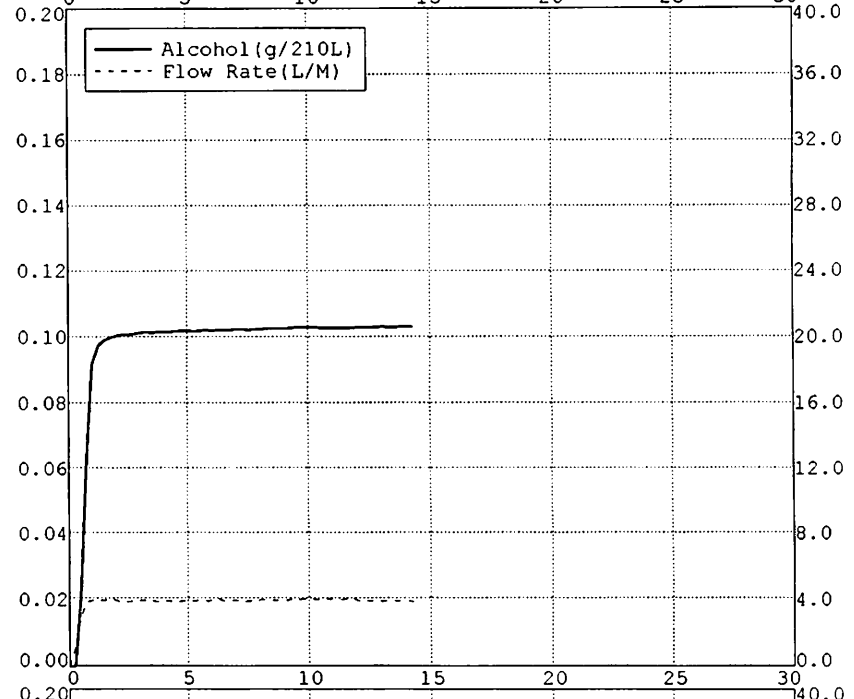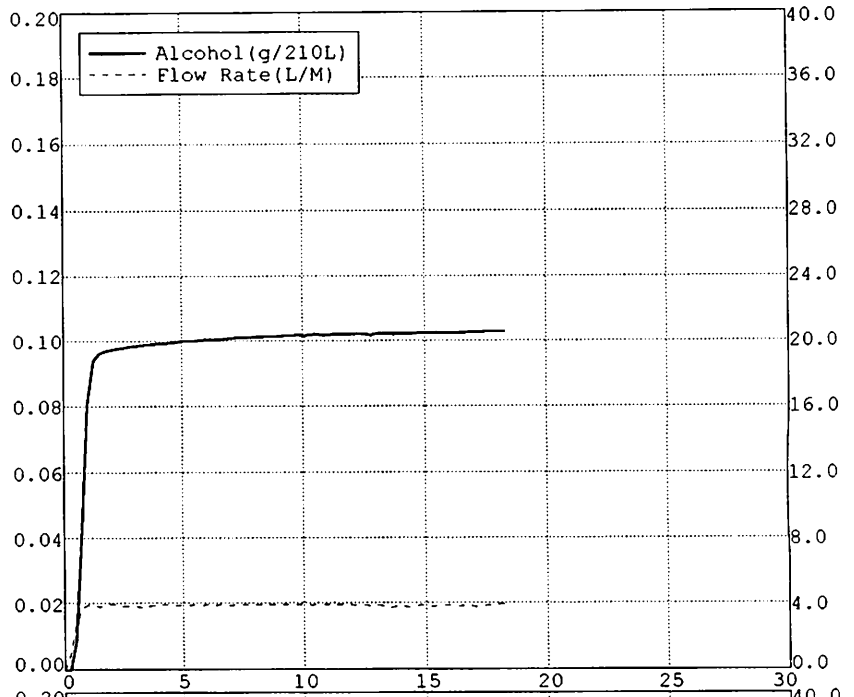

SUPERVISOR TEST

WFO




ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 100197

Date: 09/11/2019

OPERATOR NAME:
JOHN R BOWERS
Permit #: 46887
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:13
INTERNAL STANDARD	VERIFIED	21:13
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	21:14
BLANK TEST	0.00	21:15
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	21:15
BLANK TEST	0.00	21:16
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	21:16
BLANK TEST	0.00	21:17

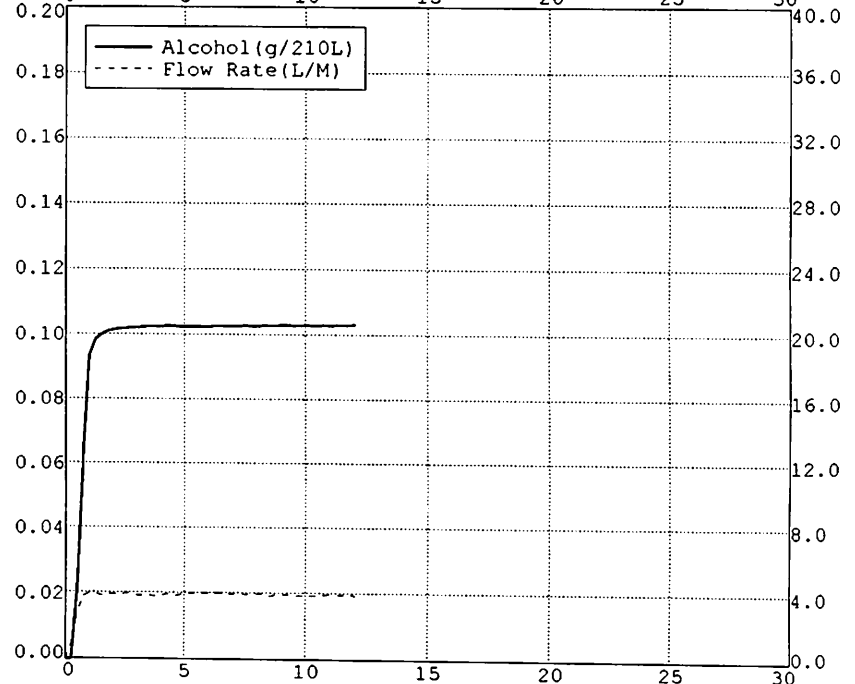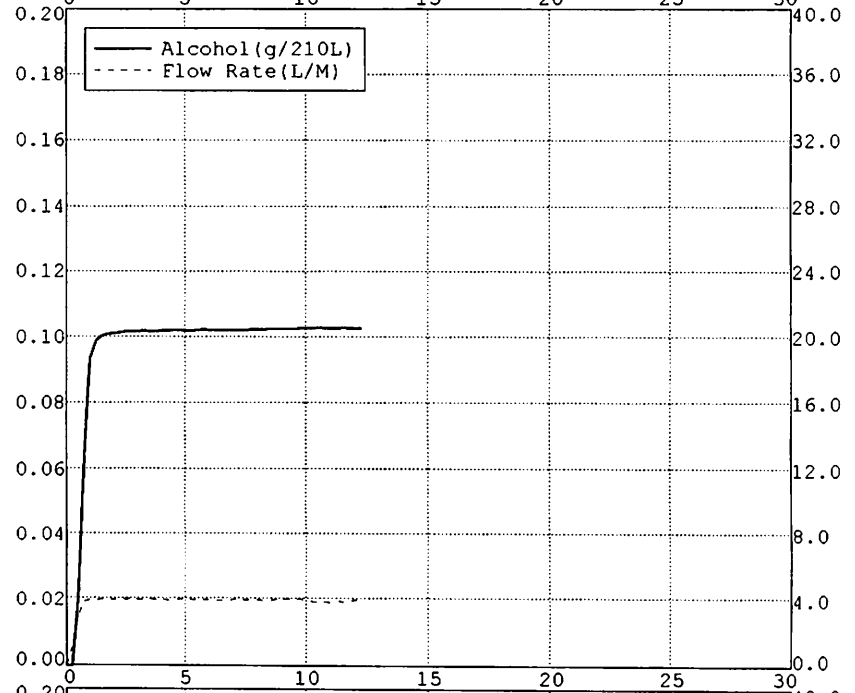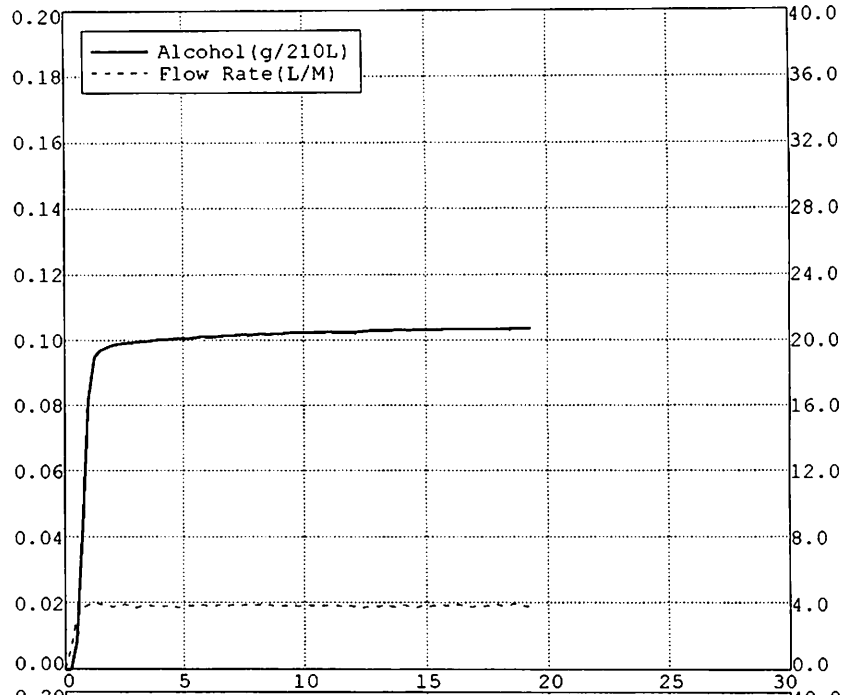

SUPERVISOR TEST

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 100197




Date: 09/18/2019

OPERATOR NAME:
MICHAEL P GIBBONS
Permit #: 45972
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:11
INTERNAL STANDARD	VERIFIED	22:11
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	22:12
BLANK TEST	0.00	22:12
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	22:13
BLANK TEST	0.00	22:14
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	22:14
BLANK TEST	0.00	22:15

WFO Weekly Test

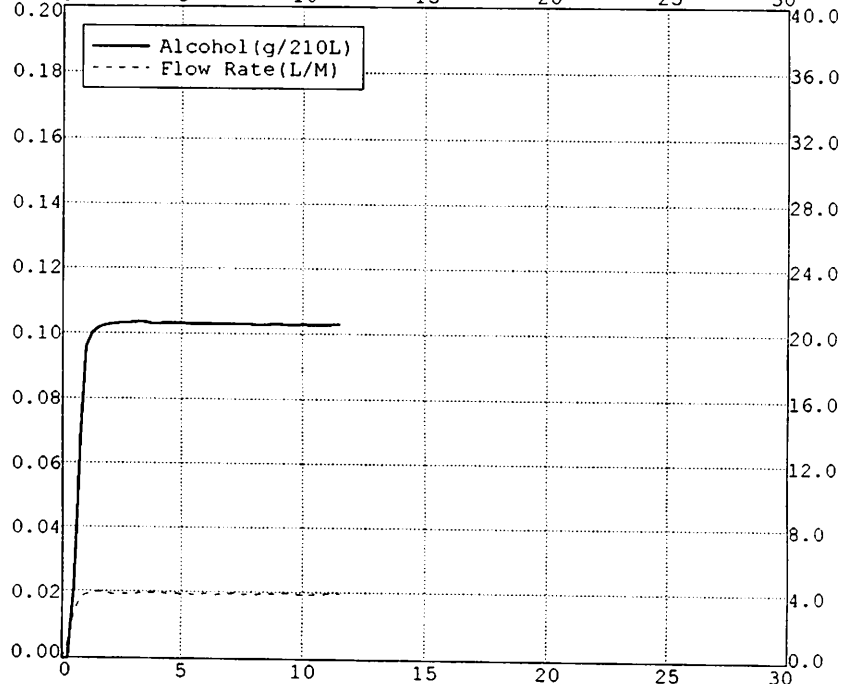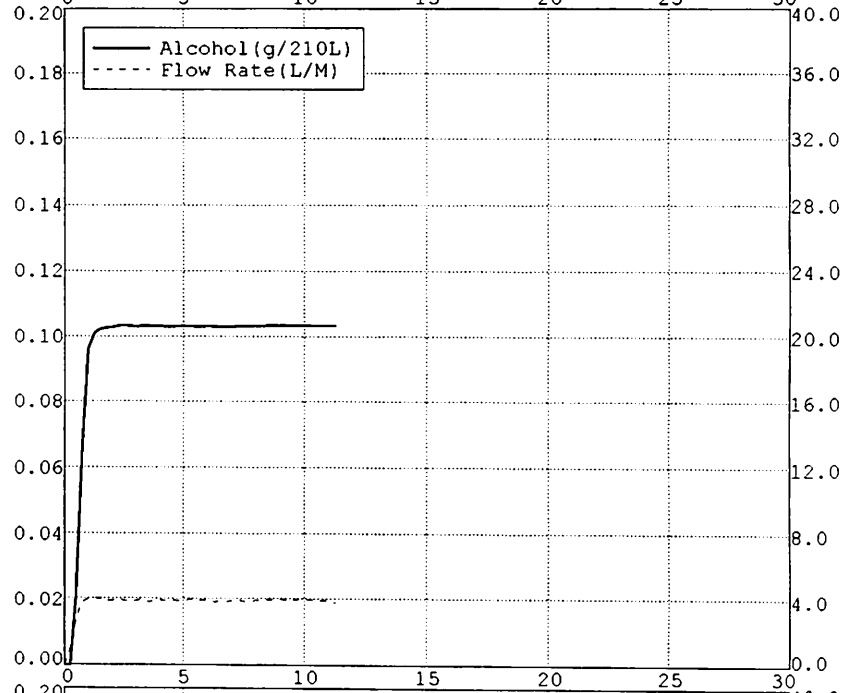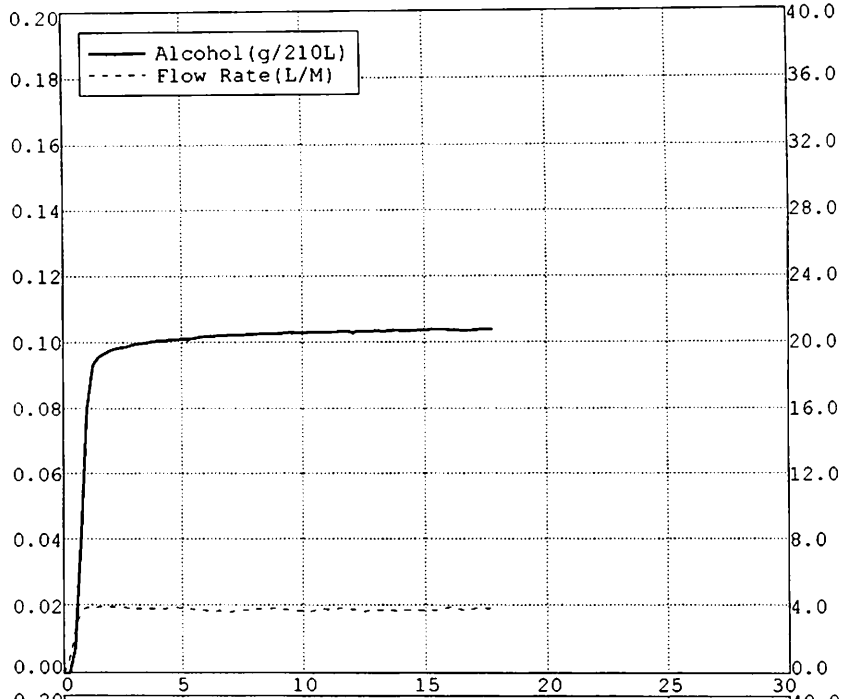

SUPERVISOR TEST

WFO



ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 100197

Date: 09/26/2019

OPERATOR NAME:
JOHN R BOWERS
Permit #: 46887
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:39
INTERNAL STANDARD	VERIFIED	02:39
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	02:40
BLANK TEST	0.00	02:41
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	02:41
BLANK TEST	0.00	02:42
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	02:42
BLANK TEST	0.00	02:43

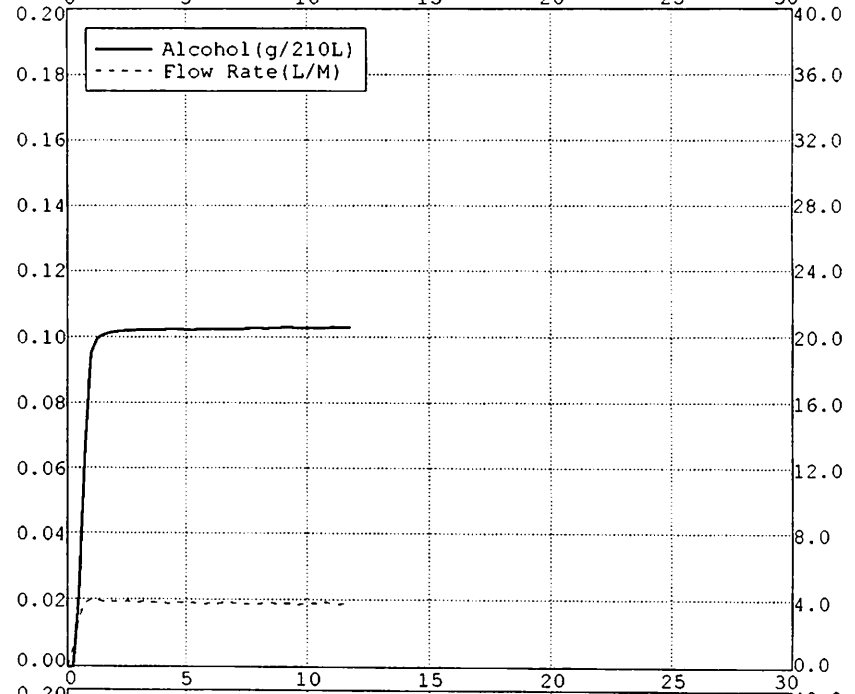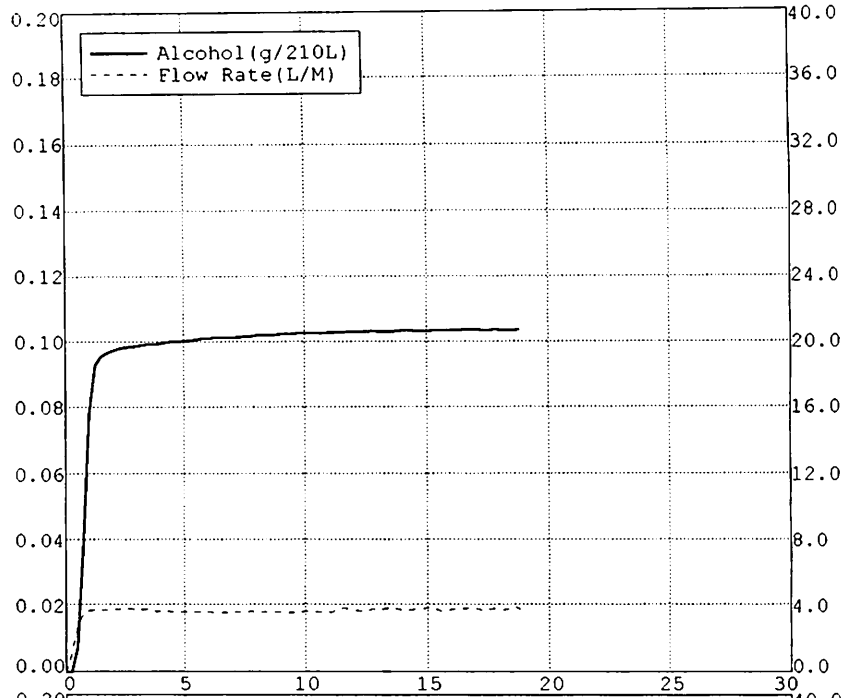

SUPERVISOR TEST

WFO

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 100197

Date: 10/16/2019

OPERATOR NAME:
BRETT A GRABELDINGER
Permit #: 46896
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:24
INTERNAL STANDARD	VERIFIED	23:24
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	23:25
BLANK TEST	0.00	23:26
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	23:26
BLANK TEST	0.00	23:27
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.10	23:28
BLANK TEST	0.00	23:28

