

SUPERVISOR TEST




ROME CITY  
POLICE DEPT  
DATAMASTER dmt: 106106

Date: 11/30/2019

OPERATOR NAME:  
HOLLIE B SILVERMAN  
Permit #: 39044  
Operator Agency/Dept: ROME CITY PD  
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:24
INTERNAL STANDARD	VERIFIED	19:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:24
BLANK TEST	0.00	19:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:26
BLANK TEST	0.00	19:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:27
BLANK TEST	0.00	19:28

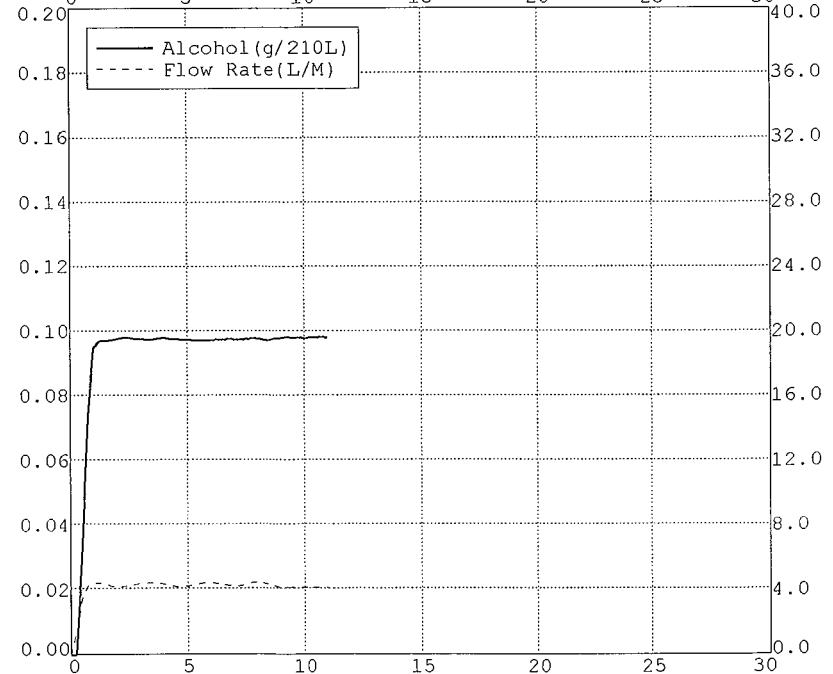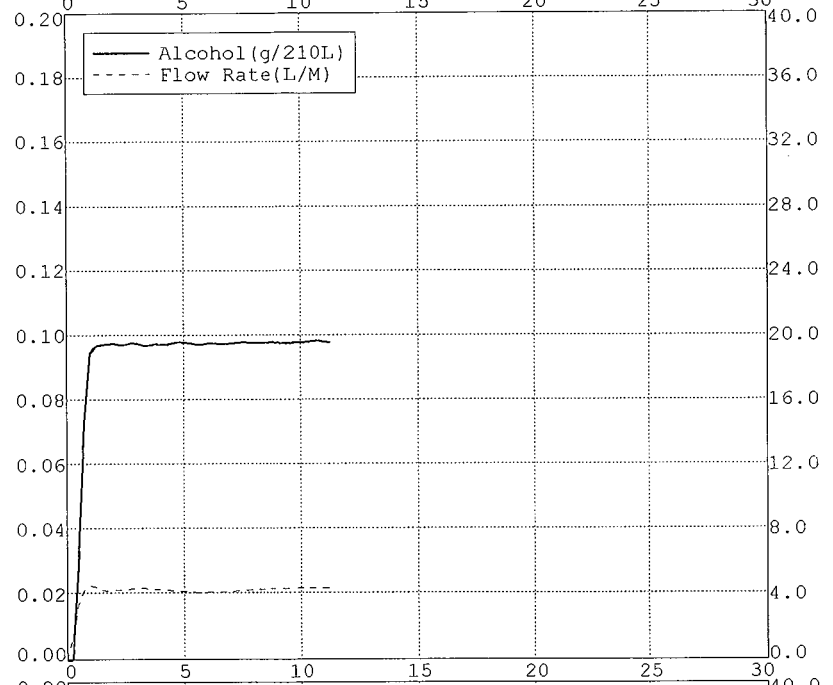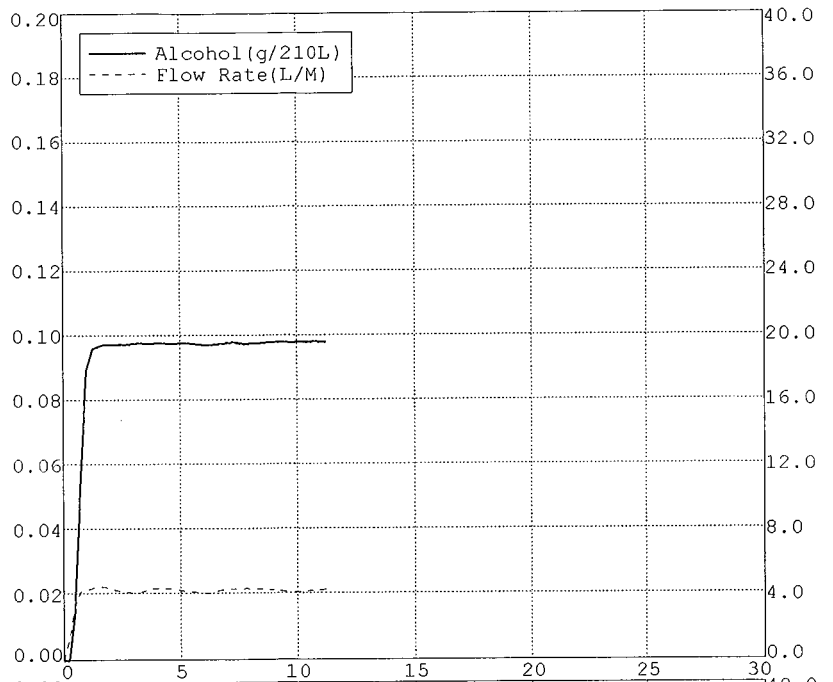

Hollie B Silverman Rome PD 11/30/19  
Hollie B Silverman 10605

SUPERVISOR TEST




ROME CITY  
POLICE DEPT  
DATAMASTER dmt: 106106

Date: 11/22/2019

OPERATOR NAME:  
HOLLIE B SILVERMAN  
Permit #: 39044  
Operator Agency/Dept: ROME CITY PD  
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:59
INTERNAL STANDARD	VERIFIED	17:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:00
BLANK TEST	0.00	18:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:01
BLANK TEST	0.00	18:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:02
BLANK TEST	0.00	18:03

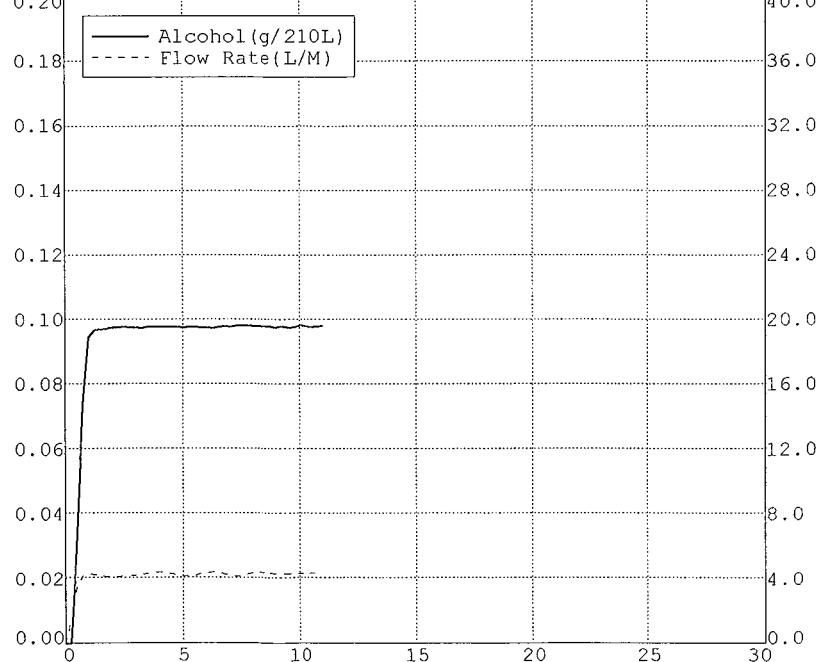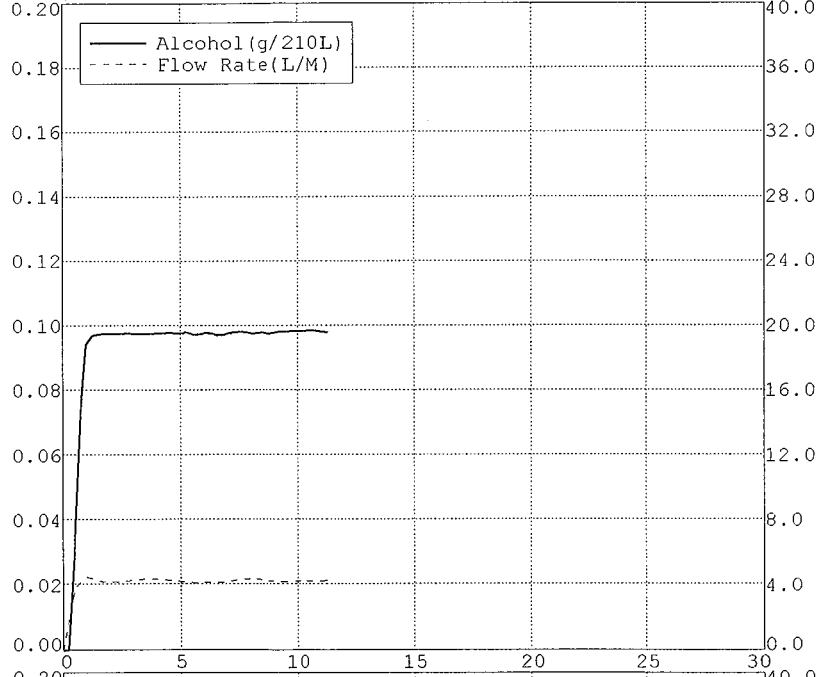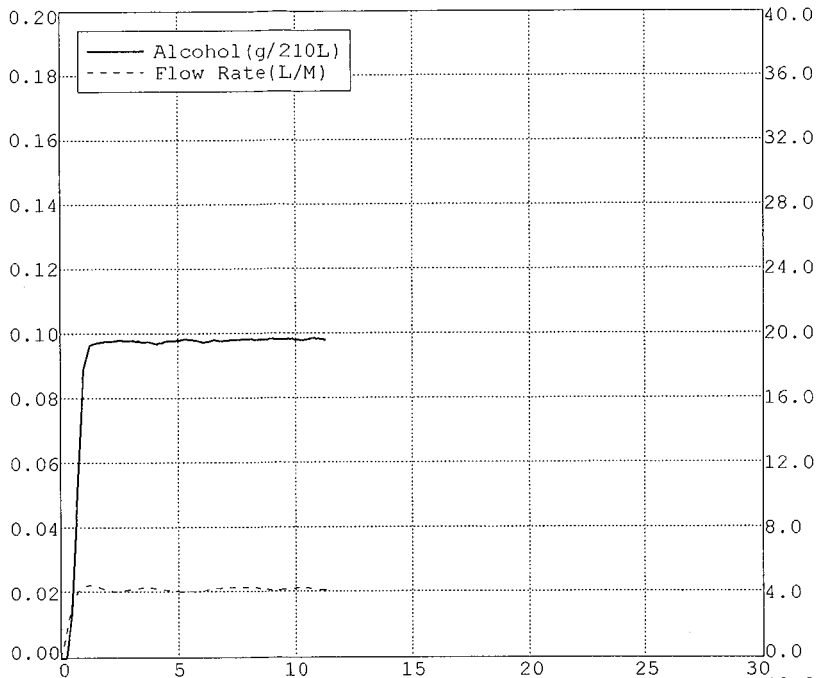

Hollie Silverman Rome PD 11/22/19  
Hollie Silverman 10:00

SUPERVISOR TEST




ROME CITY  
POLICE DEPT  
DATAMASTER dmt: 106106

Date: 11/16/2019

OPERATOR NAME:  
HOLLIE B SILVERMAN  
Permit #: 39044  
Operator Agency/Dept: ROME CITY PD  
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:24
INTERNAL STANDARD	VERIFIED	15:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:24
BLANK TEST	0.00	15:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:26
BLANK TEST	0.00	15:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:27
BLANK TEST	0.00	15:28

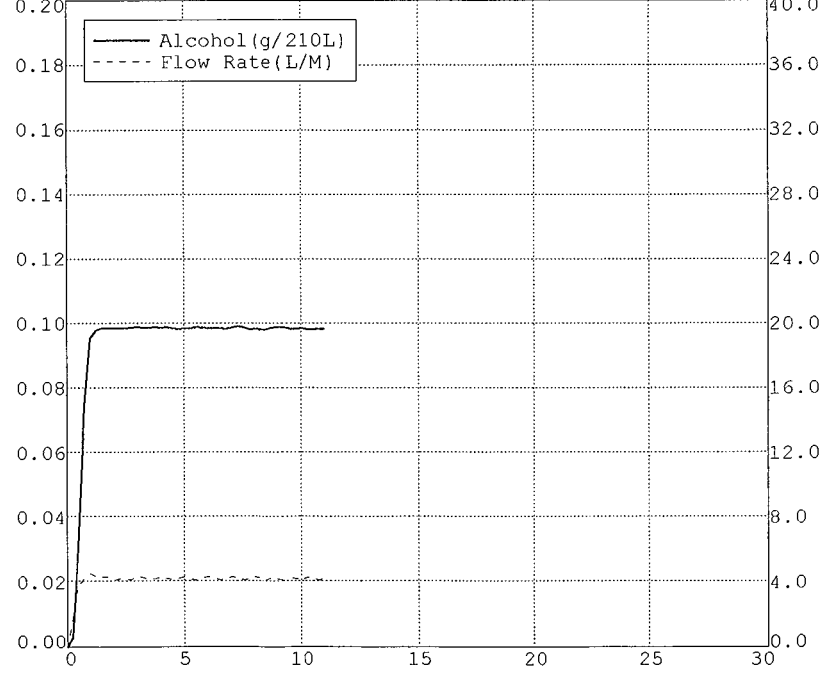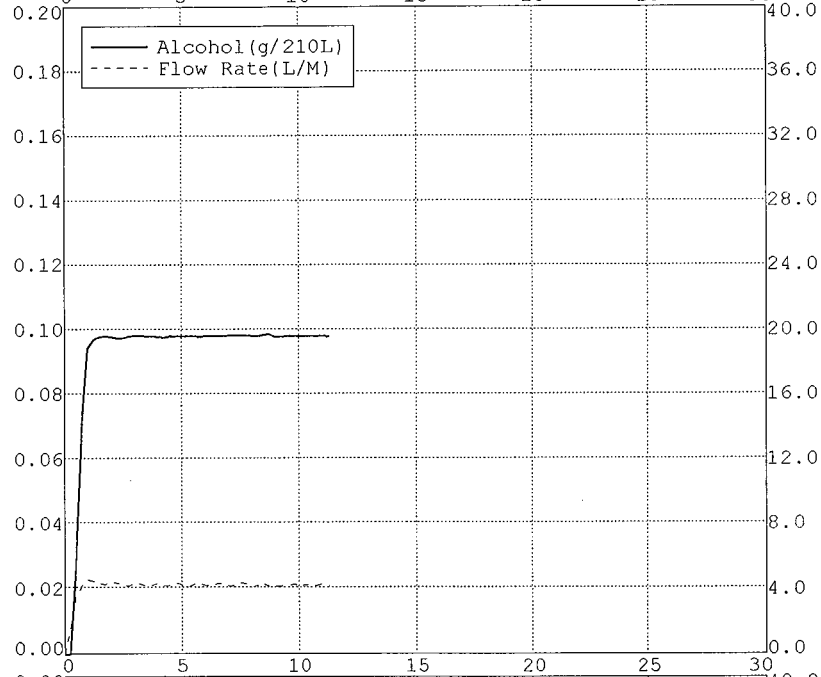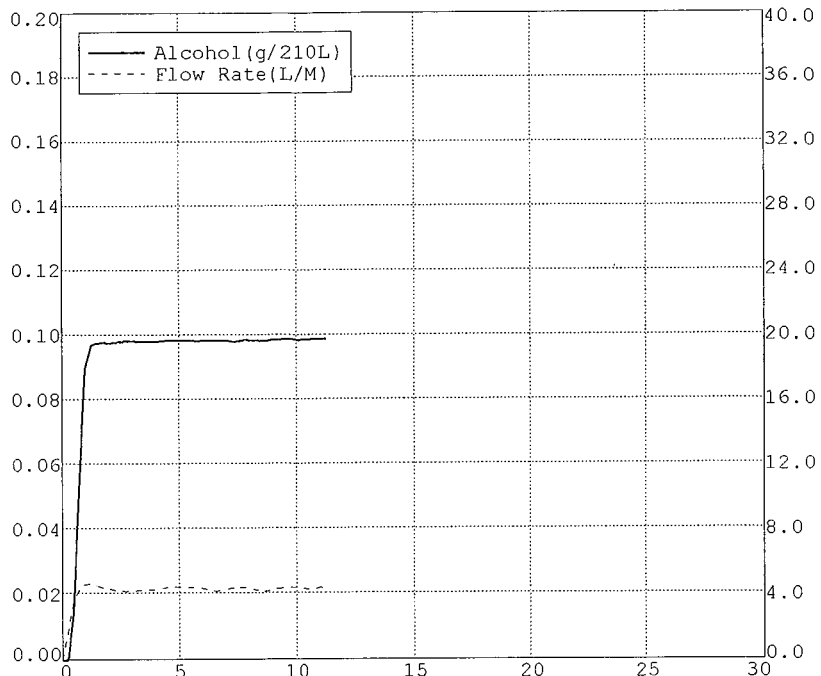

Hollie Silverman Rome PD 11/16/19  
Hollie Silverman 10805

SUPERVISOR TEST


ROME CITY  
POLICE DEPT  
DATAMASTER dmt: 106106

ate: 11/08/2019

OPERATOR NAME:  
HOLLIE B SILVERMAN  
Permit #: 39044  
Operator Agency/Dept: ROME CITY PD  
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:18
INTERNAL STANDARD	VERIFIED	15:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:19
BLANK TEST	0.00	15:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:20
BLANK TEST	0.00	15:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:21
BLANK TEST	0.00	15:22

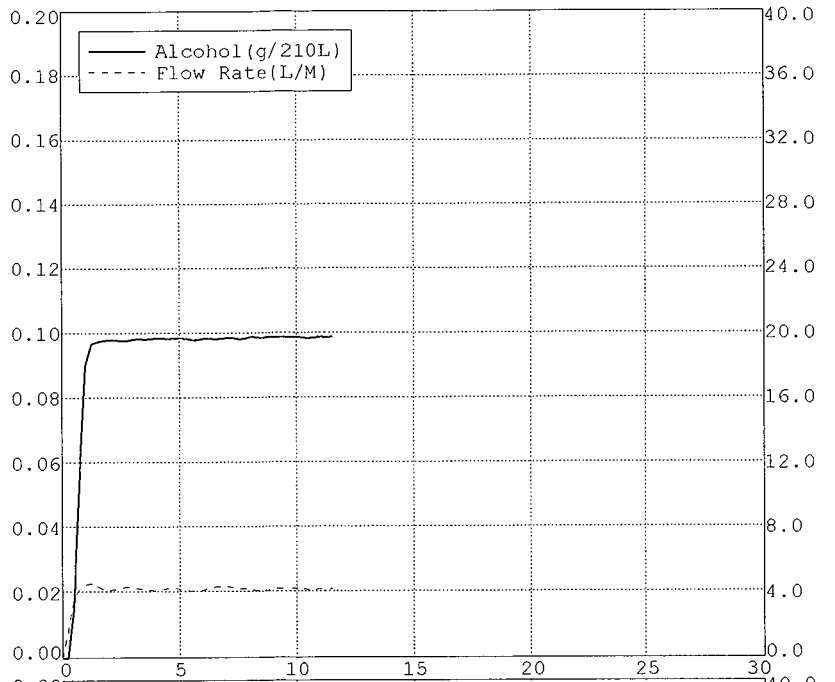

Hollie B Silverman ROME PD 11/08/19  
Hollie B Silverman 106106

SOLUTION CHANGE




ROME CITY  
POLICE DEPT  
DATAMASTER dmt: 106106

Date: 11/02/2019

OPERATOR NAME:  
HOLLIE B SILVERMAN  
Permit #: 39044  
Operator Agency/Dept: ROME CITY PD  
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:37
INTERNAL STANDARD	VERIFIED	15:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:38
BLANK TEST	0.00	15:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:39
BLANK TEST	0.00	15:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:40
BLANK TEST	0.00	15:41

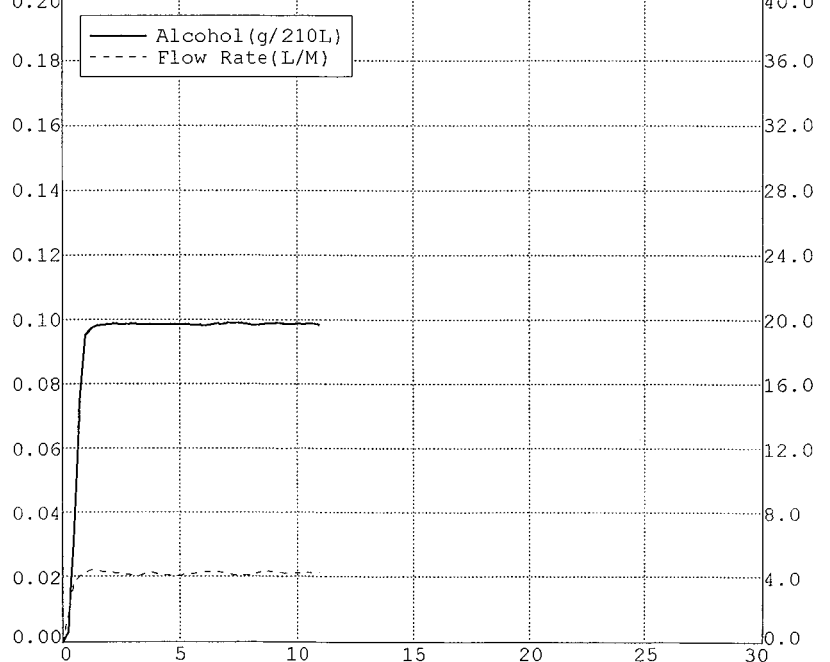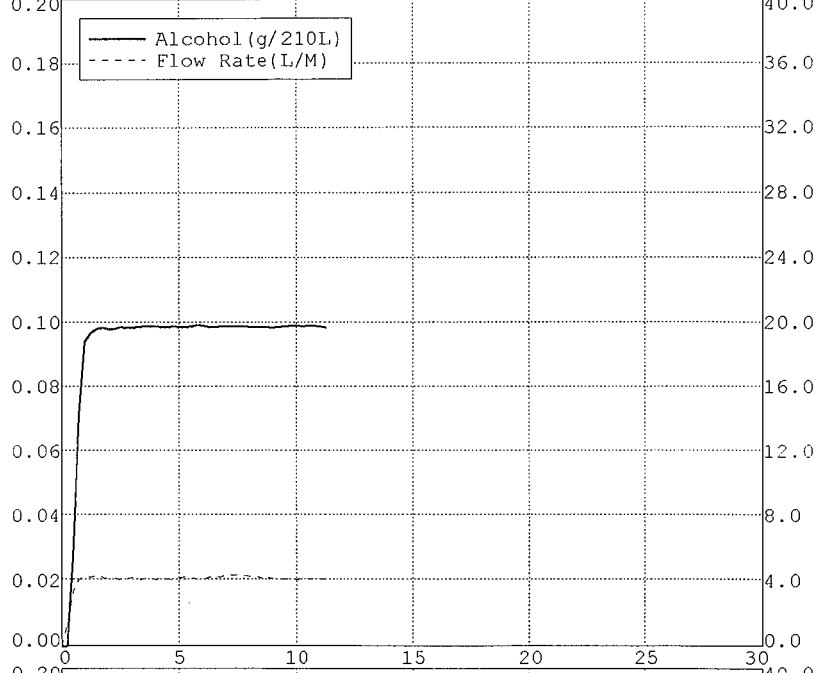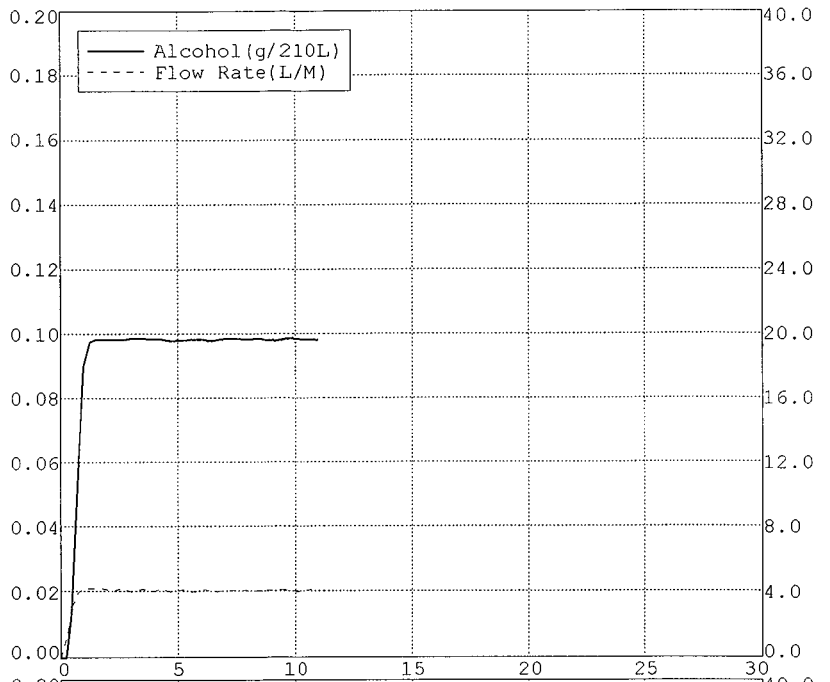

*Hollie Silverman Rome PD 11/02/19*  
*Hollie Silverman 10905*