

SOLUTION CHANGE




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 03/01/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:42
INTERNAL STANDARD	VERIFIED	16:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:42
BLANK TEST	0.00	16:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:44
BLANK TEST	0.00	16:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:45
BLANK TEST	0.00	16:46

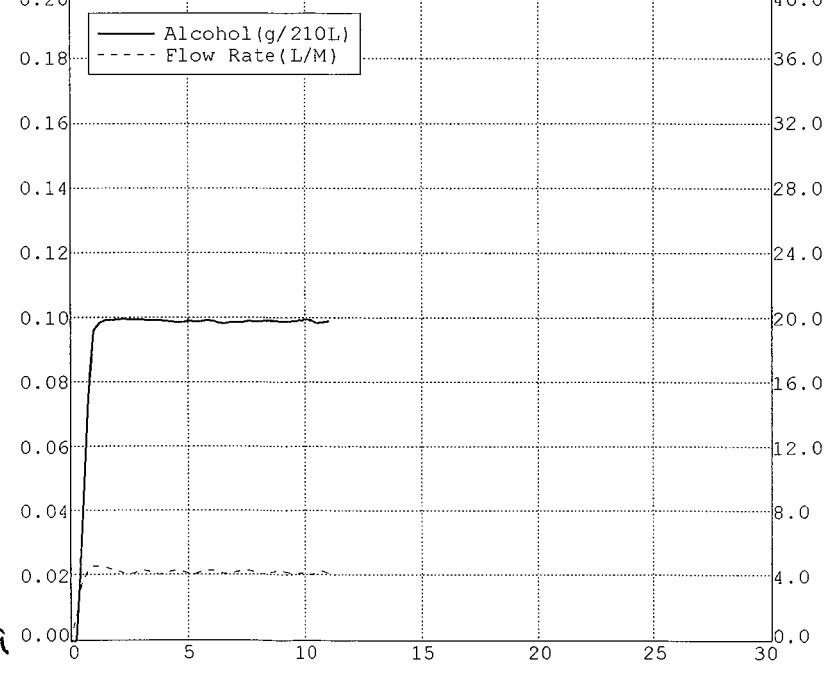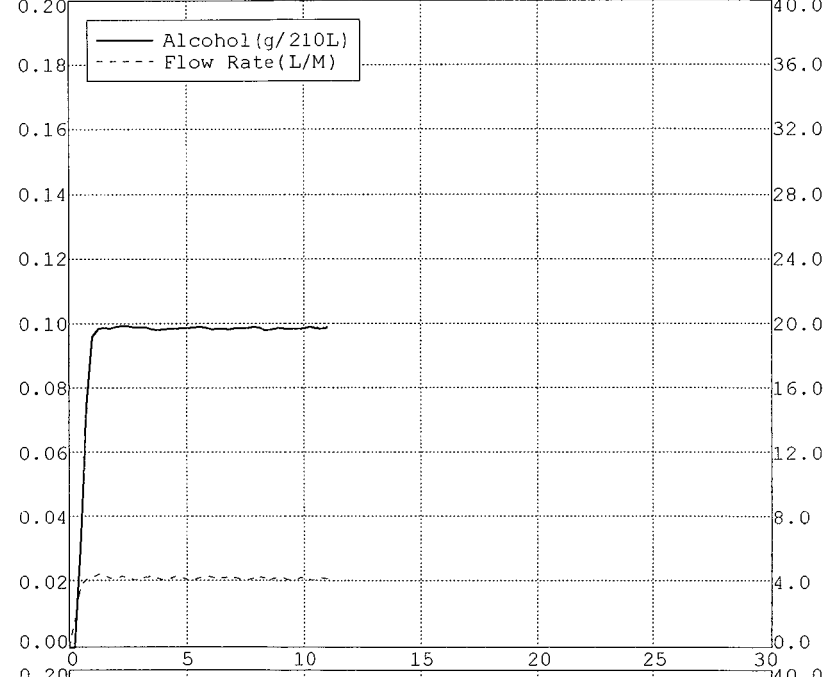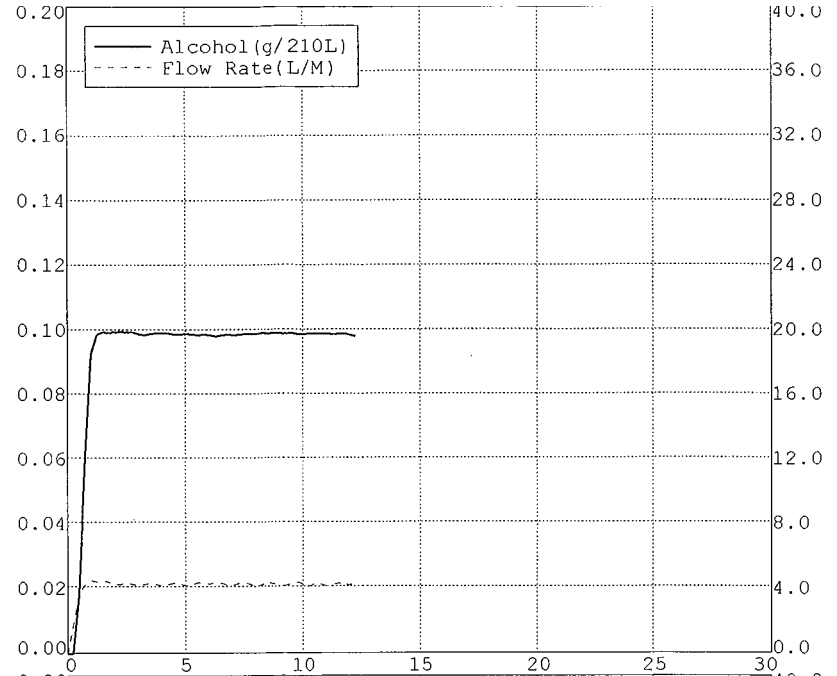

Hollie Kennedy Rome PD 03/01/19
Hollie Kennedy

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 03/08/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:57
INTERNAL STANDARD	VERIFIED	21:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:57
BLANK TEST	0.00	21:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:58
BLANK TEST	0.00	21:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	22:00
BLANK TEST	0.00	22:01

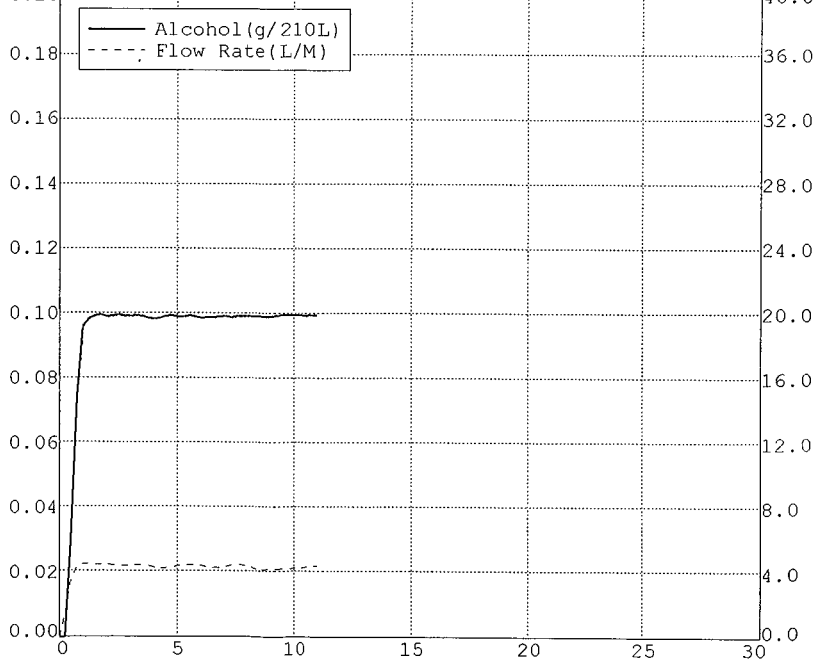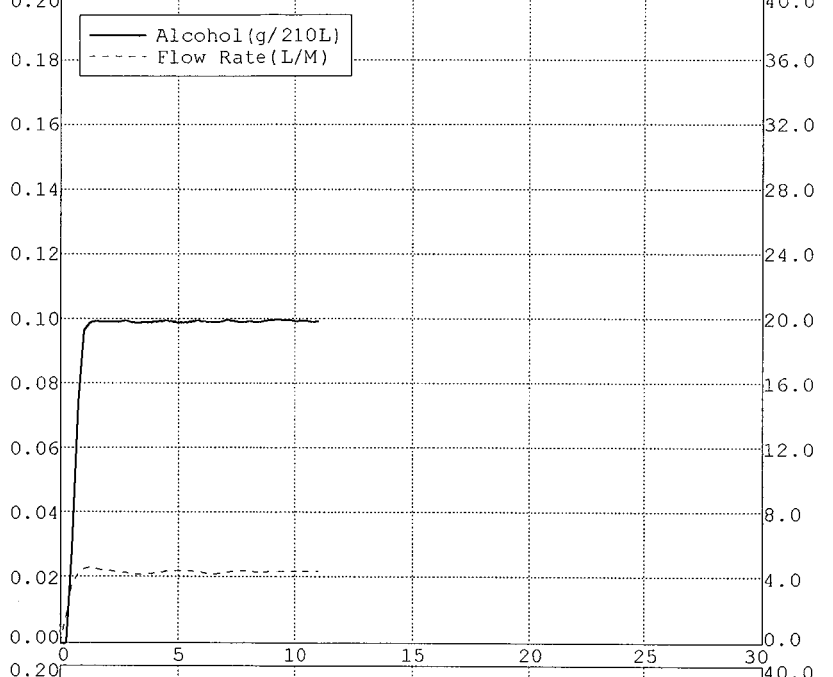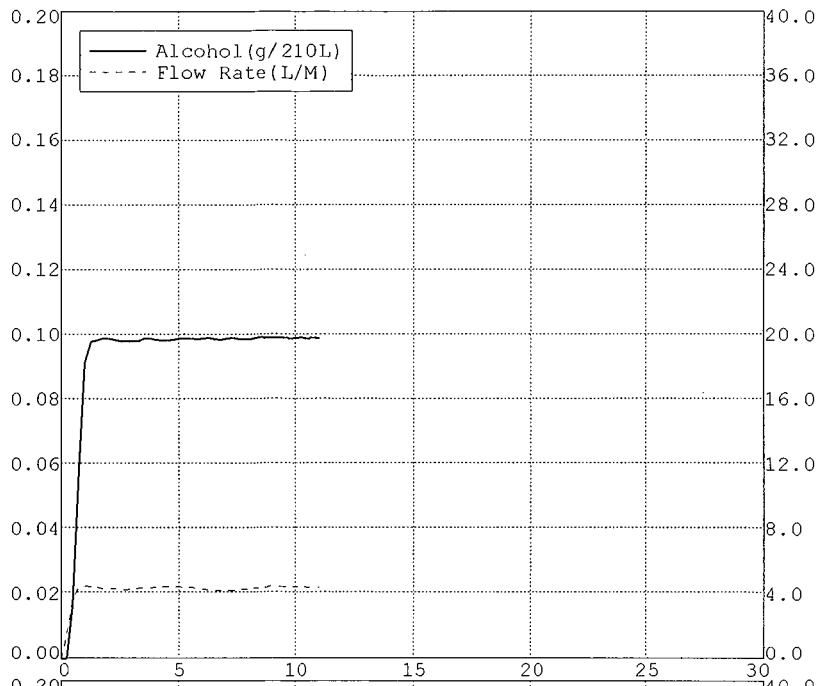

Hollie B Kennedy Rome PD 03/08/19
Hollie B Kennedy

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 03/15/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:08
INTERNAL STANDARD	VERIFIED	22:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:09
BLANK TEST	0.00	22:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	22:10
BLANK TEST	0.00	22:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	22:11
BLANK TEST	0.00	22:12

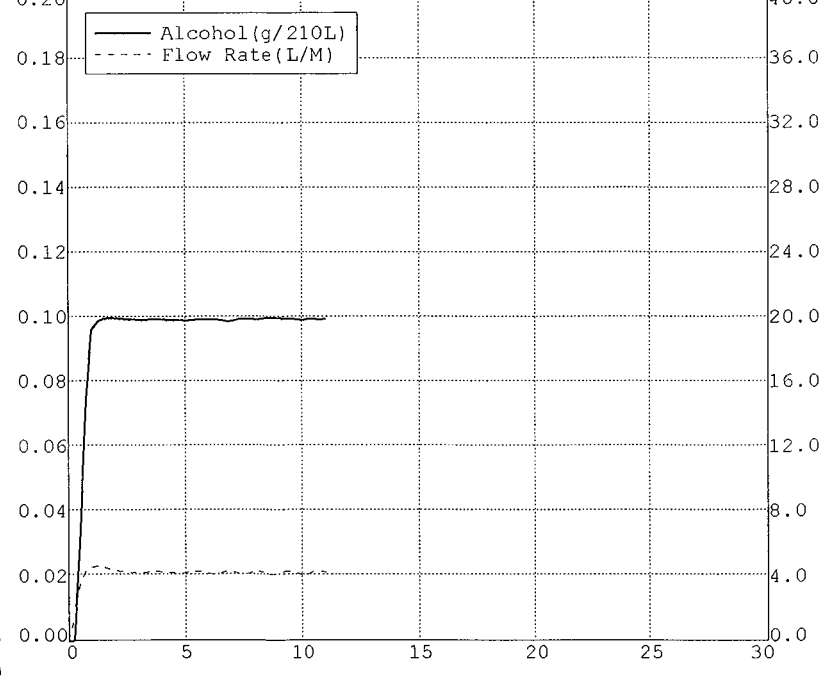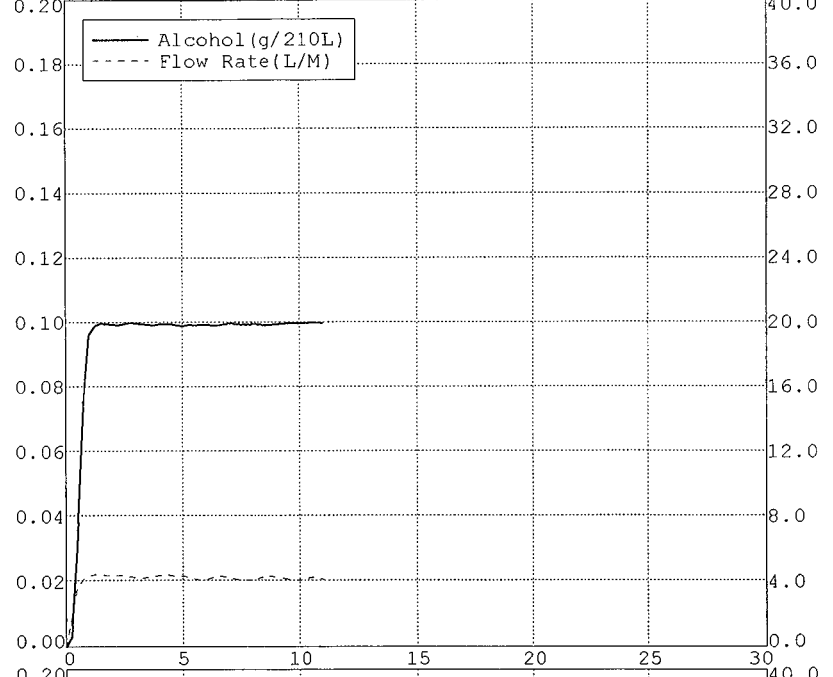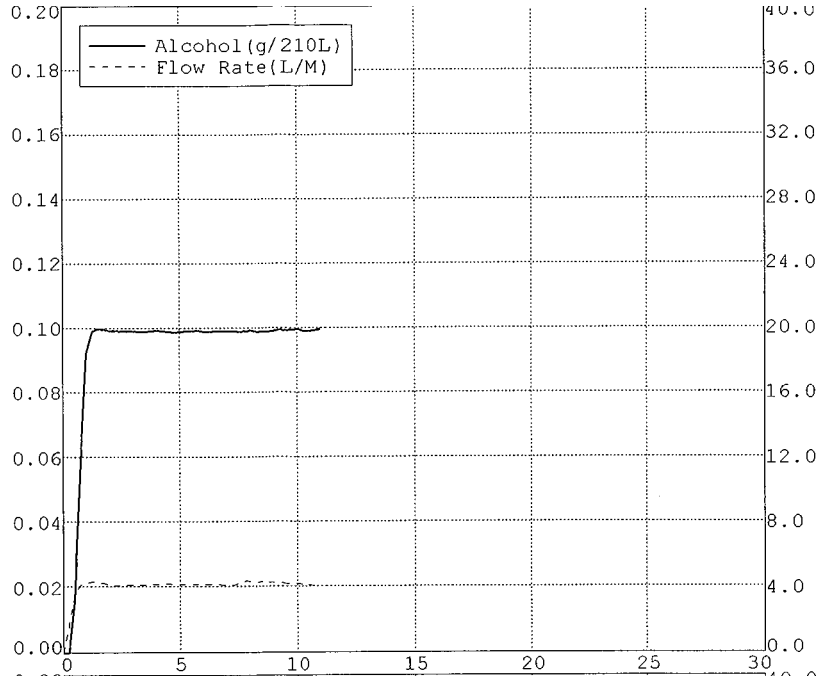

Hollie Kennedy Rome PD 03/15/19
1/29/19

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 03/25/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:24
INTERNAL STANDARD	VERIFIED	14:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:24
BLANK TEST	0.00	14:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:25
BLANK TEST	0.00	14:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:26
BLANK TEST	0.00	14:27

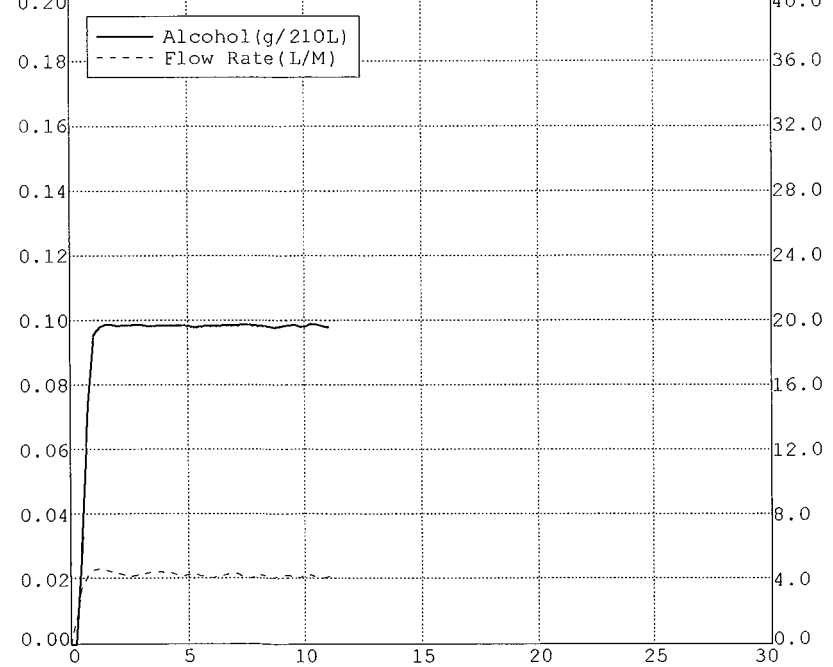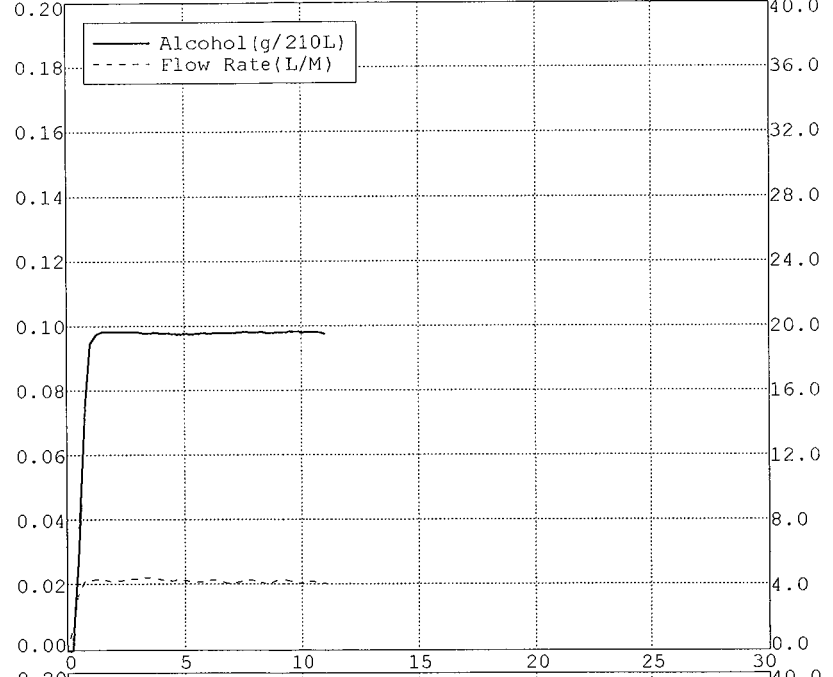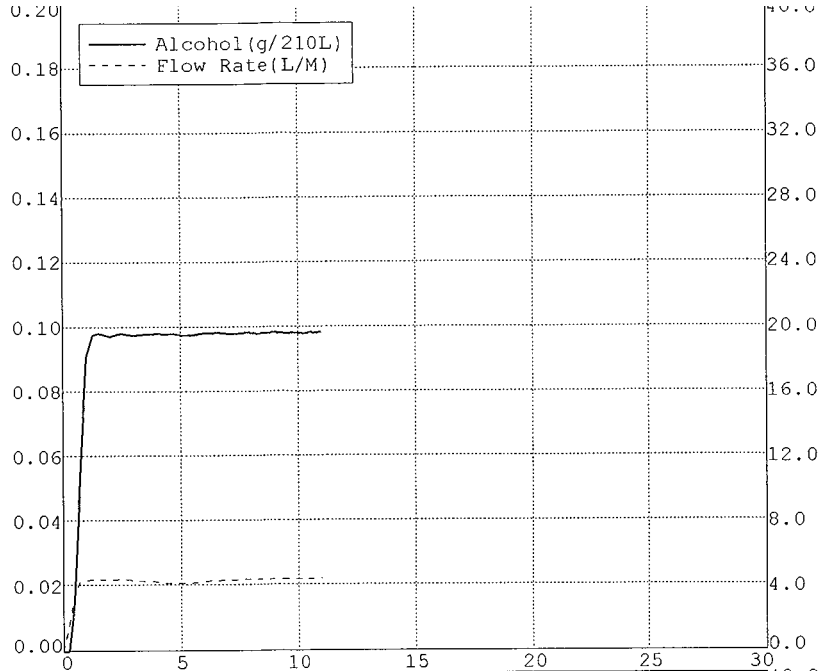

Hollie Kennedy 03/25/19
Steve [unclear] 10:05

SUPERVISOR TEST




ROME CITY
POLICE DEPT
DATAMASTER dmt: 106106

Date: 03/29/2019

OPERATOR NAME:
HOLLIE B KENNEDY
Permit #: 39044
Operator Agency/Dept: ROME CITY PD
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:08
INTERNAL STANDARD	VERIFIED	18:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:09
BLANK TEST	0.00	18:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:10
BLANK TEST	0.00	18:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:11
BLANK TEST	0.00	18:12

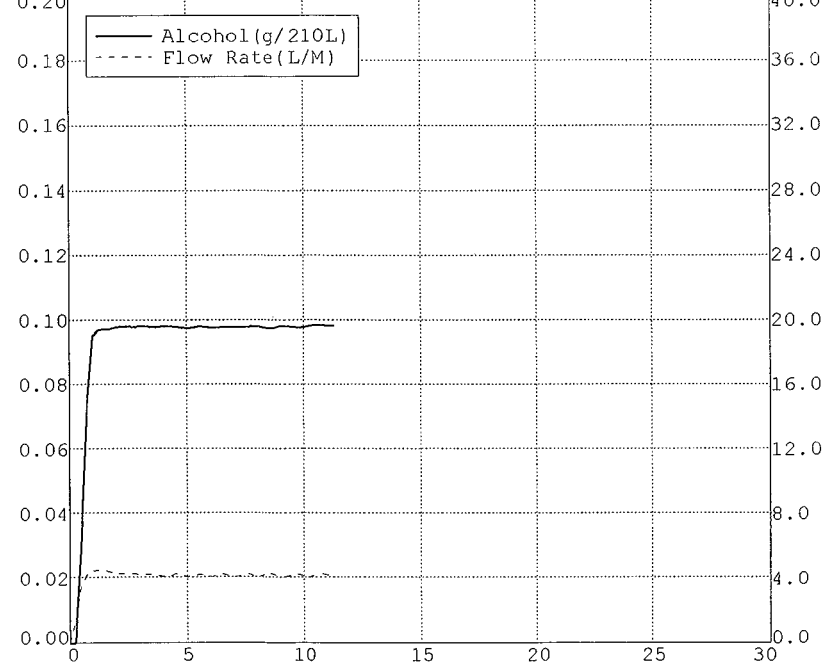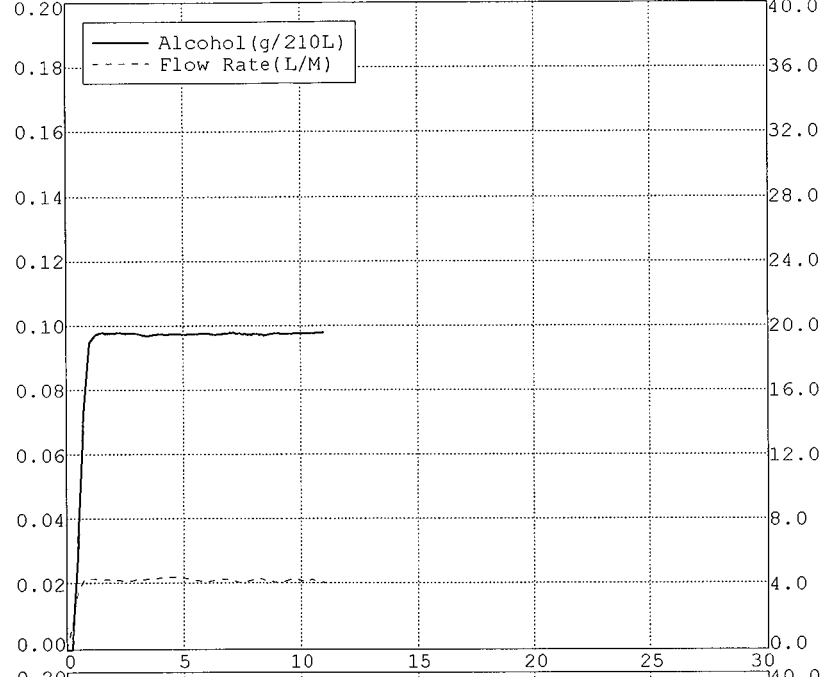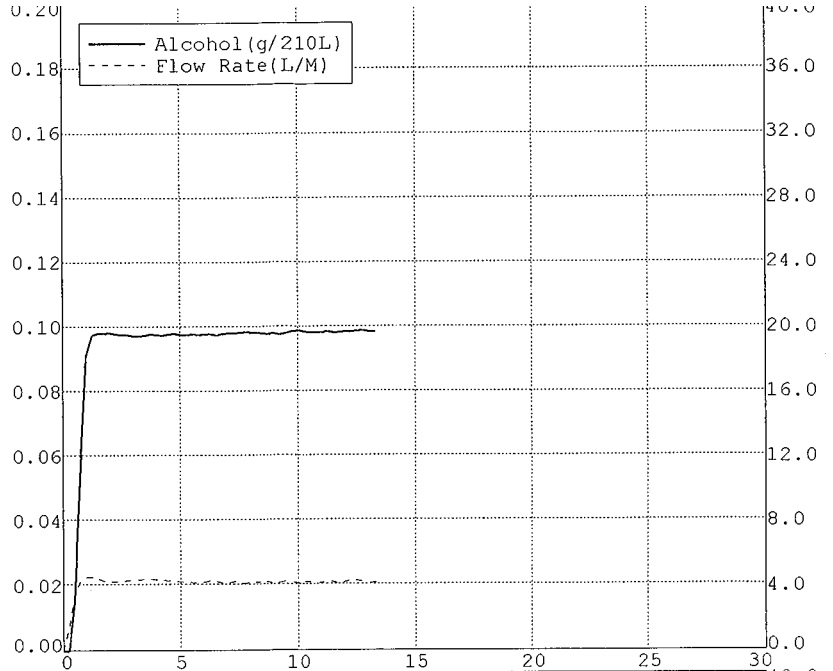

Hollie Kennedy *Rome PD* *03/29/19*
Paul Wiley *10605*