

SUPERVISOR TEST




UTICA CITY  
POLICE DEPT  
DATAMASTER dmt: 107308

Date: 12/10/2019

OPERATOR NAME: *RMS*  
MICHAEL J CLIVE  
Permit #: 36682  
Operator Agency/Dept: UTICA CITY PD  
Reference Standard #: 19250  
*19-46759*

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:47
INTERNAL STANDARD	VERIFIED	12:47
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:48
BLANK TEST	0.00	12:49
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:49
BLANK TEST	0.00	12:50
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:50
BLANK TEST	0.00	12:51

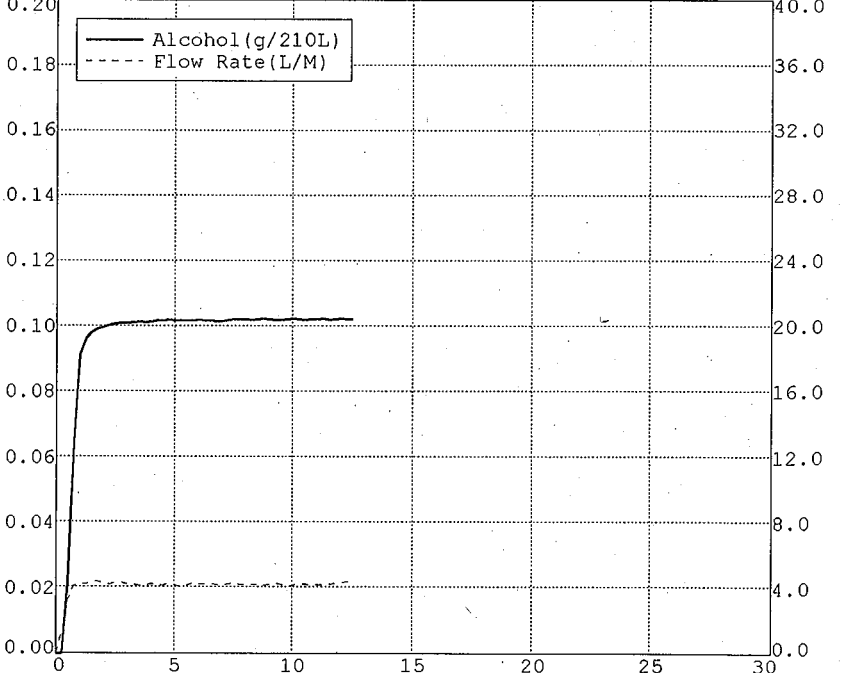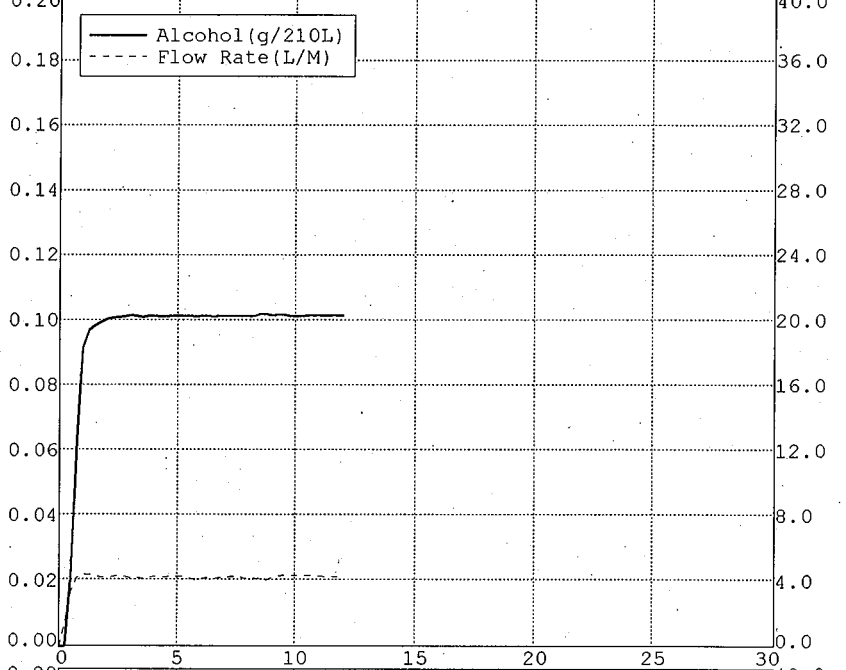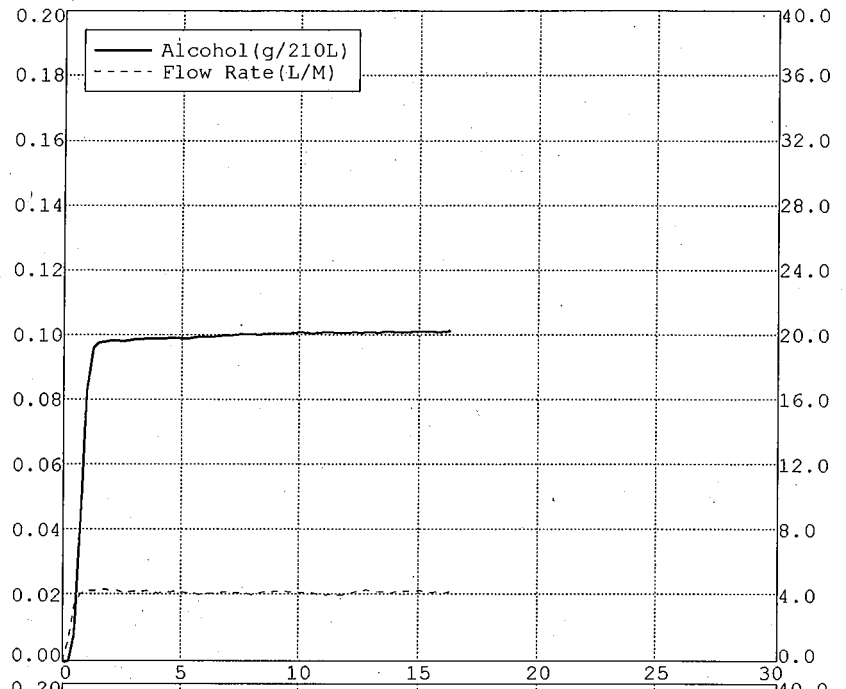

SUPERVISOR TEST

UTICA CITY  
 POLICE DEPT  
 DATAMASTER dmt: 100282

Date: 12/10/2019

*RMS  
 19-46759*

OPERATOR NAME:  
 MICHAEL J CLIVE  
 Permit #: 366682  
 Operator Agency/Dept: UTICA CITY PD  
 Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:09
INTERNAL STANDARD	VERIFIED	12:09
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	12:10
BLANK TEST	0.00	12:10
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	12:11
BLANK TEST	0.00	12:12
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	12:12
BLANK TEST	0.00	12:13

