

SUPERVISOR TEST

UTICA CITY
 POLICE DEPT
 DATAMASTER dmt: 107308




Date: 02/04/2020

RM
20-3893

OPERATOR NAME:
 MICHAEL J CLIVE
 Permit #: 36682
 Operator Agency/Dept: UTICA CITY PD
 Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:57
INTERNAL STANDARD	VERIFIED	12:57
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:57
BLANK TEST	0.00	12:58
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:58
BLANK TEST	0.00	12:59
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:59
BLANK TEST	0.00	13:00

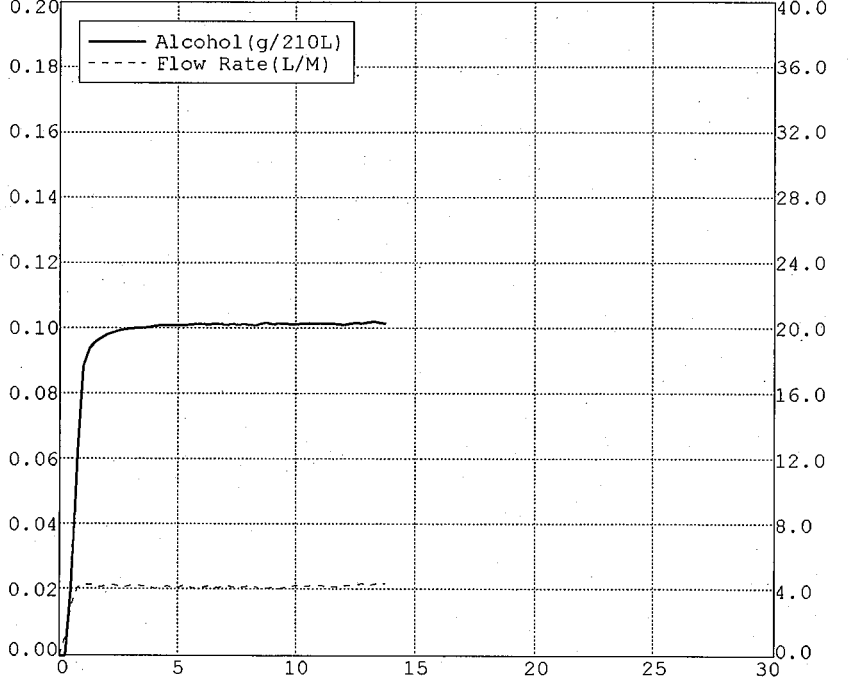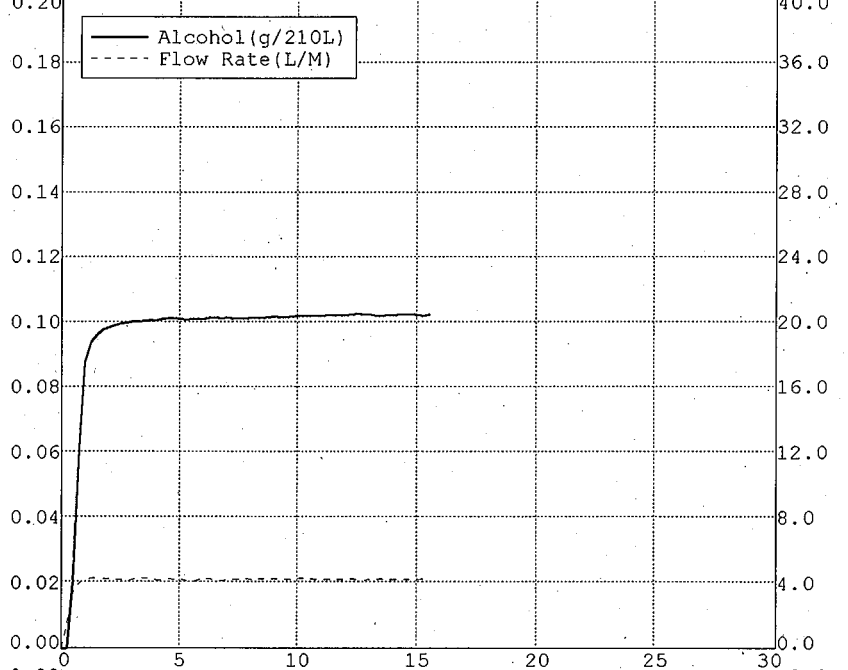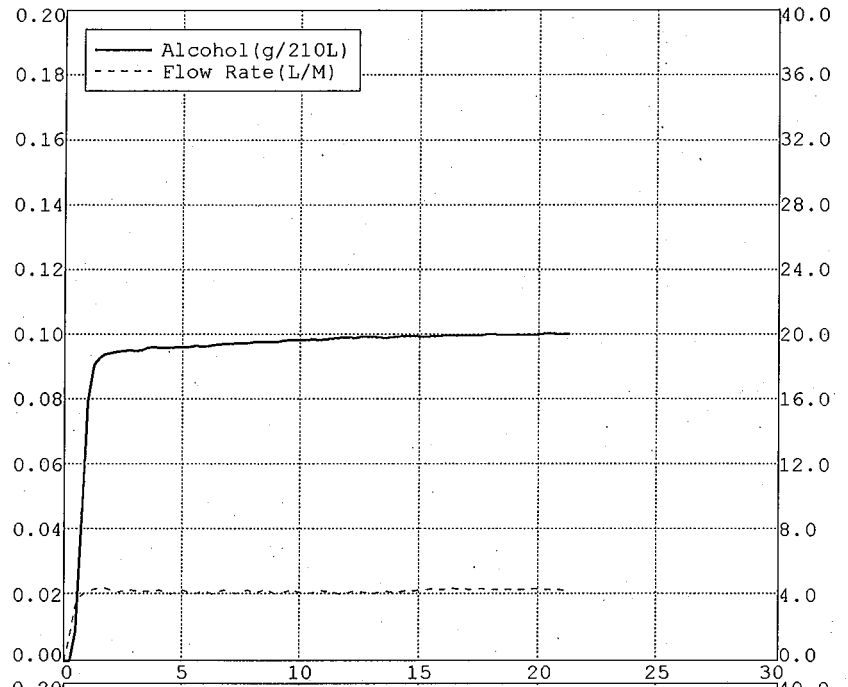

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282

Date: 02/04/2020

Rm
20-3893

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:56
INTERNAL STANDARD	VERIFIED	12:56
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	12:56
BLANK TEST	0.00	12:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:57
BLANK TEST	0.00	12:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:58
BLANK TEST	0.00	12:59

