

SUPERVISOR TEST




UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308

Date: 04/21/2020

OPERATOR NAME: *Rm*
MICHAEL J CLIVE *20-13044*
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:46
INTERNAL STANDARD	VERIFIED	10:46
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:47
BLANK TEST	0.00	10:47
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:48
BLANK TEST	0.00	10:49
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	10:49
BLANK TEST	0.00	10:50

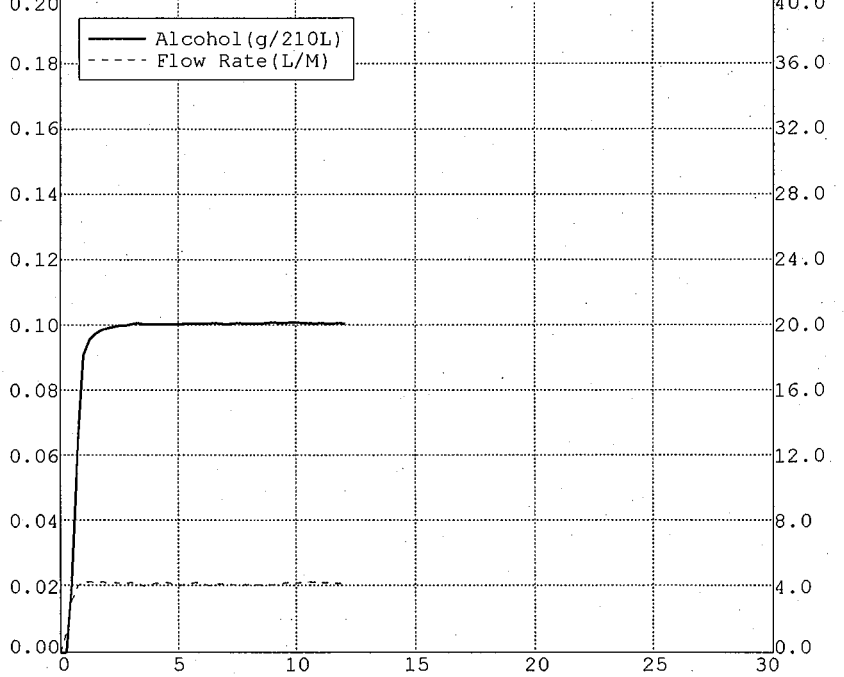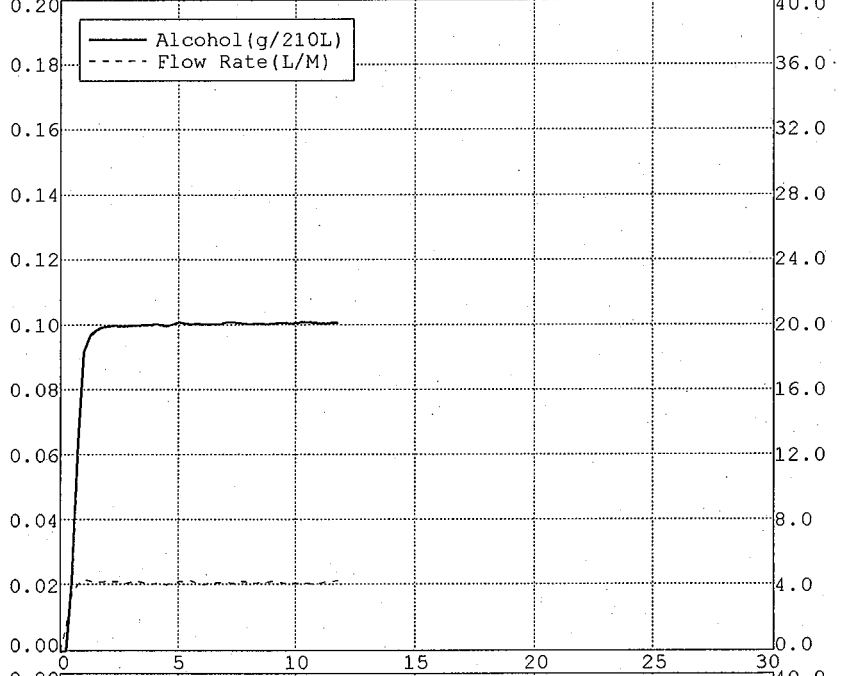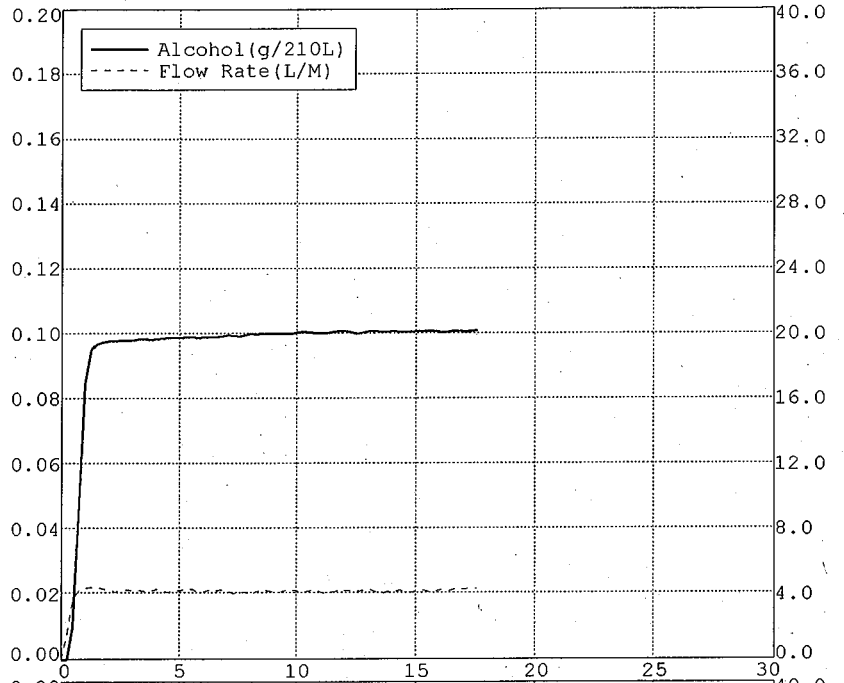

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282

Date: 04/21/2020

RMJ
20-13044

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:20
INTERNAL STANDARD	VERIFIED	10:20
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	10:20
BLANK TEST	0.00	10:21
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	10:22
BLANK TEST	0.00	10:22
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	10:23
BLANK TEST	0.00	10:24

