

SUPERVISOR TEST

UTICA CITY  
 POLICE DEPT  
 DATAMASTER dmt: 107308




Date: 04/07/2020

*Rem  
 20-11416*

OPERATOR NAME:  
 MICHAEL J CLIVE  
 Permit #: 36682  
 Operator Agency/Dept: UTICA CITY PD  
 Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:45
INTERNAL STANDARD	VERIFIED	11:45
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:45
BLANK TEST	0.00	11:46
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:46
BLANK TEST	0.00	11:47
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:47
BLANK TEST	0.00	11:48

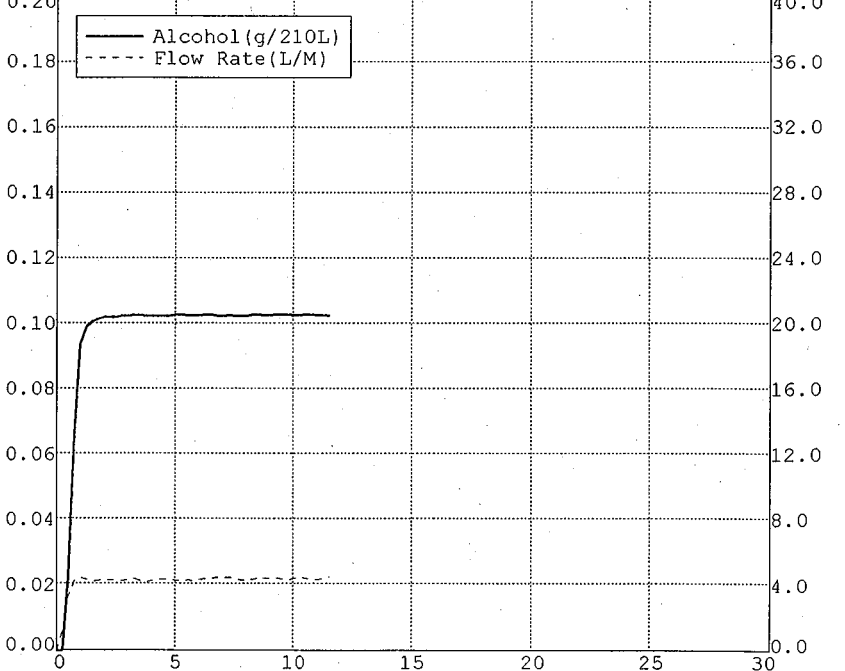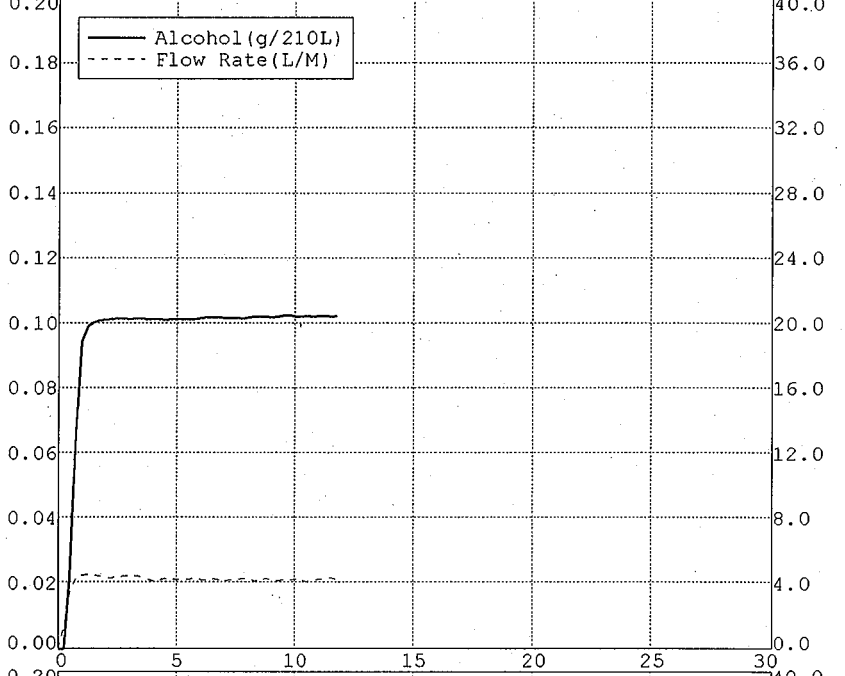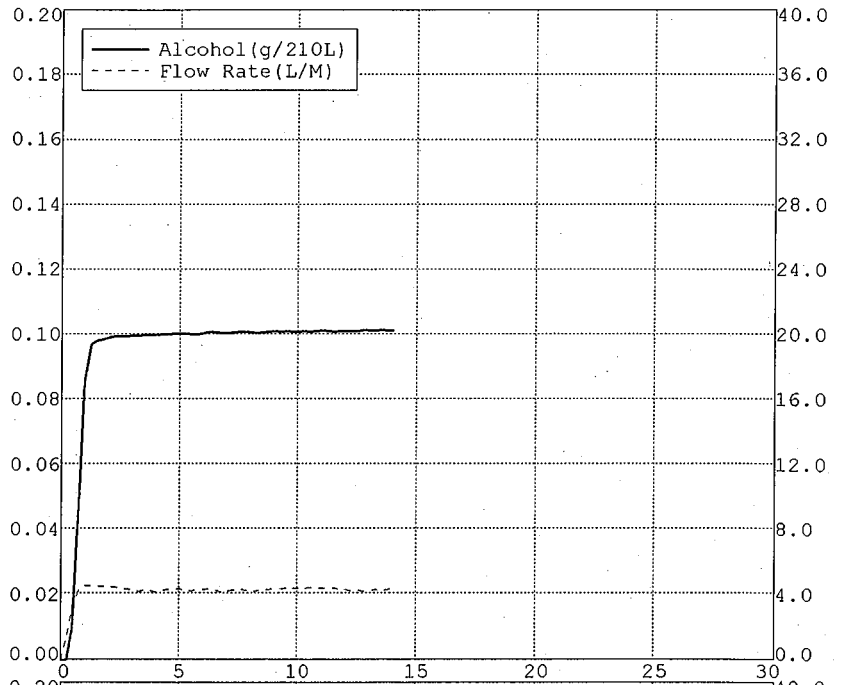

SUPERVISOR TEST

UTICA CITY  
POLICE DEPT  
DATAMASTER dmt: 100282

Date: 04/07/2020

*RM*  
*20-11416*

OPERATOR NAME:  
MICHAEL J CLIVE  
Permit #: 36682  
Operator Agency/Dept: UTICA CITY PD  
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:37
INTERNAL STANDARD	VERIFIED	10:37
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	10:37
BLANK TEST	0.00	10:38
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	10:38
BLANK TEST	0.00	10:39
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	10:39
BLANK TEST	0.00	10:40

