

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308




Date: 05/12/2020

RM7
20-151/03

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:16
INTERNAL STANDARD	VERIFIED	10:16
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:17
BLANK TEST	0.00	10:18
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:18
BLANK TEST	0.00	10:19
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:19
BLANK TEST	0.00	10:20

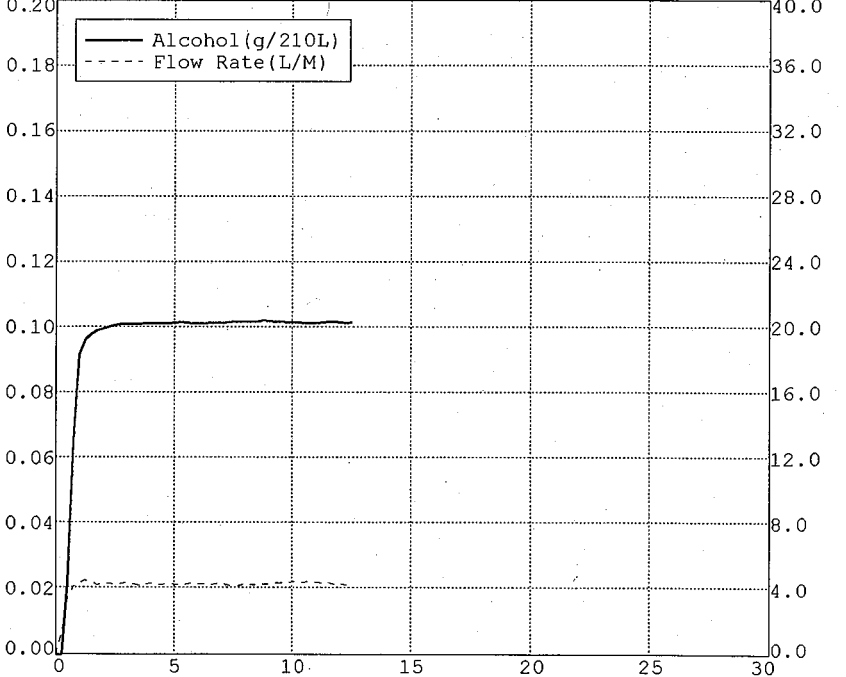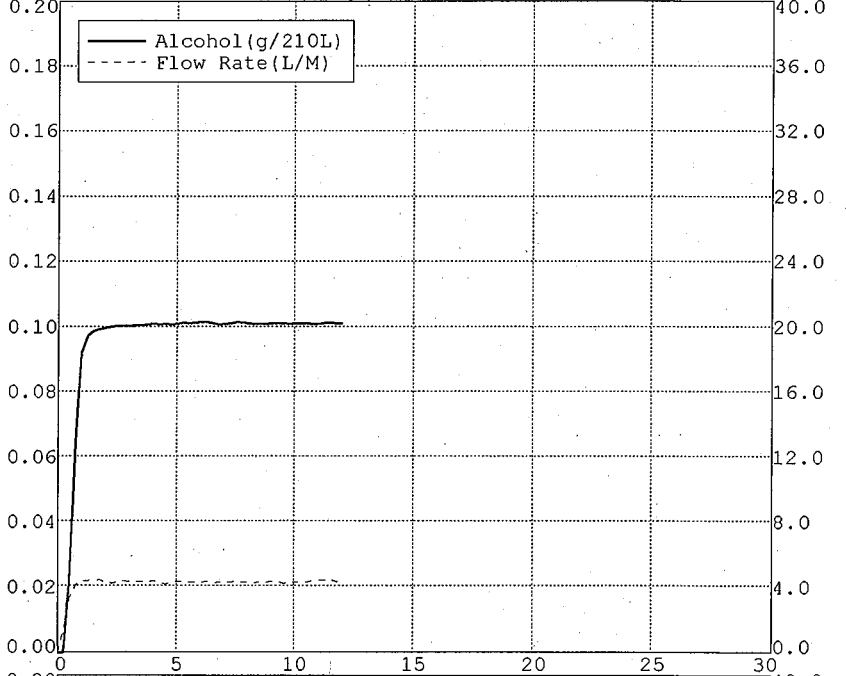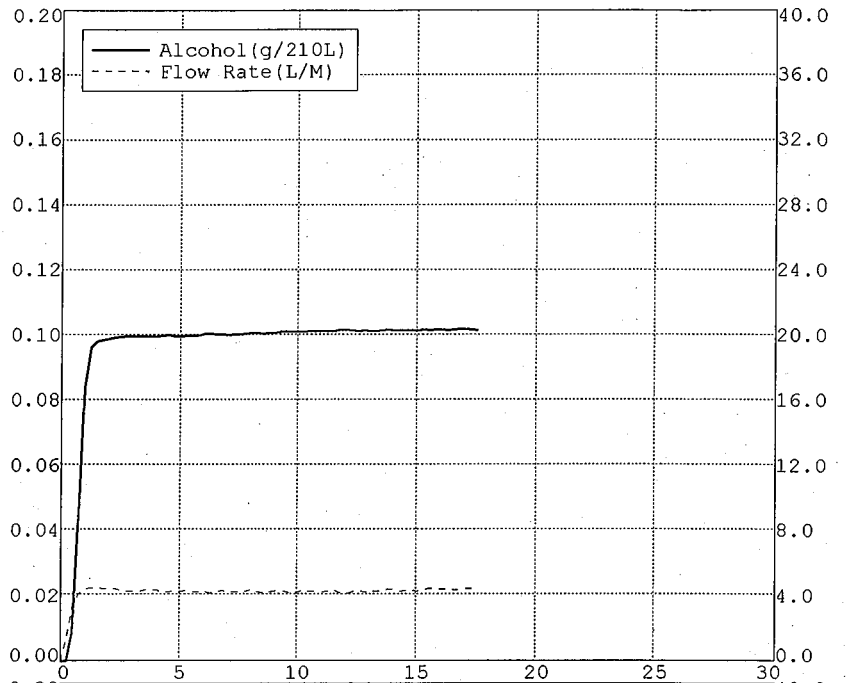

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282

Date: 05/12/2020

*RMS
20-154/03*

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:44
INTERNAL STANDARD	VERIFIED	09:44
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	09:44
BLANK TEST	0.00	09:45
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	09:45
BLANK TEST	0.00	09:46
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	09:46
BLANK TEST	0.00	09:47

